

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020819\
 Data File : FB019672.D
 Signal(s) : FID2B.CH
 Acq On : 8 Feb 2019 14:35
 Operator : MJ/SJ
 Sample : K1349-03
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Feb 08 23:09:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.045	218658	18.705 ng/ml
Target Compounds			
6) t Toluene	10.893	29630	1.694 ng/ml
8) t m-Xylene	13.479	19146	0.837 ng/ml
9) t O-Xylene	14.206	10321	0.462 ng/ml
10) t 1,2,4-Trimethylbenzene	16.494	23932	1.033 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020819\
Data File : FB019672.D
Signal(s) : FID2B.CH
Acq On : 8 Feb 2019 14:35
Operator : MJ/SJ
Sample : K1349-03
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 08 23:09:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

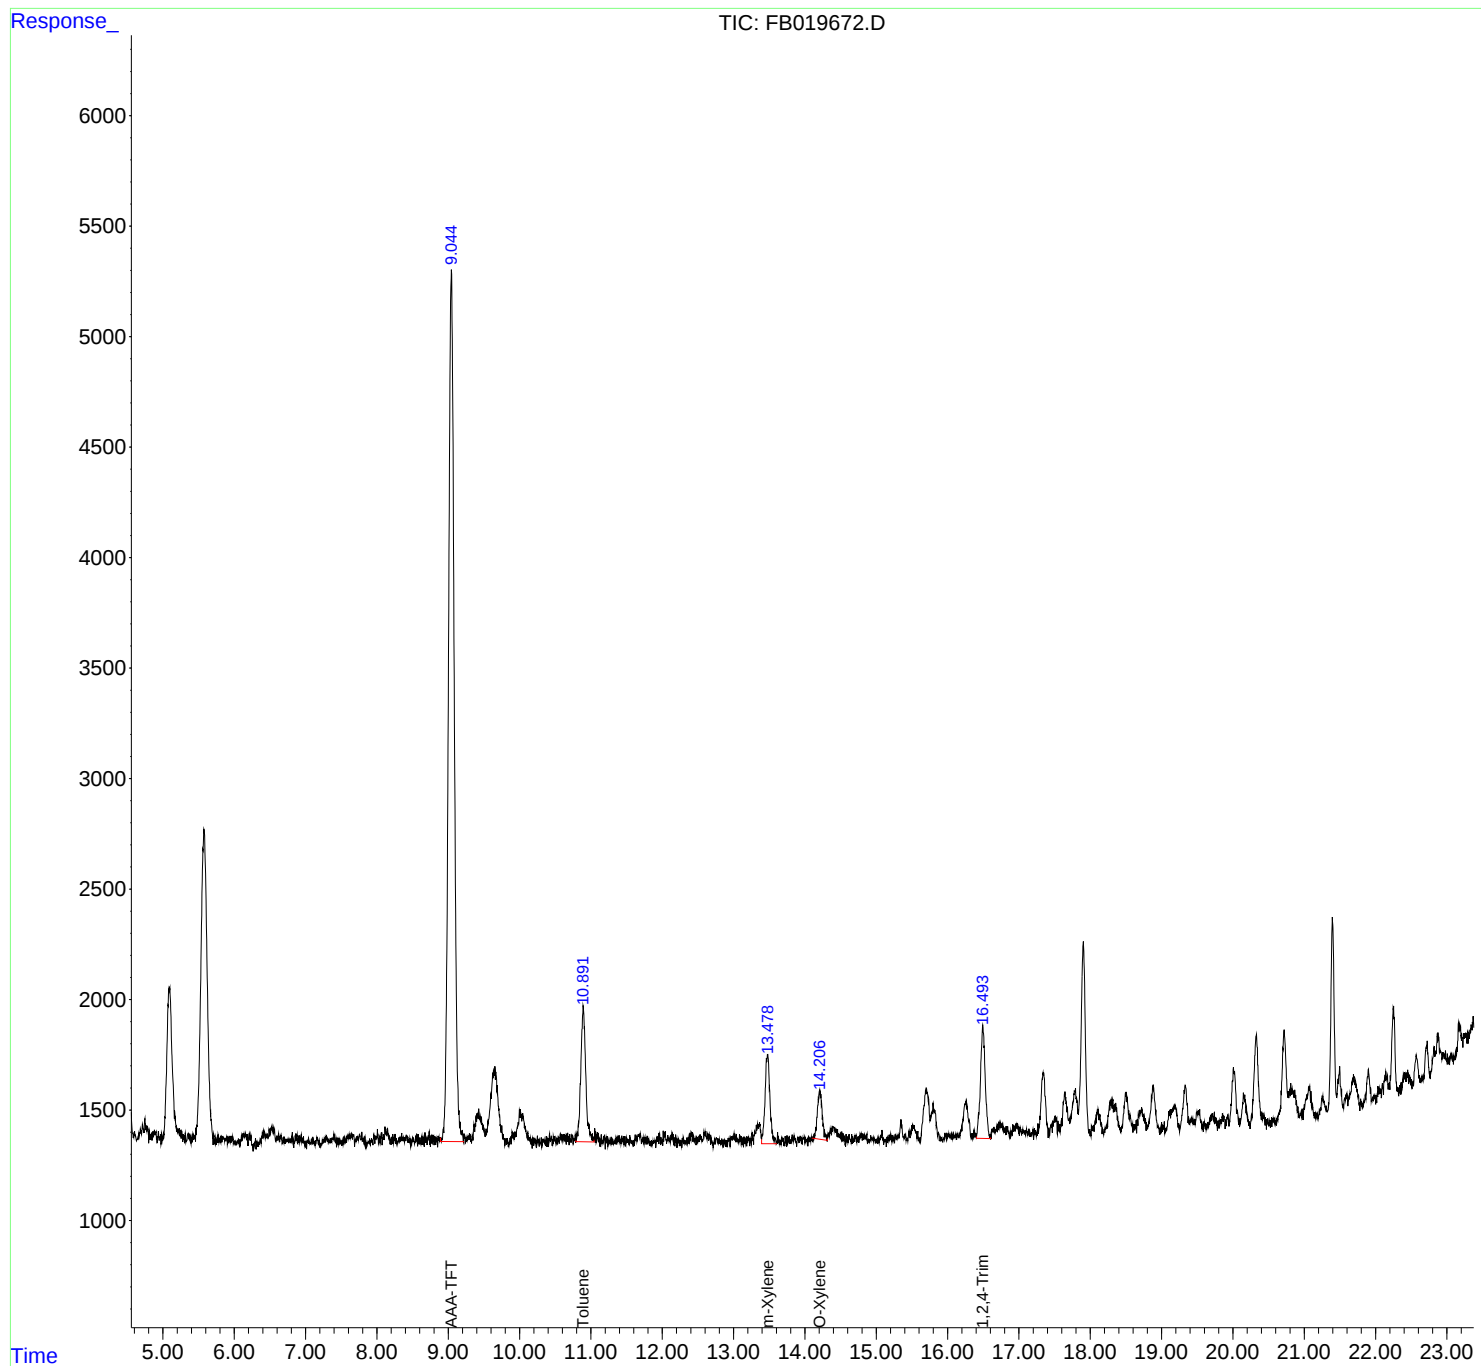


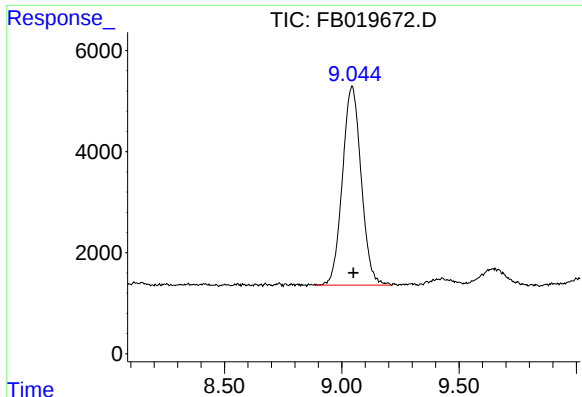

#5 AAA-TFT


R.T.: 9.045 min
Delta R.T.: -0.005 min
Response: 218658
Conc: 18.71 ng/ml

Instrument :
FID_B
ClientSampleId :

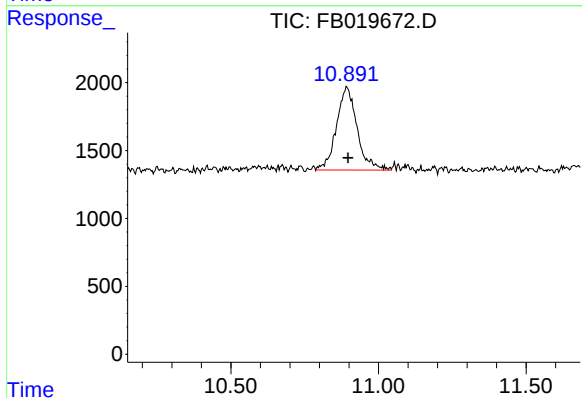


#6 Toluene

R.T.: 10.893 min
Delta R.T.: -0.003 min
Response: 29630
Conc: 1.69 ng/ml

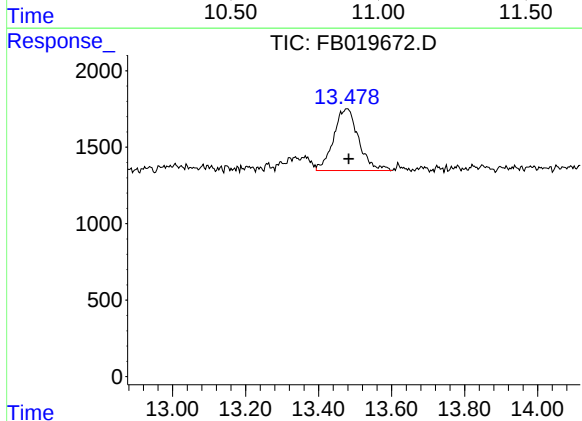


#8 m-Xylene

R.T.: 13.479 min
Delta R.T.: -0.003 min
Response: 19146
Conc: 0.84 ng/ml

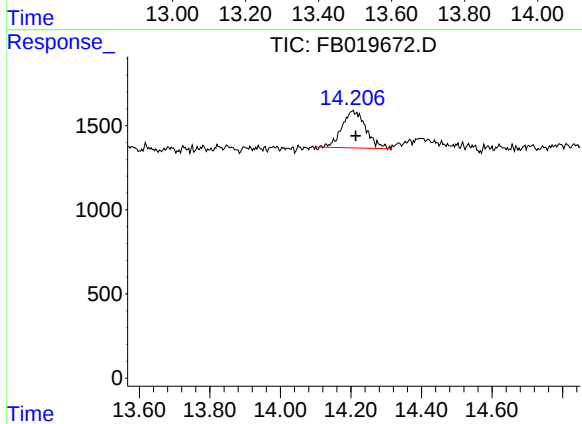

#9 O-Xylene

R.T.: 14.206 min
Delta R.T.: -0.008 min
Response: 10321
Conc: 0.46 ng/ml

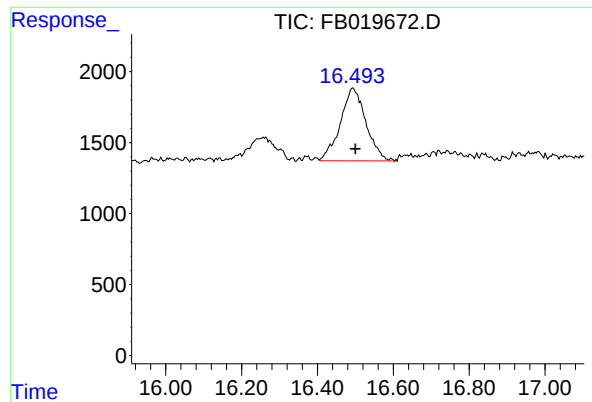

#10 1,2,4-Trimethylbenzene

R.T.: 16.494 min
Delta R.T.: -0.006 min
Response: 23932
Conc: 1.03 ng/ml

Instrument :
FID_B
ClientSampleId :