

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020819\
 Data File : FB019676.D
 Signal(s) : FID2B.CH
 Acq On : 8 Feb 2019 16:35
 Operator : MJ/SJ
 Sample : K1422-03MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TEST-PIT-1-BMS

Integration File: Calibration.e
 Quant Time: Feb 08 23:09:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.043	210833	18.036 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.898	567278	32.766 ng/ml
2) t 2,2,4-Trimethylpentane	7.658	497410	29.994 ng/ml
3) t n-Heptane	7.999	156470	9.710 ng/ml
4) t Benzene	8.136	195094	10.343 ng/ml
6) t Toluene	10.891	499346	28.546 ng/ml
7) t Ethylbenzene	13.343	198493	9.045 ng/ml
8) t m-Xylene	13.476	414586	18.114 ng/ml
9) t O-Xylene	14.208	408816	18.304 ng/ml
10) t 1,2,4-Trimethylbenzene	16.494	407758	17.598 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020819\
Data File : FB019676.D
Signal(s) : FID2B.CH
Acq On : 8 Feb 2019 16:35
Operator : MJ/SJ
Sample : K1422-03MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TEST-PIT-1-BMS

Integration File: Calibration.e
Quant Time: Feb 08 23:09:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

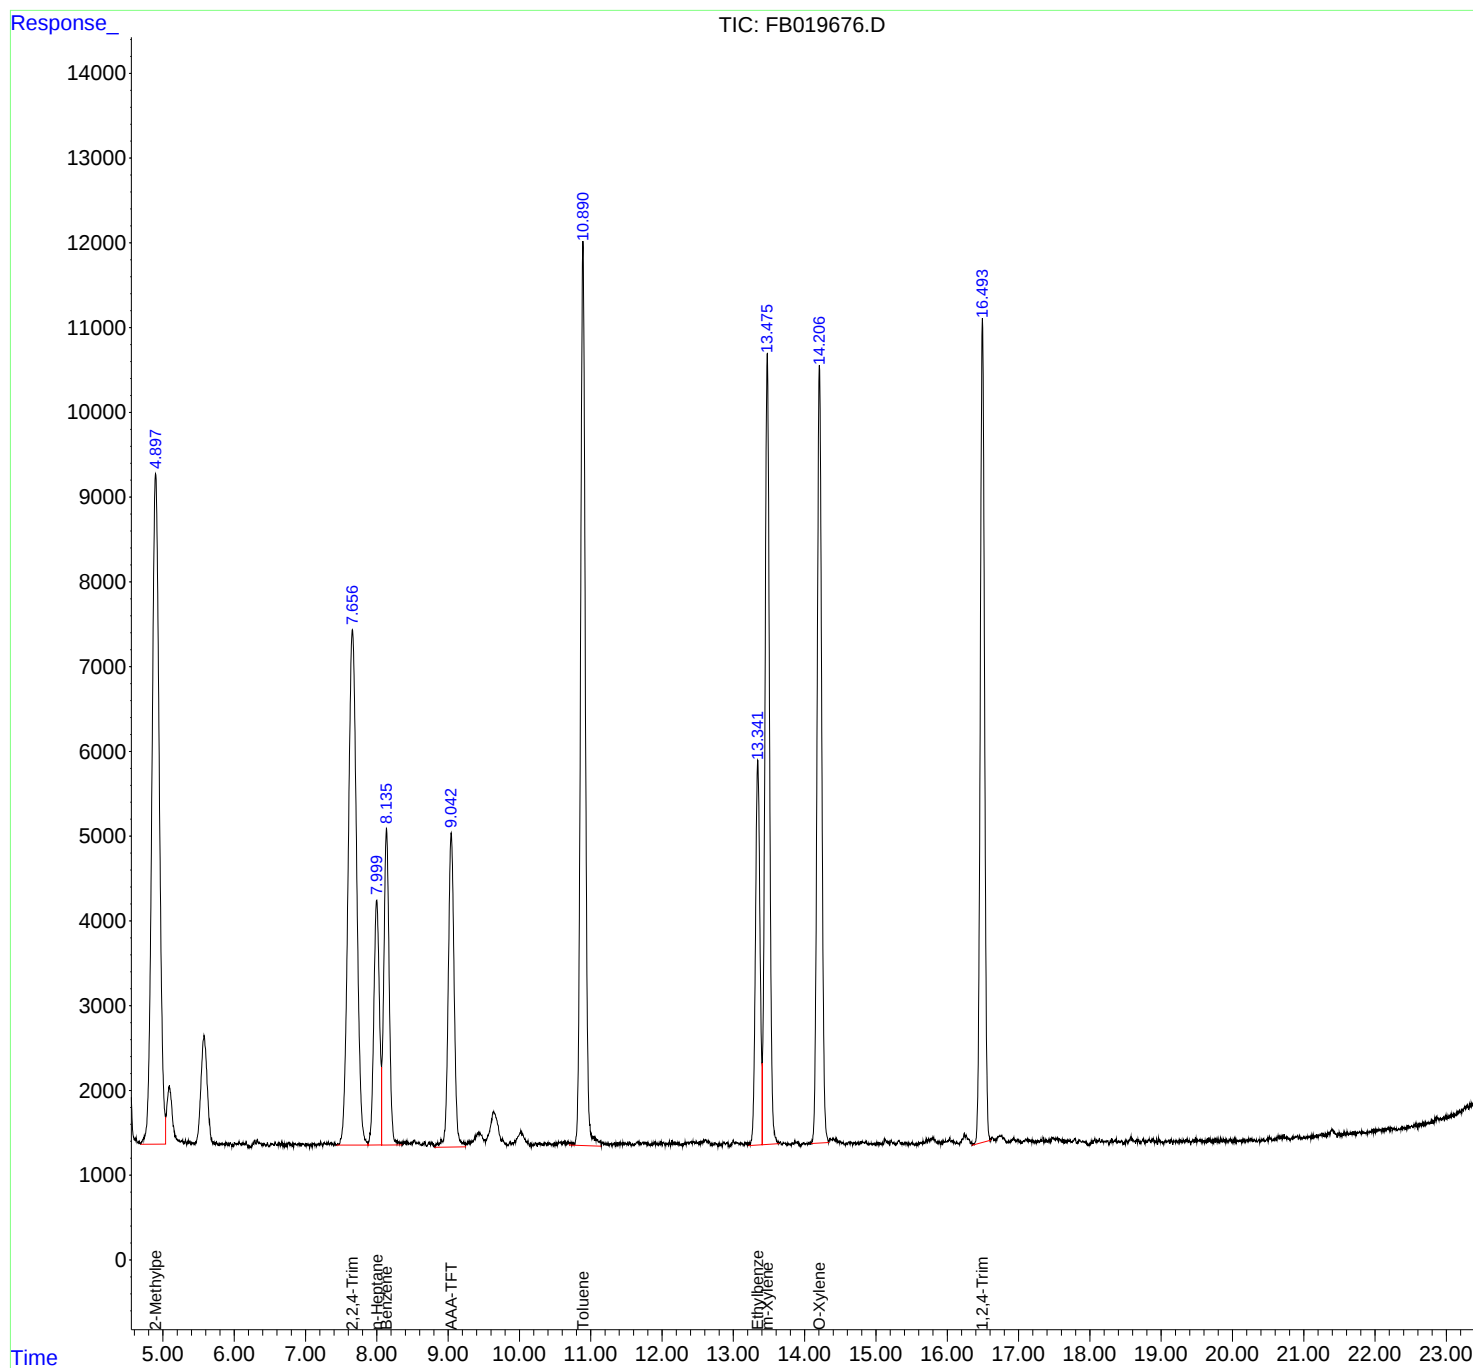


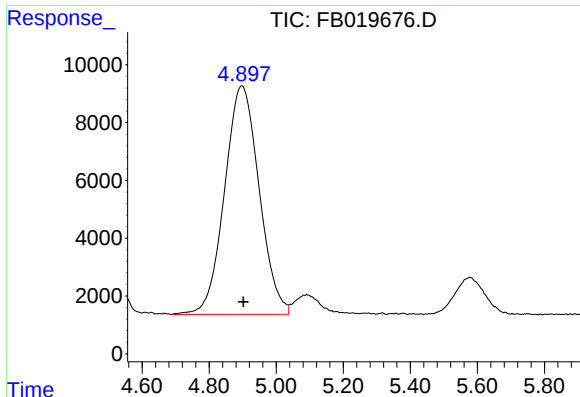

#1 2-Methylpentane


R.T.: 4.898 min
Delta R.T.: -0.004 min
Response: 567278
Conc: 32.77 ng/ml

Instrument :
FID_B
ClientSampleId :
TEST-PIT-1-BMS

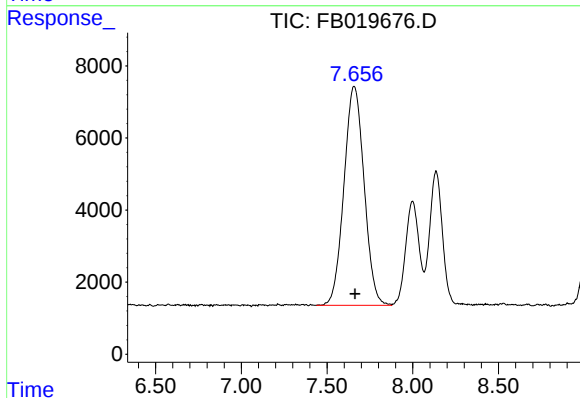


#2 2,2,4-Trimethylpentane

R.T.: 7.658 min
Delta R.T.: -0.006 min
Response: 497410
Conc: 29.99 ng/ml

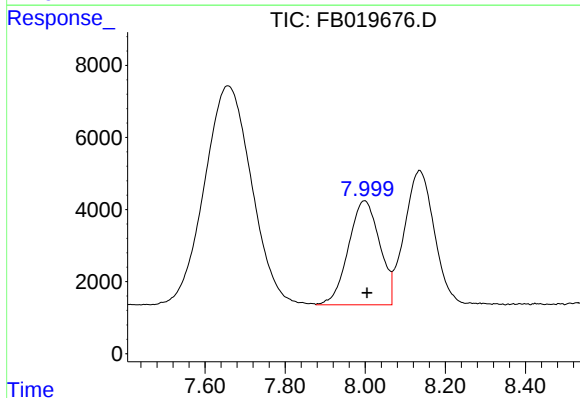


#3 n-Heptane

R.T.: 7.999 min
Delta R.T.: -0.006 min
Response: 156470
Conc: 9.71 ng/ml

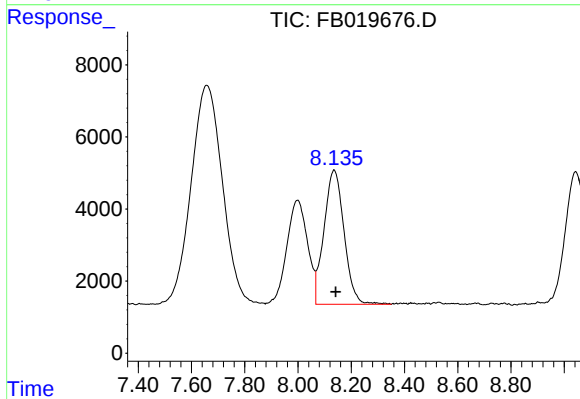

#4 Benzene


R.T.: 8.136 min
Delta R.T.: -0.005 min
Response: 195094
Conc: 10.34 ng/ml

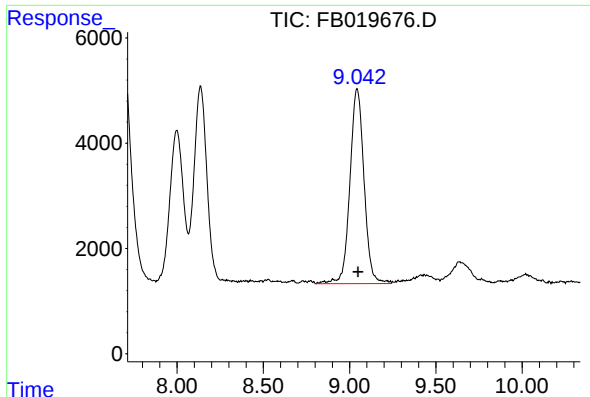

#5 AAA-TFT


R.T.: 9.043 min
Delta R.T.: -0.006 min
Response: 210833
Conc: 18.04 ng/ml

Instrument :
FID_B
ClientSampleId :
TEST-PIT-1-BMS

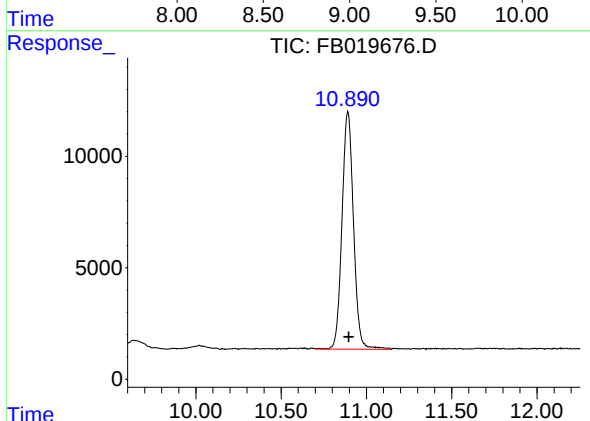


#6 Toluene

R.T.: 10.891 min
Delta R.T.: -0.005 min
Response: 499346
Conc: 28.55 ng/ml

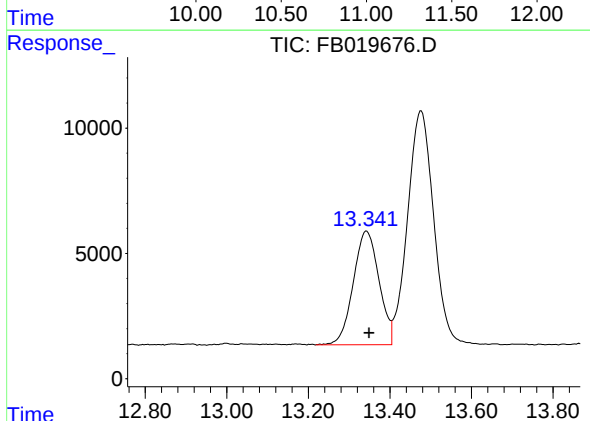


#7 Ethylbenzene

R.T.: 13.343 min
Delta R.T.: -0.006 min
Response: 198493
Conc: 9.04 ng/ml

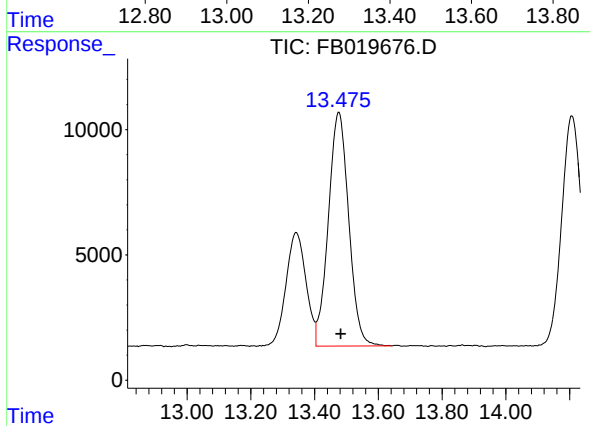

#8 m-Xylene


R.T.: 13.476 min
Delta R.T.: -0.006 min
Response: 414586
Conc: 18.11 ng/ml

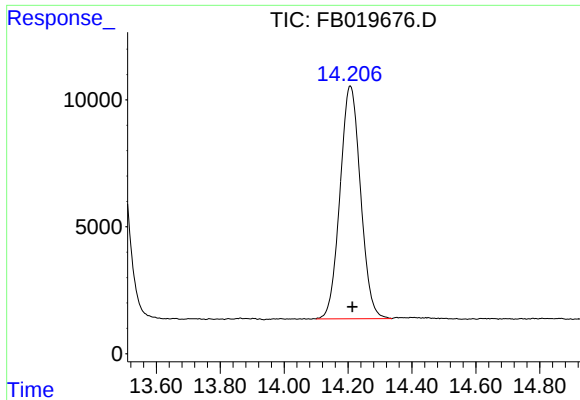

#9 O-Xylene

R.T.: 14.208 min
Delta R.T.: -0.006 min
Response: 408816
Conc: 18.30 ng/ml

Instrument :
FID_B
ClientSampleId :
TEST-PIT-1-BMS

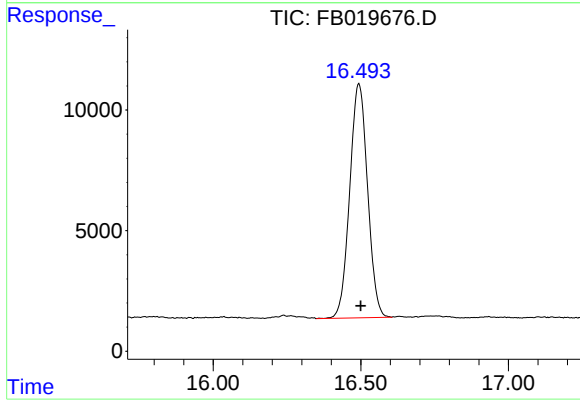

#10 1,2,4-Trimethylbenzene

R.T.: 16.494 min
Delta R.T.: -0.006 min
Response: 407758
Conc: 17.60 ng/ml