

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020819\
 Data File : FB019677.D
 Signal(s) : FID2B.CH
 Acq On : 8 Feb 2019 17:05
 Operator : MJ/SJ
 Sample : K1422-03MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TEST-PIT-1-BMSD

Integration File: Calibration.e
 Quant Time: Feb 08 23:10:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.044	192431	16.462 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.899	534742	30.887 ng/ml
2) t 2,2,4-Trimethylpentane	7.658	462371	27.881 ng/ml
3) t n-Heptane	7.999	145063	9.002 ng/ml
4) t Benzene	8.136	187555	9.944 ng/ml
6) t Toluene	10.891	480521	27.470 ng/ml
7) t Ethylbenzene	13.343	193067	8.798 ng/ml
8) t m-Xylene	13.476	404393	17.669 ng/ml
9) t O-Xylene	14.208	397961	17.818 ng/ml
10) t 1,2,4-Trimethylbenzene	16.494	398398	17.194 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020819\
Data File : FB019677.D
Signal(s) : FID2B.CH
Acq On : 8 Feb 2019 17:05
Operator : MJ/SJ
Sample : K1422-03MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TEST-PIT-1-BMSD

Integration File: Calibration.e
Quant Time: Feb 08 23:10:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

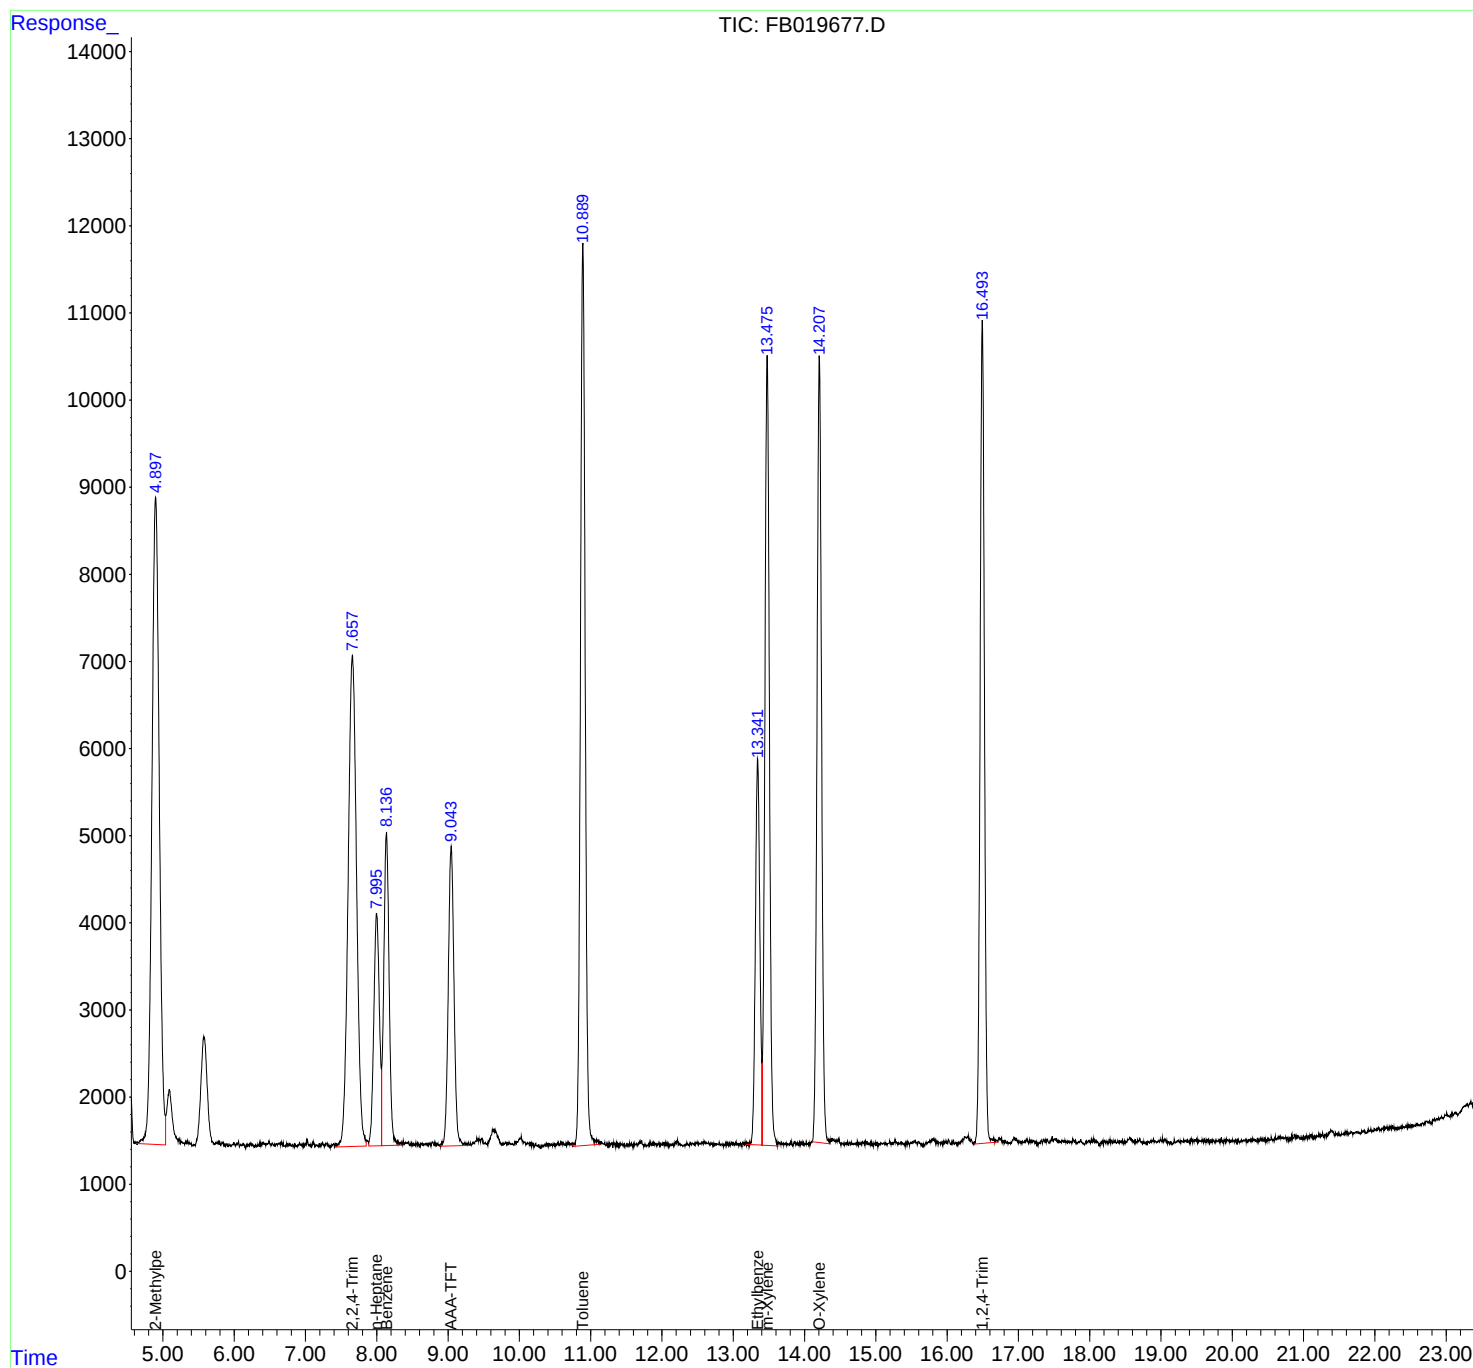


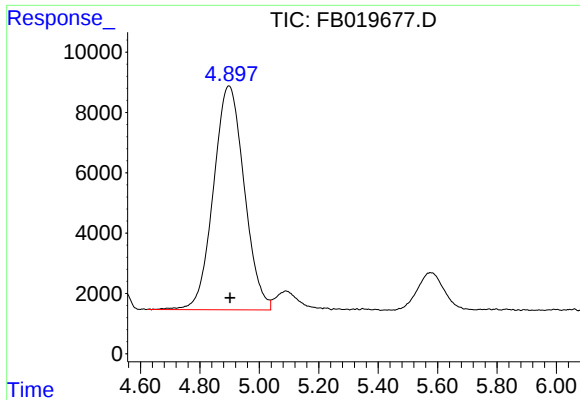

#1 2-Methylpentane


R.T.: 4.899 min
Delta R.T.: -0.003 min
Response: 534742
Conc: 30.89 ng/ml

Instrument :
FID_B
ClientSampleId :
TEST-PIT-1-BMSD

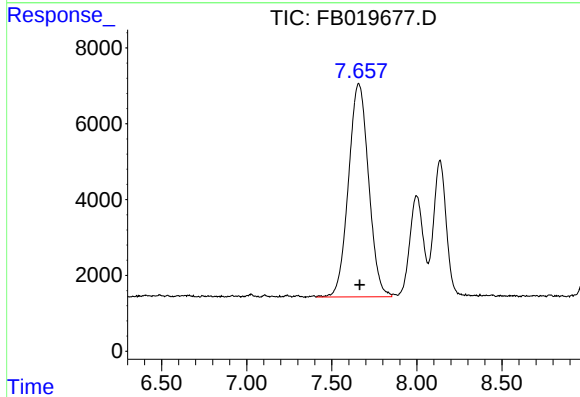


#2 2,2,4-Trimethylpentane

R.T.: 7.658 min
Delta R.T.: -0.006 min
Response: 462371
Conc: 27.88 ng/ml

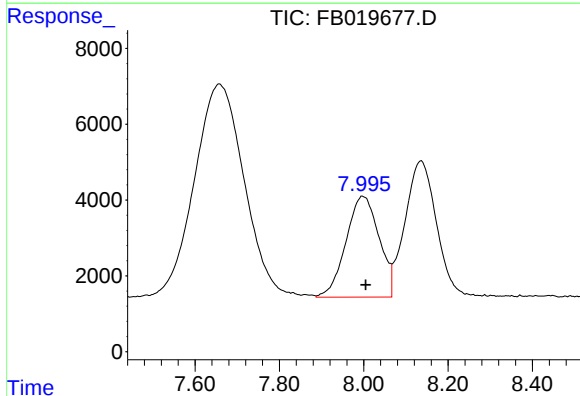


#3 n-Heptane

R.T.: 7.999 min
Delta R.T.: -0.006 min
Response: 145063
Conc: 9.00 ng/ml

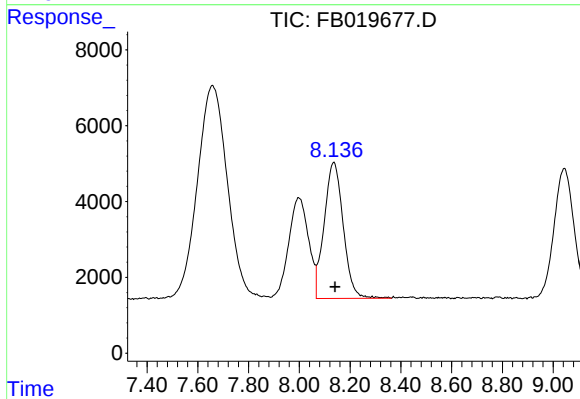

#4 Benzene


R.T.: 8.136 min
Delta R.T.: -0.005 min
Response: 187555
Conc: 9.94 ng/ml

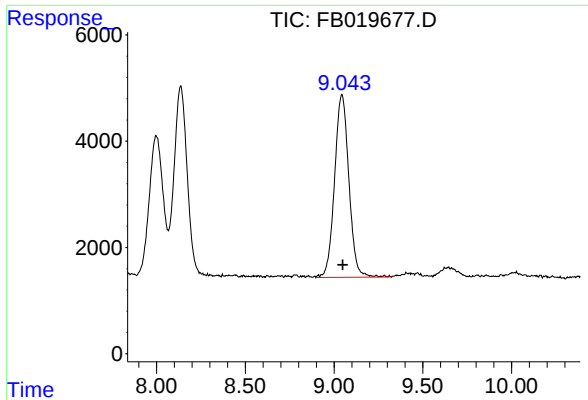

#5 AAA-TFT


R.T.: 9.044 min
Delta R.T.: -0.005 min
Response: 192431
Conc: 16.46 ng/ml

Instrument :
FID_B
ClientSampleId :
TEST-PIT-1-BMSD

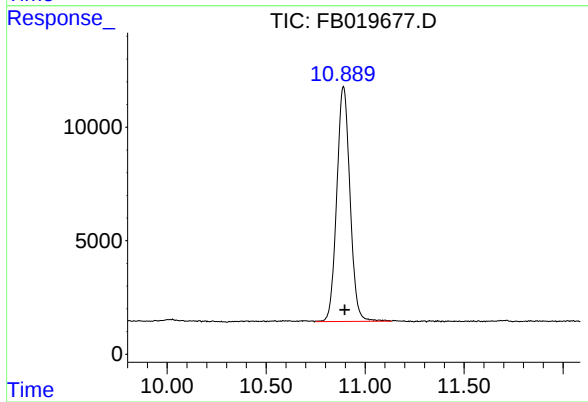


#6 Toluene

R.T.: 10.891 min
Delta R.T.: -0.006 min
Response: 480521
Conc: 27.47 ng/ml

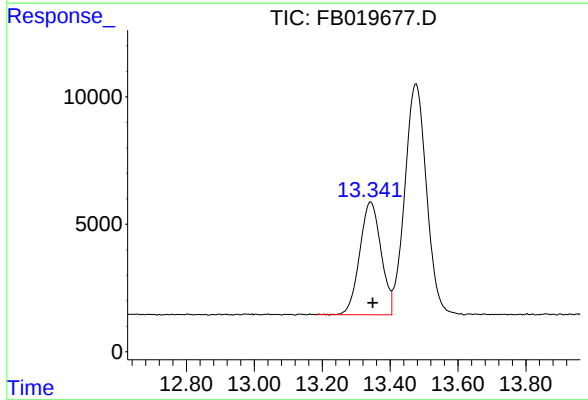


#7 Ethylbenzene

R.T.: 13.343 min
Delta R.T.: -0.006 min
Response: 193067
Conc: 8.80 ng/ml

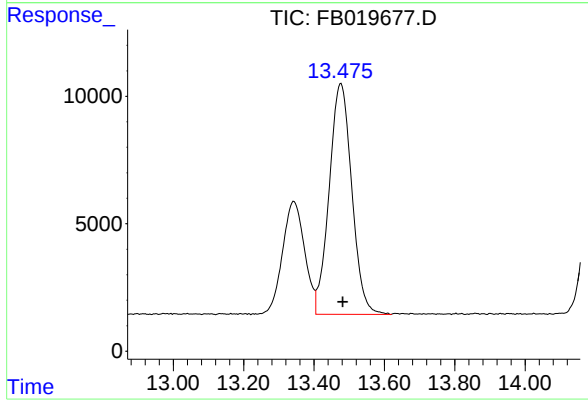

#8 m-Xylene


R.T.: 13.476 min
Delta R.T.: -0.006 min
Response: 404393
Conc: 17.67 ng/ml

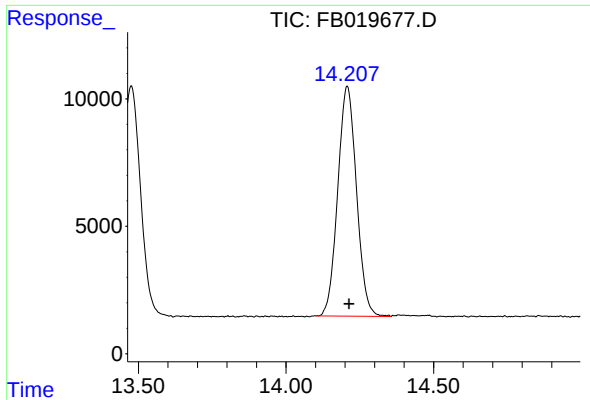

#9 O-Xylene

R.T.: 14.208 min
Delta R.T.: -0.006 min
Response: 397961
Conc: 17.82 ng/ml

Instrument :
FID_B
ClientSampleId :
TEST-PIT-1-BMSD

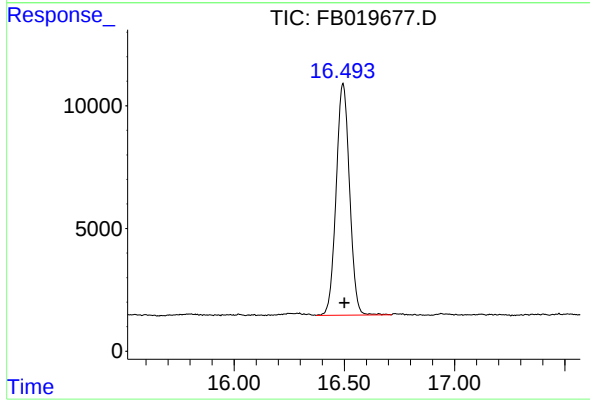

#10 1,2,4-Trimethylbenzene

R.T.: 16.494 min
Delta R.T.: -0.006 min
Response: 398398
Conc: 17.19 ng/ml