

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020823\
 Data File : FB029267.D
 Signal(s) : FID2B.CH
 Acq On : 8 Feb 2023 11:48
 Operator : YP/AJ
 Sample : BSF0208S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0208S1

Integration File: Calibration.e
 Quant Time: Feb 09 02:18:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	206710	21.491 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	474203	29.886 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	519710	30.174 ng/ml
3) t n-Heptane	7.746	177574	9.814 ng/ml
4) t Benzene	7.883	200125	9.608 ng/ml
6) t Toluene	10.615	587583	28.995 ng/ml
7) t Ethylbenzene	13.052	186193	9.755 ng/ml
8) t m-Xylene	13.185	373721	19.713 ng/ml
9) t O-Xylene	13.911	369713	20.263 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	378261	20.100 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020823\
Data File : FB029267.D
Signal(s) : FID2B.CH
Acq On : 8 Feb 2023 11:48
Operator : YP/AJ
Sample : BSF0208S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0208S1

Integration File: Calibration.e
Quant Time: Feb 09 02:18:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

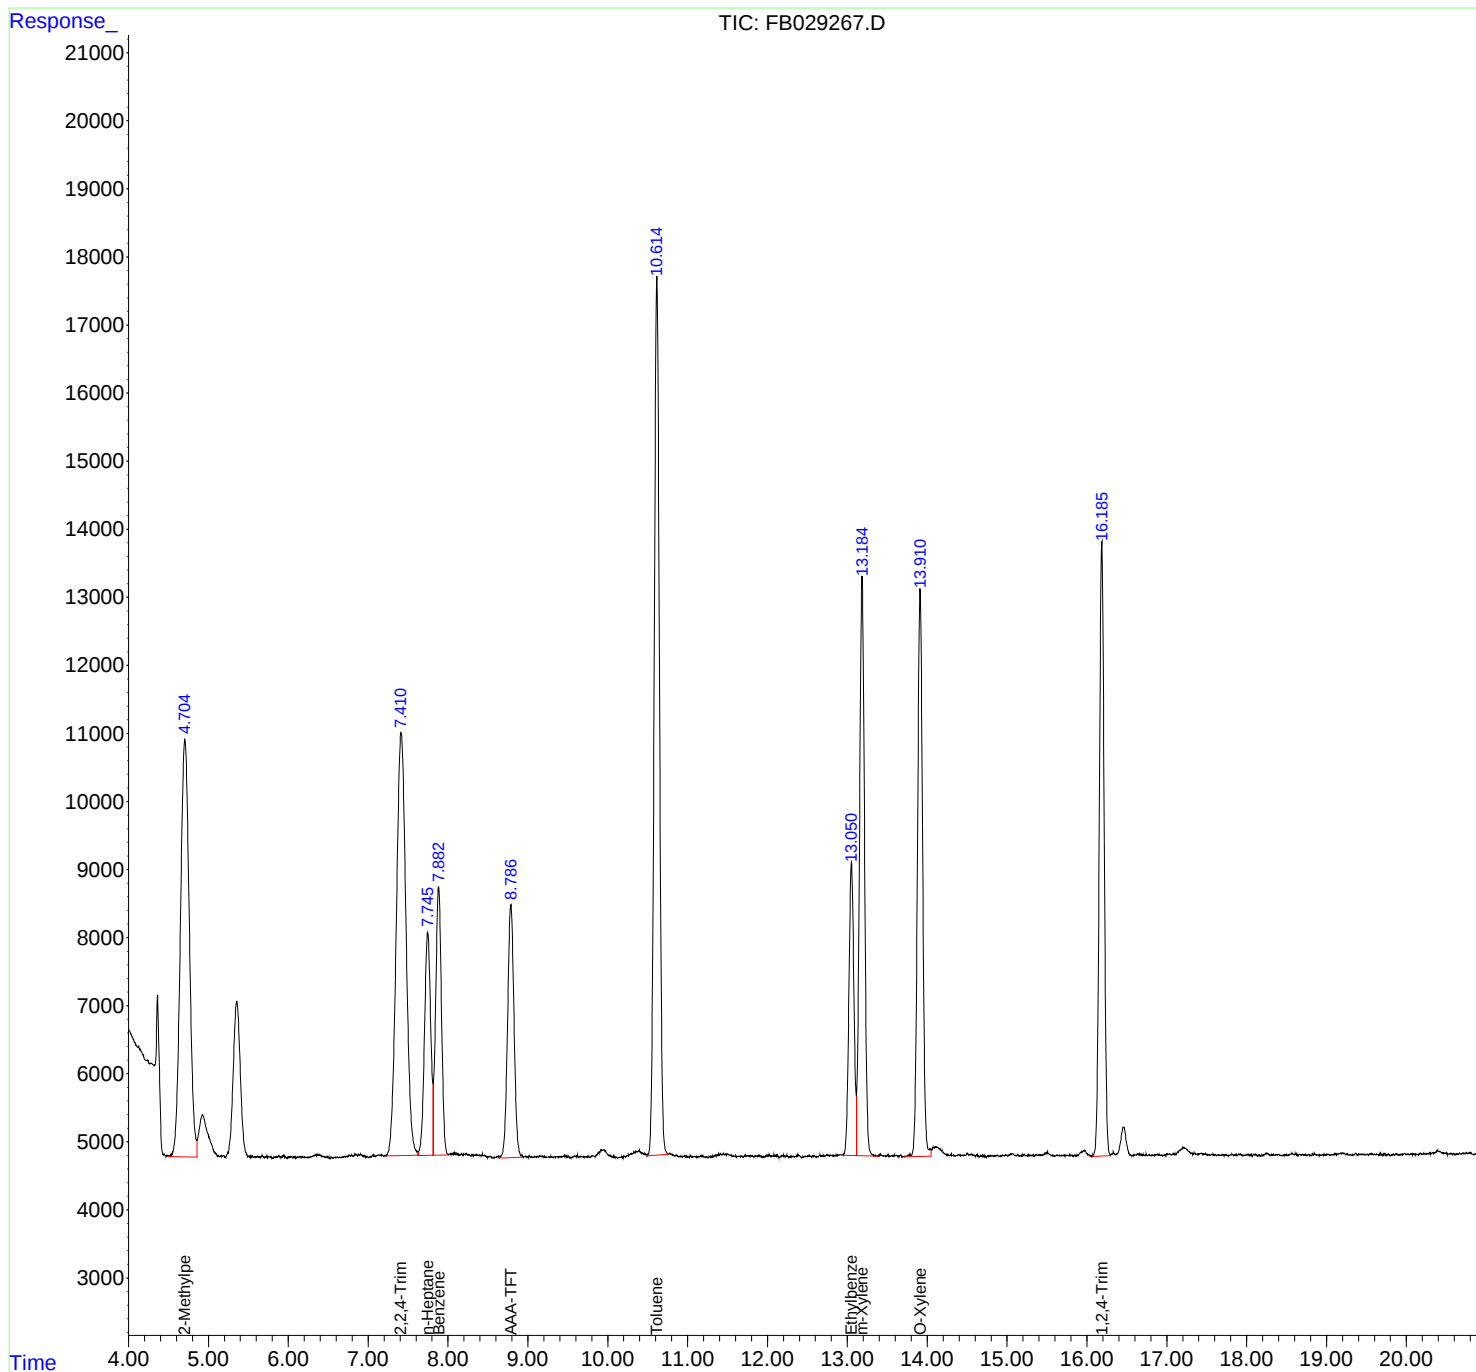


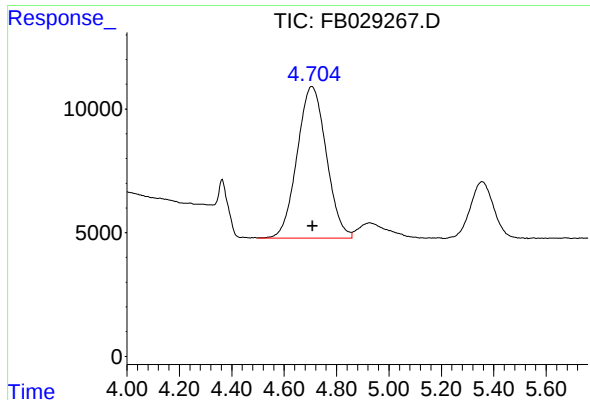

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: -0.003 min
Response: 474203
Conc: 29.89 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0208S1

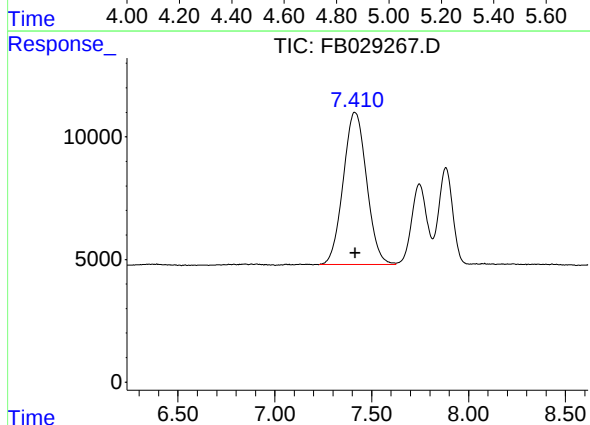


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.003 min
Response: 519710
Conc: 30.17 ng/ml

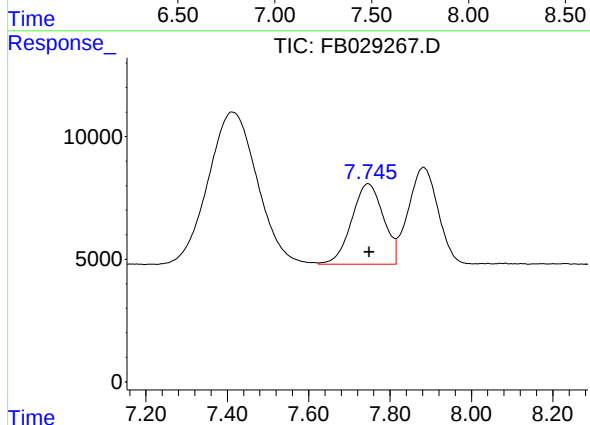


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.002 min
Response: 177574
Conc: 9.81 ng/ml

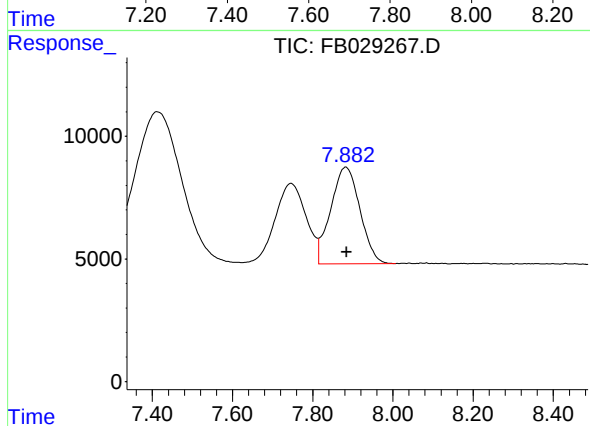

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.002 min
Response: 200125
Conc: 9.61 ng/ml

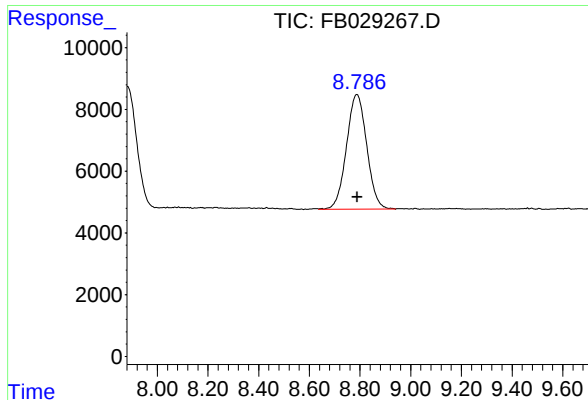

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: -0.002 min
Response: 206710
Conc: 21.49 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0208S1

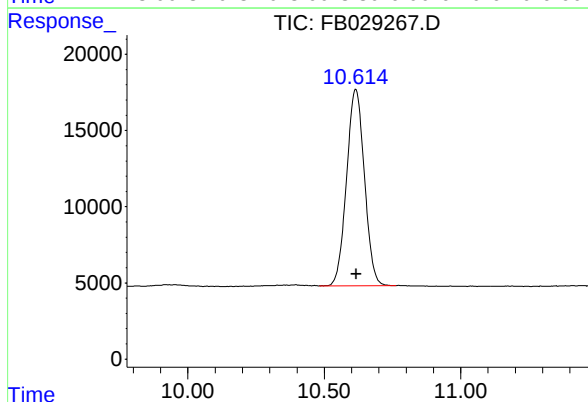


#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.002 min
Response: 587583
Conc: 29.00 ng/ml

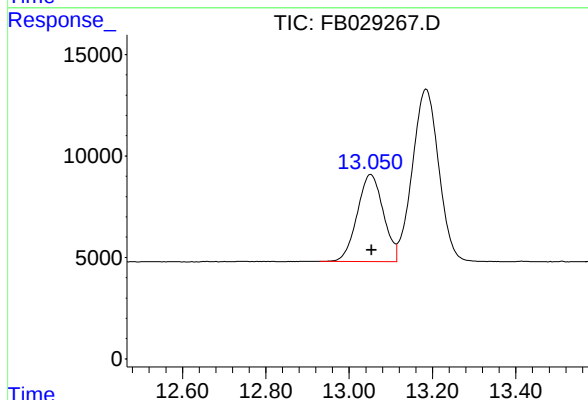


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.002 min
Response: 186193
Conc: 9.76 ng/ml

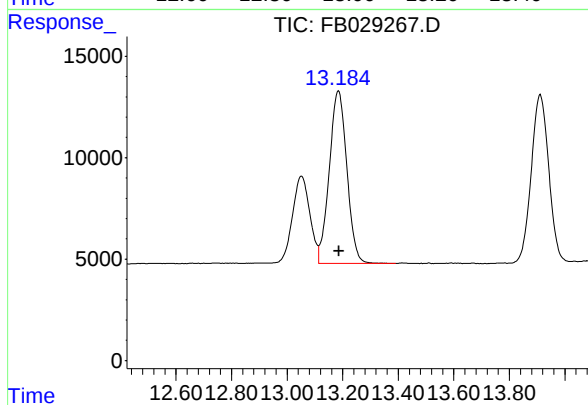

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.001 min
Response: 373721
Conc: 19.71 ng/ml

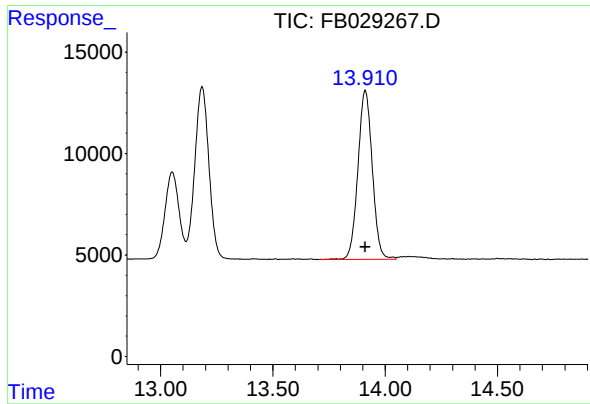

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: -0.001 min
Response: 369713
Conc: 20.26 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0208S1

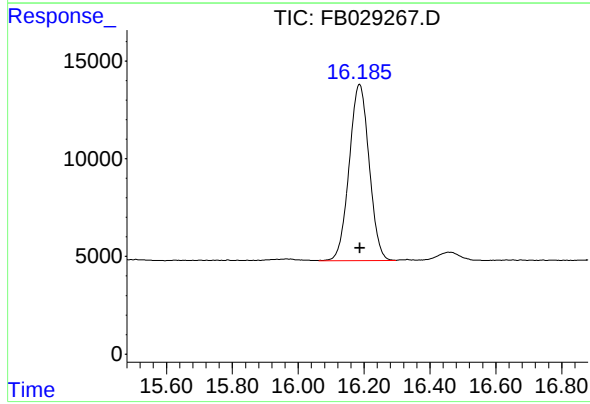

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: -0.001 min
Response: 378261
Conc: 20.10 ng/ml