

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020823\
 Data File : FB029272.D
 Signal(s) : FID2B.CH
 Acq On : 8 Feb 2023 14:53
 Operator : YP/AJ
 Sample : BSF0208S2
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0208S2

Integration File: Calibration.e
 Quant Time: Feb 09 02:19:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	193267	20.094 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	464500	29.275 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	511961	29.725 ng/ml
3) t n-Heptane	7.748	181154	10.012 ng/ml
4) t Benzene	7.886	208212	9.996 ng/ml
6) t Toluene	10.618	617209	30.457 ng/ml
7) t Ethylbenzene	13.054	192011	10.060 ng/ml
8) t m-Xylene	13.187	380770	20.085 ng/ml
9) t O-Xylene	13.913	368684	20.206 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	366334	19.466 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB020823\
Data File : FB029272.D
Signal(s) : FID2B.CH
Acq On : 8 Feb 2023 14:53
Operator : YP/AJ
Sample : BSF0208S2
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0208S2

Integration File: Calibration.e
Quant Time: Feb 09 02:19:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

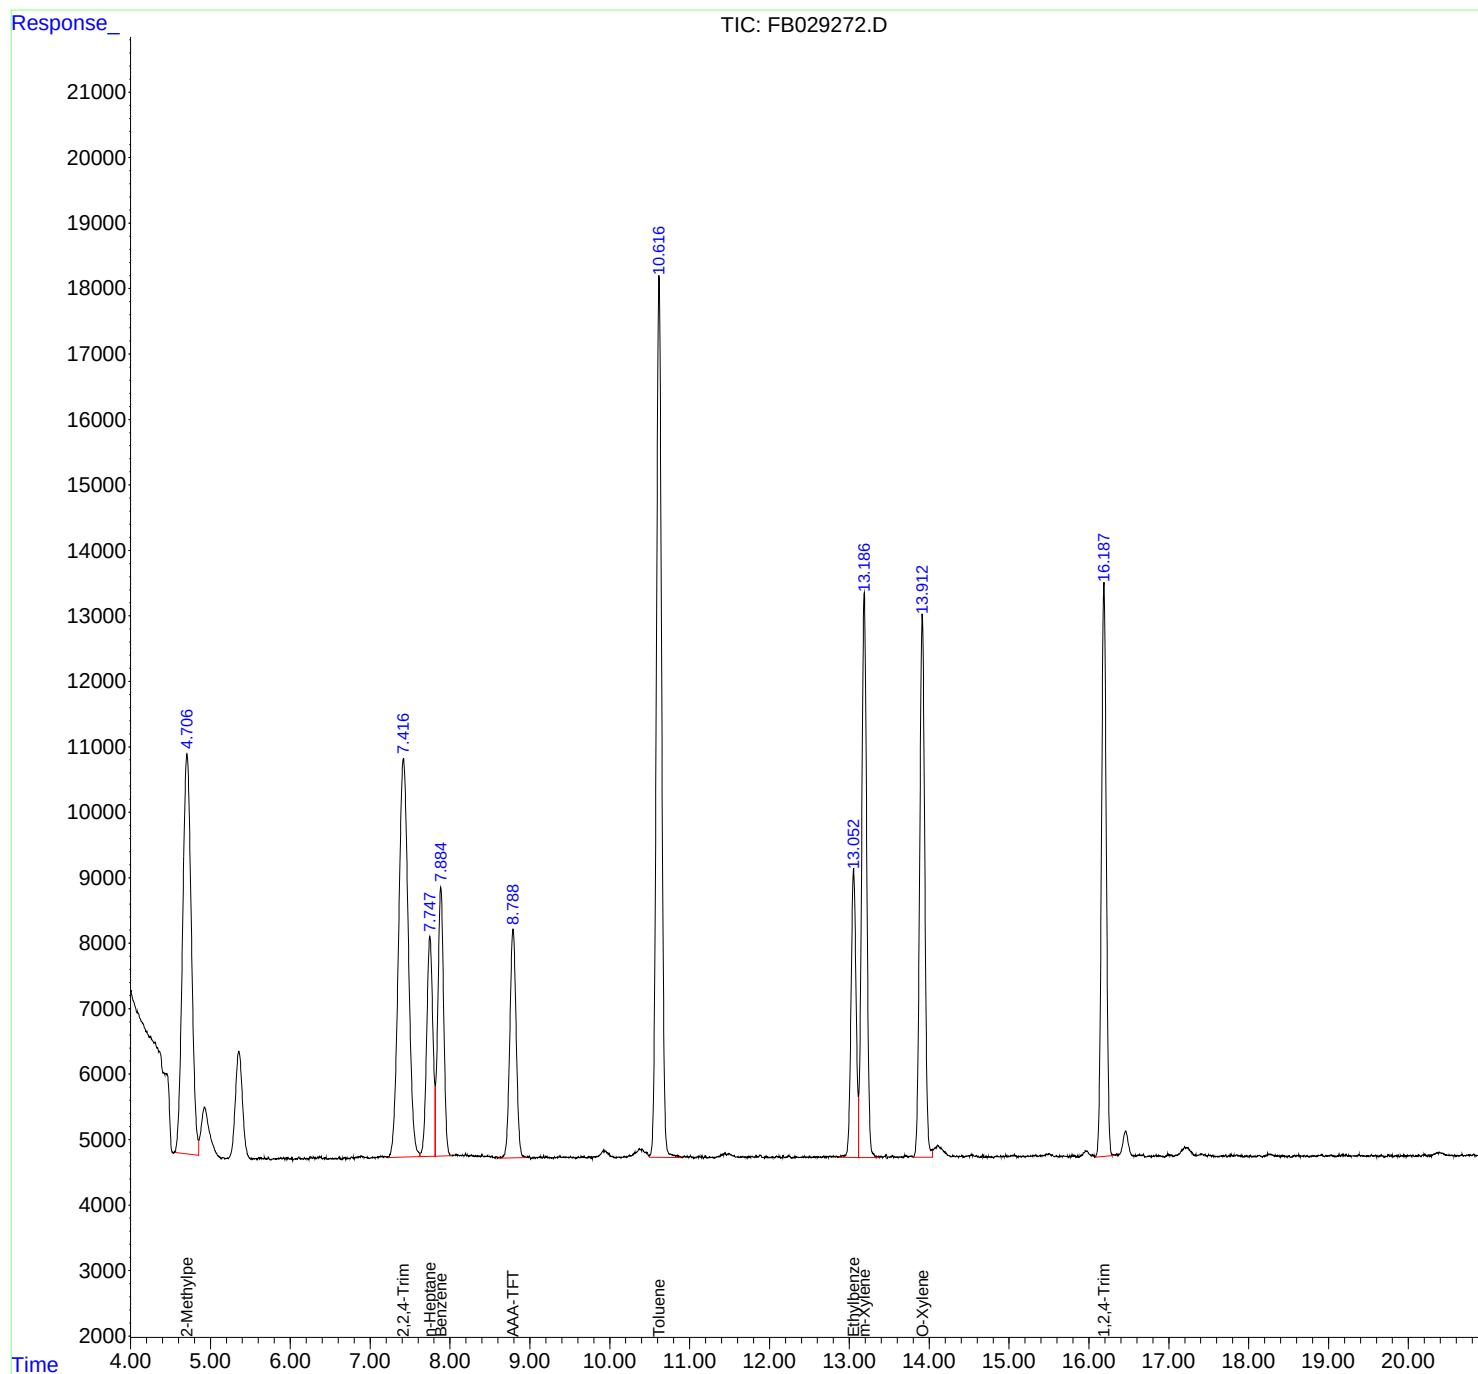


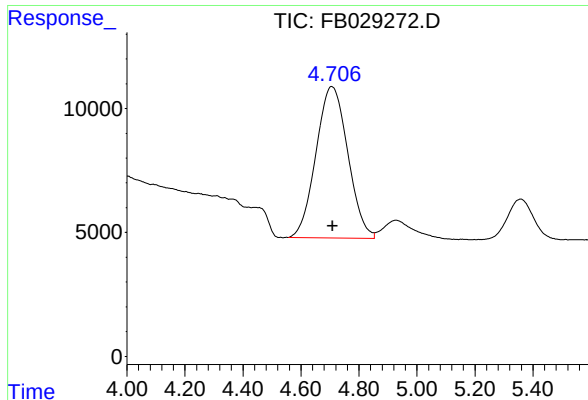

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: -0.002 min
Response: 464500
Conc: 29.27 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0208S2

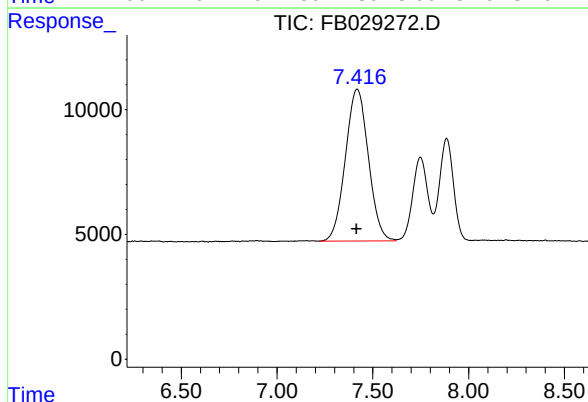


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.003 min
Response: 511961
Conc: 29.72 ng/ml

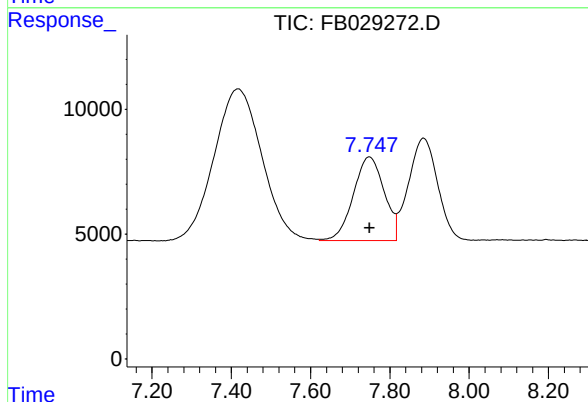


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: 0.000 min
Response: 181154
Conc: 10.01 ng/ml

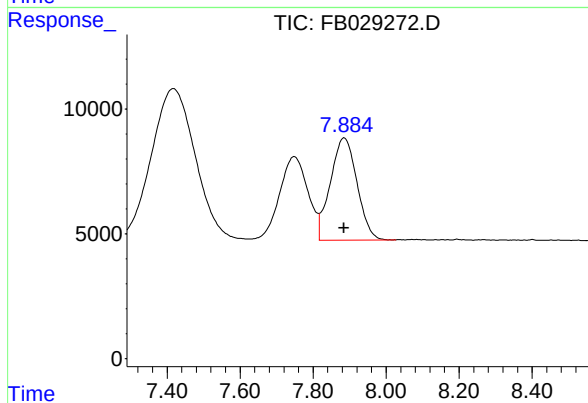

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 208212
Conc: 10.00 ng/ml

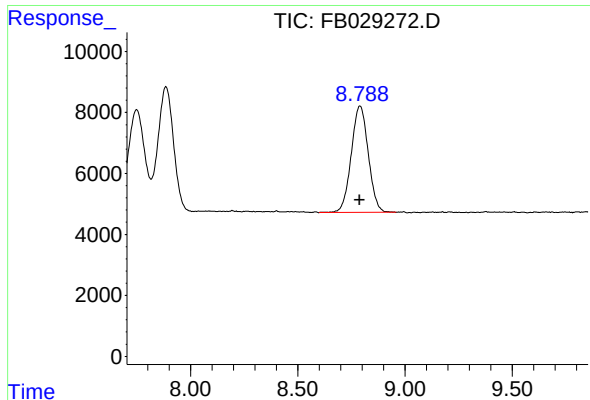

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 193267
Conc: 20.09 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0208S2

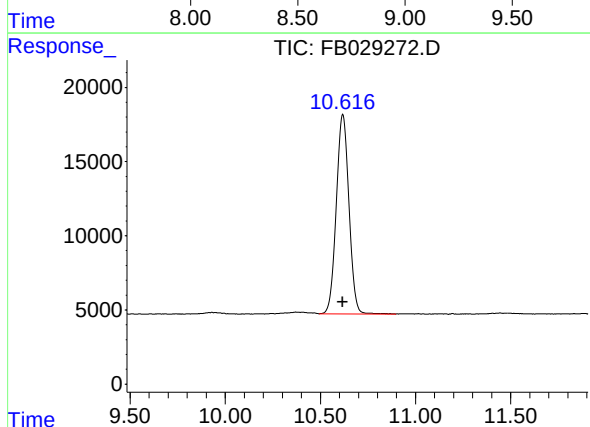


#6 Toluene

R.T.: 10.618 min
Delta R.T.: 0.000 min
Response: 617209
Conc: 30.46 ng/ml

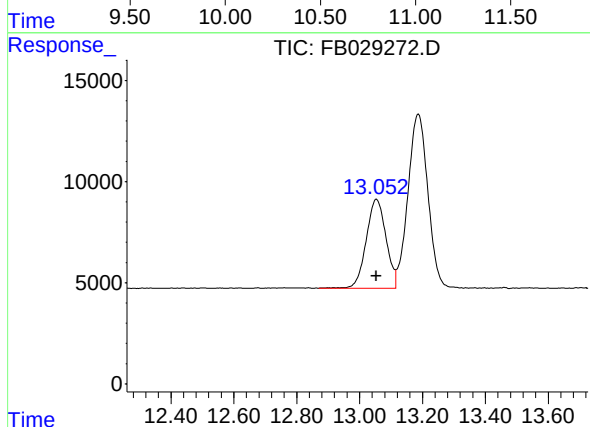


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: 0.000 min
Response: 192011
Conc: 10.06 ng/ml

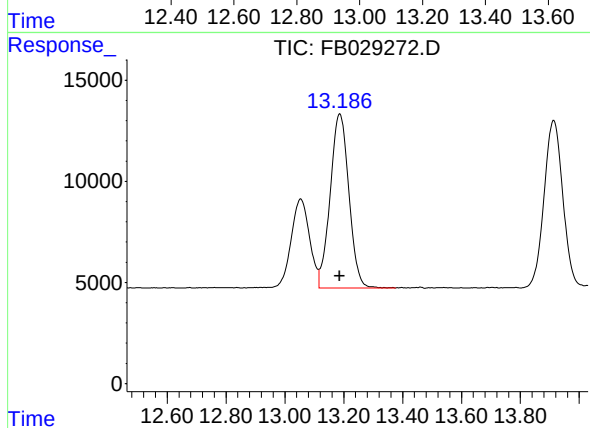

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: 0.000 min
Response: 380770
Conc: 20.09 ng/ml

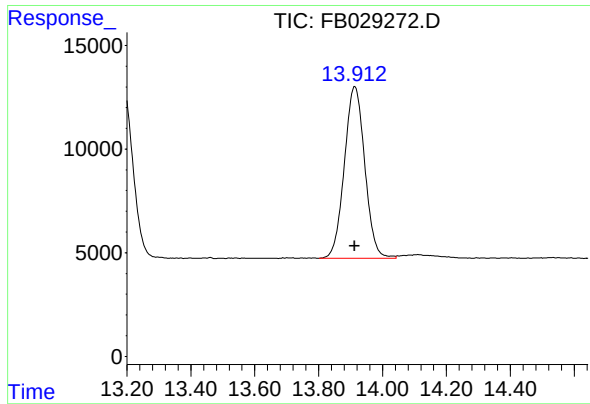

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: 0.000 min
Response: 368684
Conc: 20.21 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0208S2

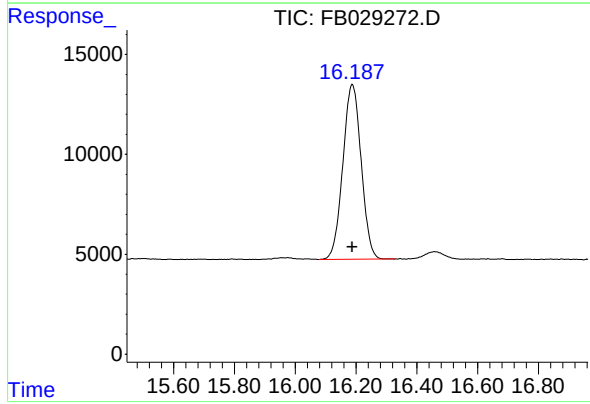

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: 0.000 min
Response: 366334
Conc: 19.47 ng/ml