

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021023\
 Data File : FB029281.D
 Signal(s) : FID2B.CH
 Acq On : 10 Feb 2023 11:33
 Operator : YP/AJ
 Sample : 01510-03
 Misc : 5.24G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Feb 13 05:49:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	164014	17.052 ng/ml
Target Compounds			
6) t Toluene	10.617	8504	0.420 ng/ml
8) t m-Xylene	13.175	150	0.008 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	13387	0.711 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021023\
Data File : FB029281.D
Signal(s) : FID2B.CH
Acq On : 10 Feb 2023 11:33
Operator : YP/AJ
Sample : 01510-03
Misc : 5.24G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 13 05:49:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

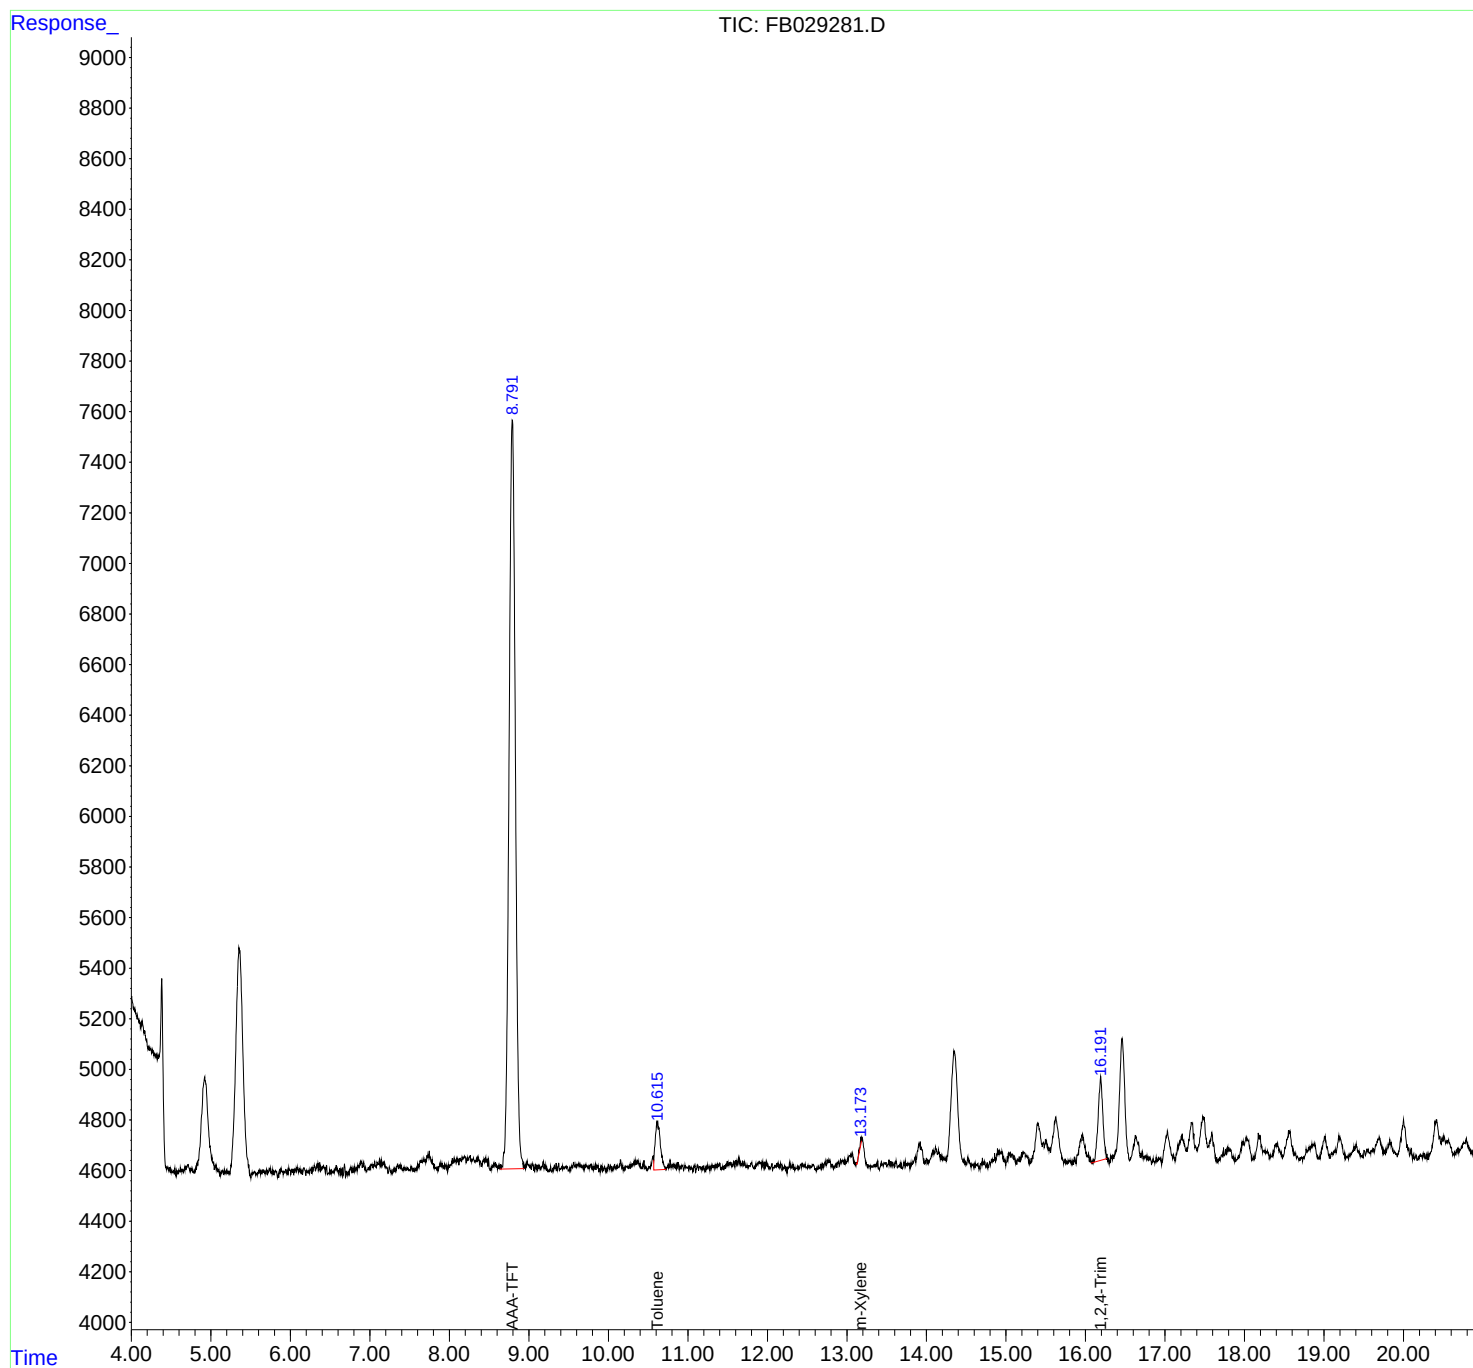


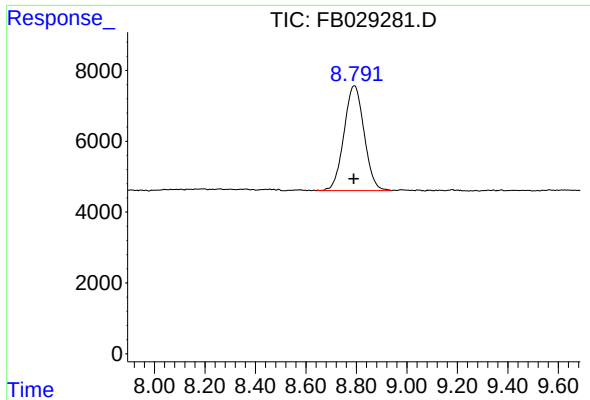

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.003 min
Response: 164014
Conc: 17.05 ng/ml

Instrument :
FID_B
ClientSampleId :

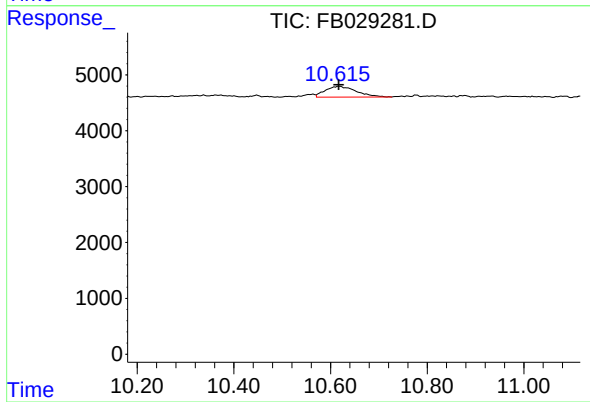


#6 Toluene

R.T.: 10.617 min
Delta R.T.: 0.000 min
Response: 8504
Conc: 0.42 ng/ml

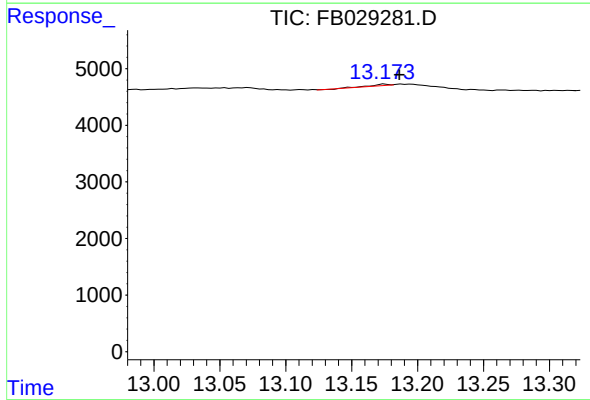

#8 m-Xylene

R.T.: 13.175 min
Delta R.T.: -0.011 min
Response: 150
Conc: 0.01 ng/ml

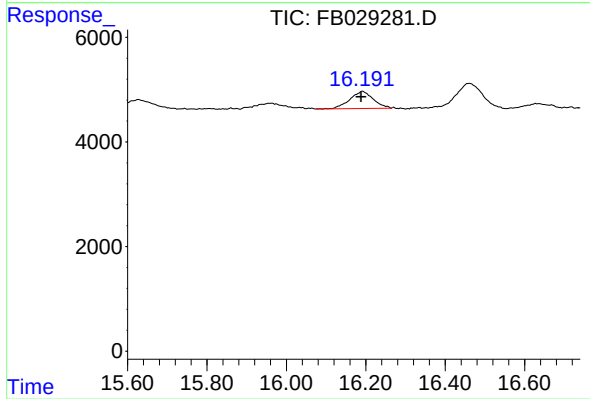

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.004 min
Response: 13387
Conc: 0.71 ng/ml