

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021023\
 Data File : FB029280.D
 Signal(s) : FID2B.CH
 Acq On : 10 Feb 2023 10:56
 Operator : YP/AJ
 Sample : BSF0210S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0210S1

Integration File: SAMPLE.e
 Quant Time: Feb 13 05:49:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	156650	16.287 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	364487	22.971 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	358789	20.831 ng/ml
3) t n-Heptane	7.751	142181	7.858 ng/ml
4) t Benzene	7.887	155373	7.459 ng/ml
6) t Toluene	10.620	456628	22.533 ng/ml
7) t Ethylbenzene	13.056	143312	7.509 ng/ml
8) t m-Xylene	13.188	283824	14.971 ng/ml
9) t O-Xylene	13.915	273400	14.984 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	270084	14.352 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021023\
Data File : FB029280.D
Signal(s) : FID2B.CH
Acq On : 10 Feb 2023 10:56
Operator : YP/AJ
Sample : BSF0210S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0210S1

Integration File: SAMPLE.e
Quant Time: Feb 13 05:49:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

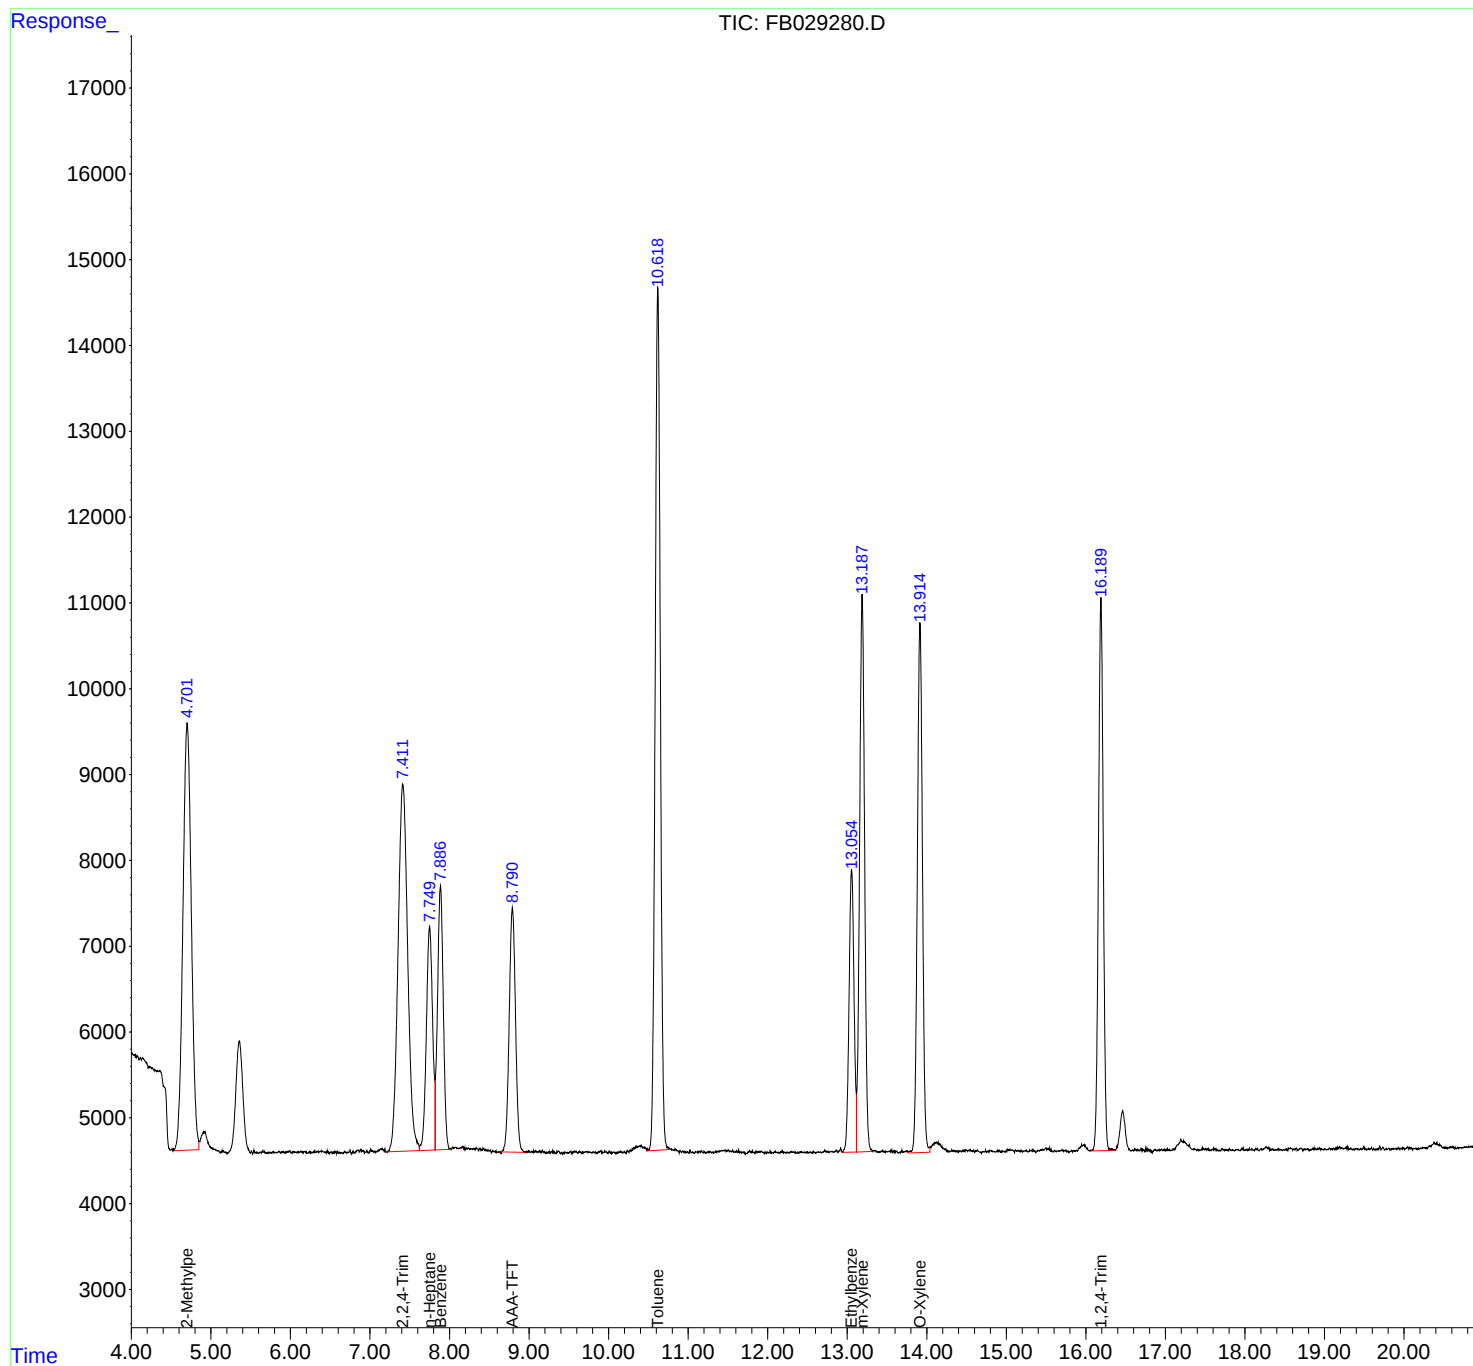


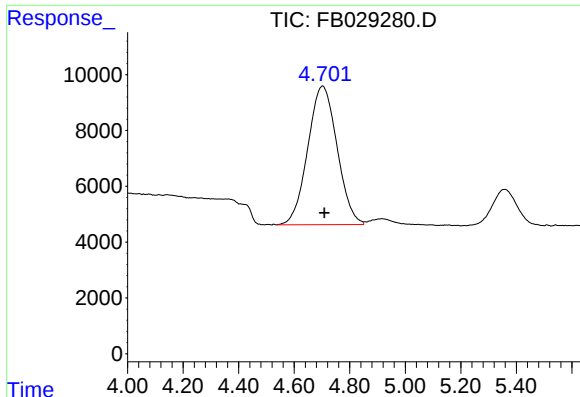

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: -0.006 min
Response: 364487
Conc: 22.97 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0210S1

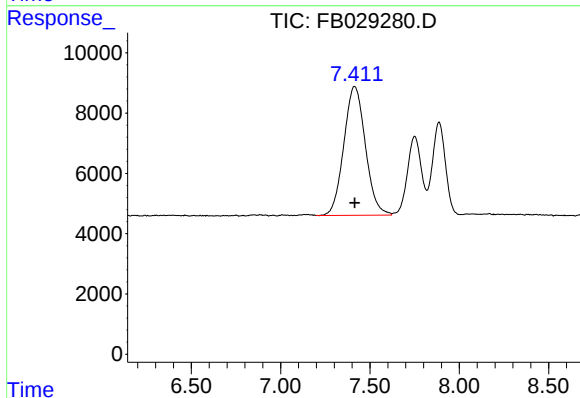


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.002 min
Response: 358789
Conc: 20.83 ng/ml

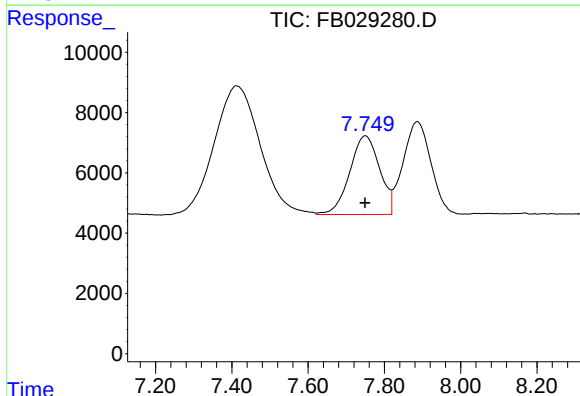


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.002 min
Response: 142181
Conc: 7.86 ng/ml

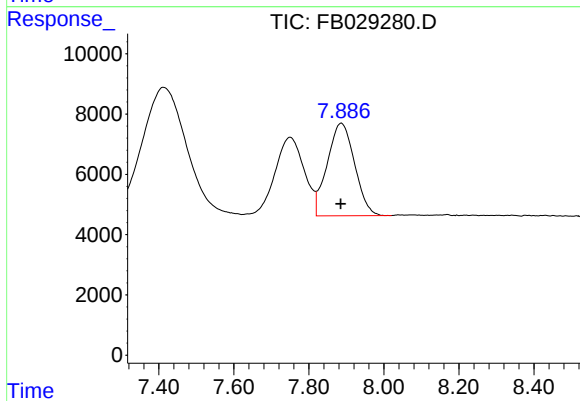

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.002 min
Response: 155373
Conc: 7.46 ng/ml

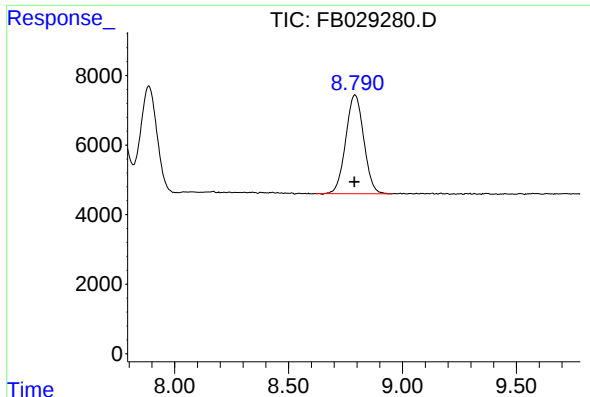

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.002 min
Response: 156650
Conc: 16.29 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0210S1

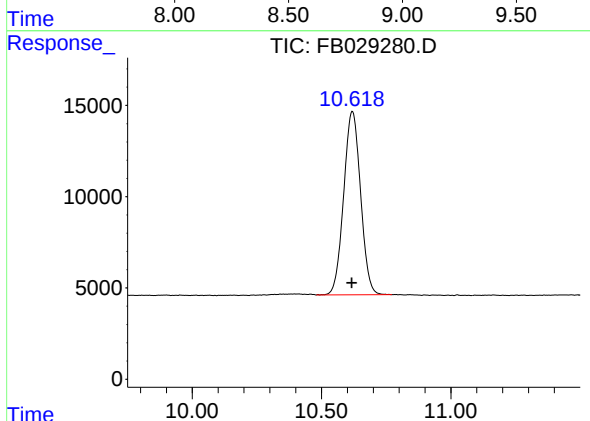


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.002 min
Response: 456628
Conc: 22.53 ng/ml

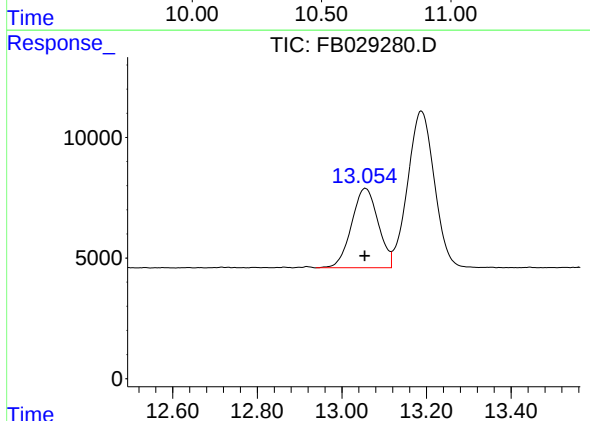


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.002 min
Response: 143312
Conc: 7.51 ng/ml

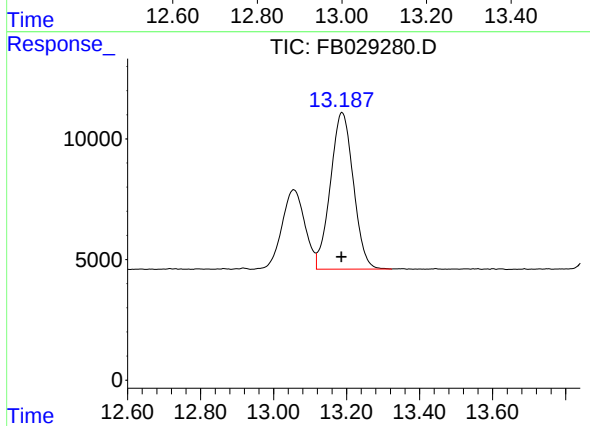

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: 0.002 min
Response: 283824
Conc: 14.97 ng/ml

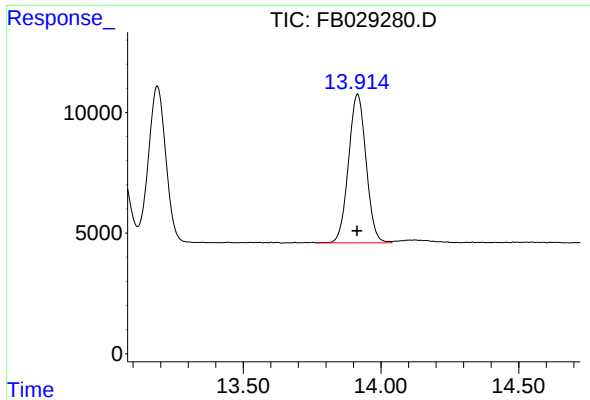

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: 0.003 min
Response: 273400
Conc: 14.98 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0210S1

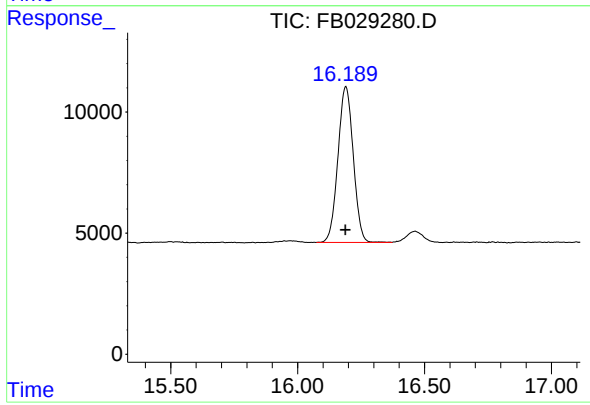

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: 0.002 min
Response: 270084
Conc: 14.35 ng/ml