

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021122\
 Data File : FB026612.D
 Signal(s) : FID2B.CH
 Acq On : 11 Feb 2022 9:21
 Operator : AJ/MA
 Sample : 5 GRO STD
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 5 GRO STD

Integration File: Calibration.e
 Quant Time: Feb 11 12:13:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021122.M
 Quant Title :
 QLast Update : Fri Feb 11 12:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	56828	4.707 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	132629	7.268 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	145370	7.158 ng/ml
3) t n-Heptane	7.743	47426	2.315 ng/ml
4) t Benzene	7.881	55836	2.374 ng/ml
6) t Toluene	10.612	161292	7.240 ng/ml
7) t Ethylbenzene	13.050	49470	2.406 ng/ml
8) t m-Xylene	13.182	99911	4.873 ng/ml
9) t O-Xylene	13.908	97081	4.912 ng/ml
10) t 1,2,4-Trimethylbenzene	16.184	104054	5.283 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021122\
Data File : FB026612.D
Signal(s) : FID2B.CH
Acq On : 11 Feb 2022 9:21
Operator : AJ/MA
Sample : 5 GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
5 GRO STD

Integration File: Calibration.e
Quant Time: Feb 11 12:13:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021122.M
Quant Title :
QLast Update : Fri Feb 11 12:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

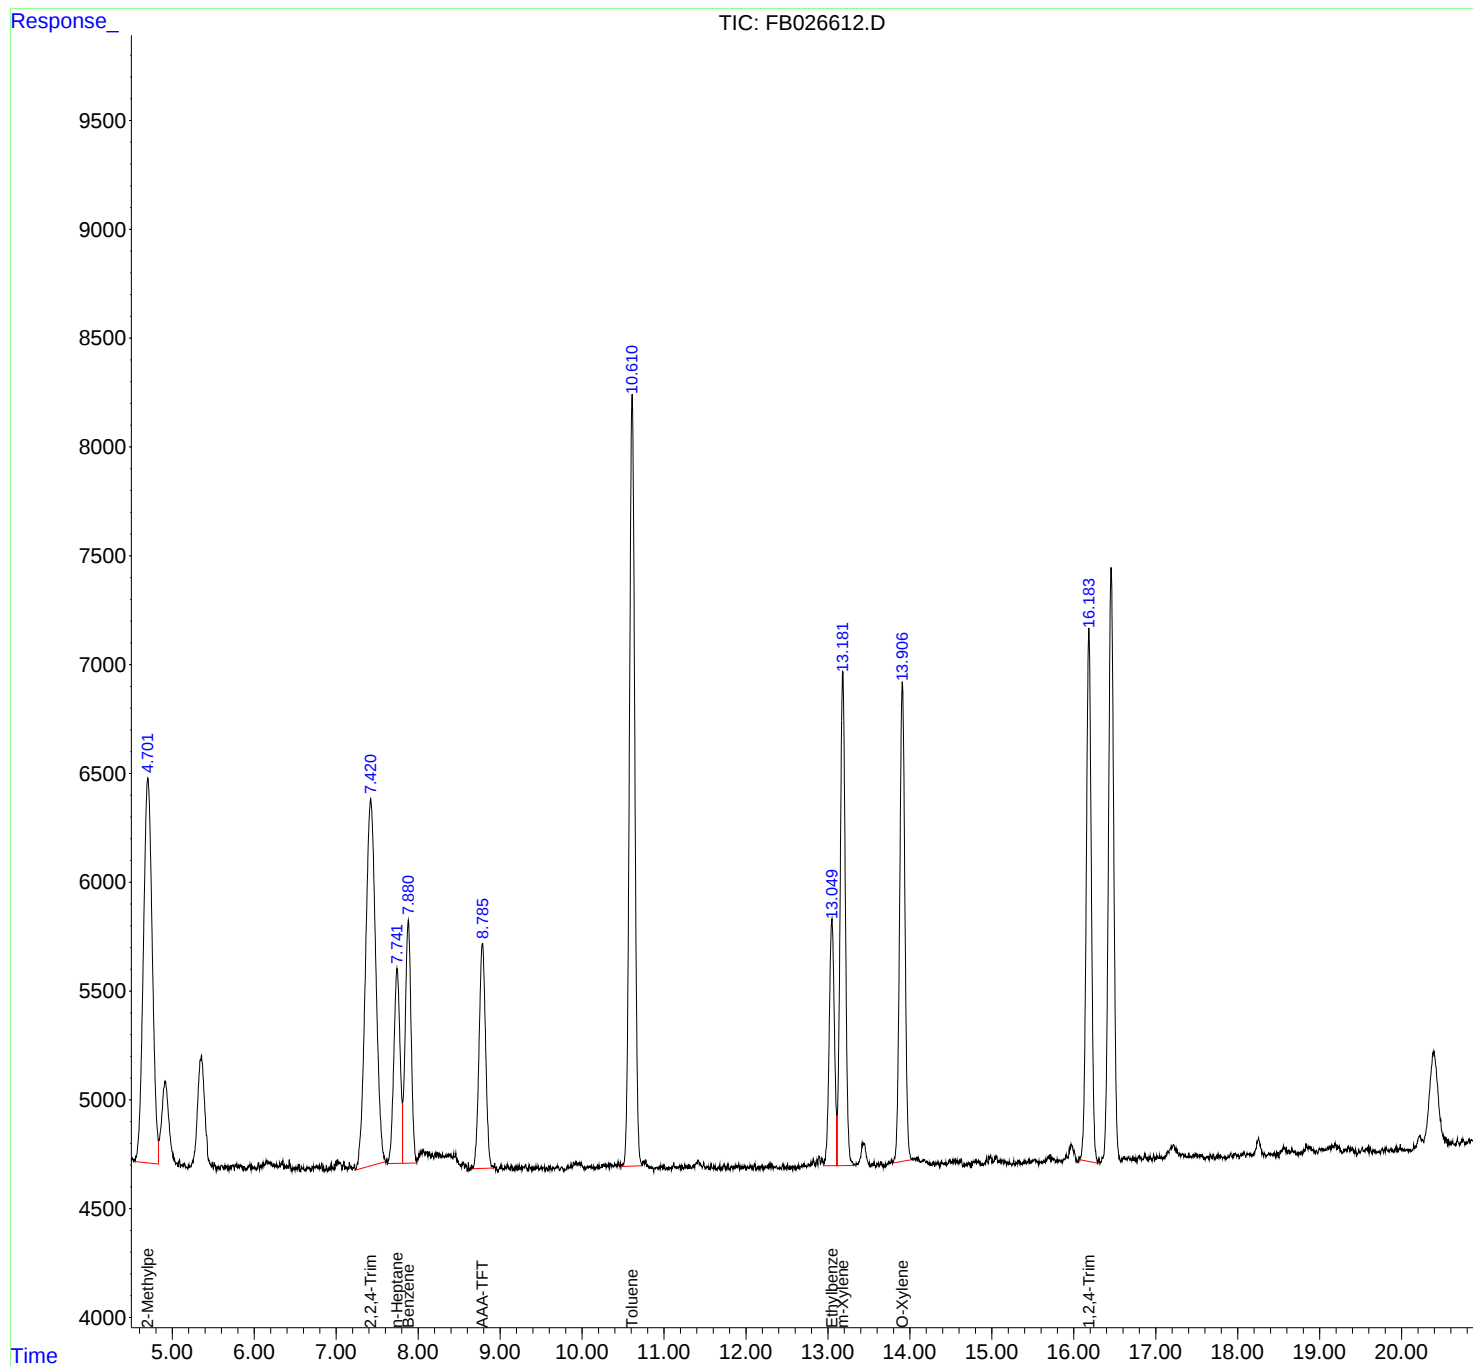


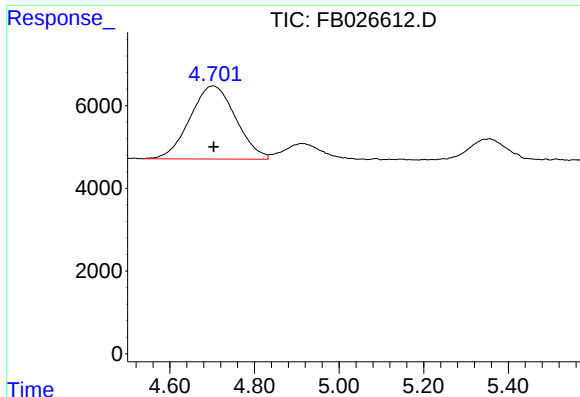

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: -0.001 min
Response: 132629
Conc: 7.27 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

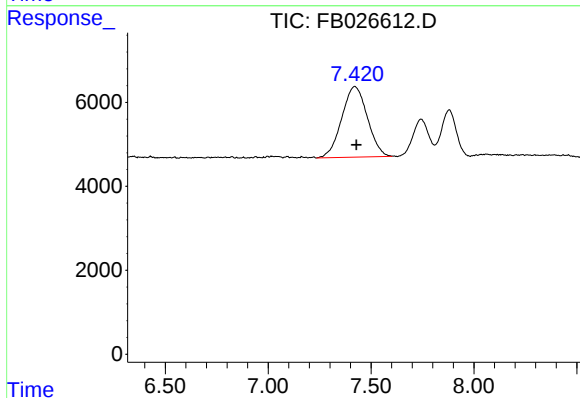


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: -0.007 min
Response: 145370
Conc: 7.16 ng/ml

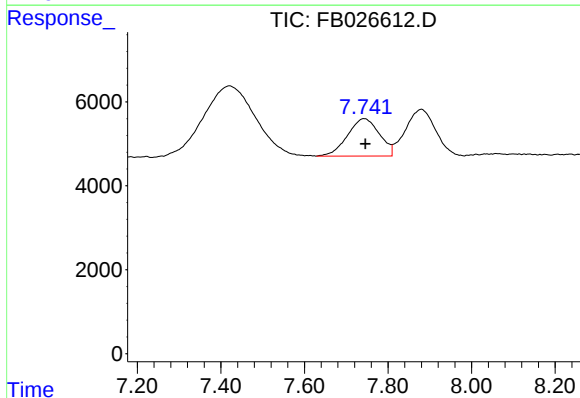


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: -0.004 min
Response: 47426
Conc: 2.32 ng/ml

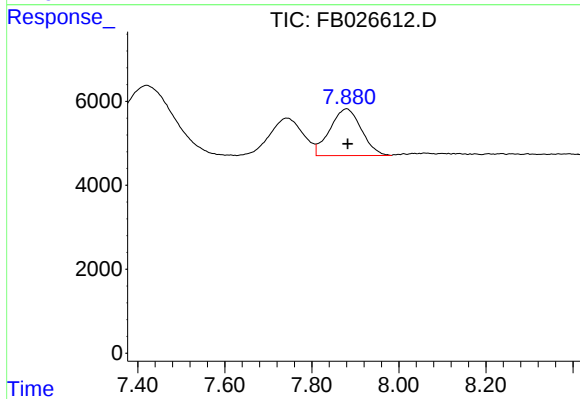

#4 Benzene


R.T.: 7.881 min
Delta R.T.: -0.001 min
Response: 55836
Conc: 2.37 ng/ml

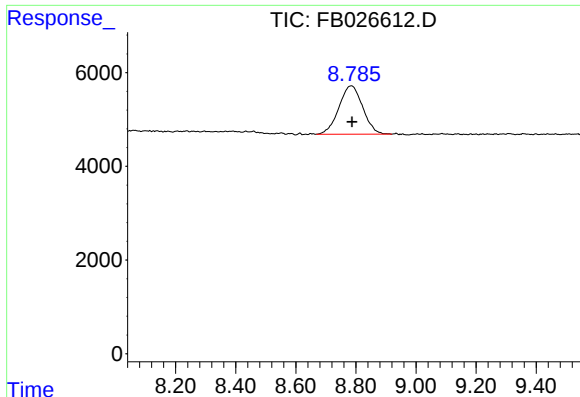

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: 0.000 min
Response: 56828
Conc: 4.71 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

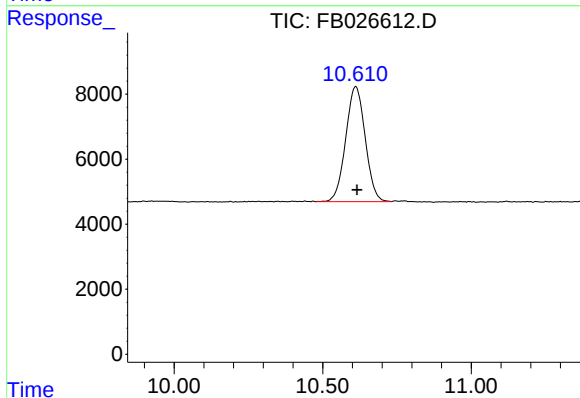


#6 Toluene

R.T.: 10.612 min
Delta R.T.: -0.003 min
Response: 161292
Conc: 7.24 ng/ml

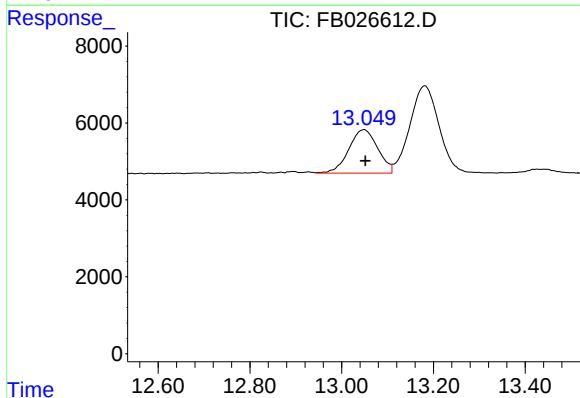


#7 Ethylbenzene

R.T.: 13.050 min
Delta R.T.: -0.002 min
Response: 49470
Conc: 2.41 ng/ml

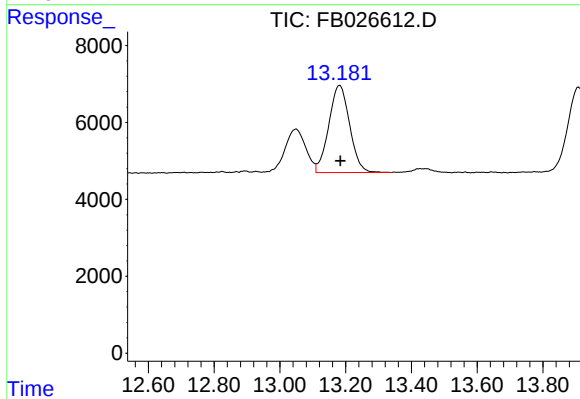

#8 m-Xylene


R.T.: 13.182 min
Delta R.T.: -0.002 min
Response: 99911
Conc: 4.87 ng/ml

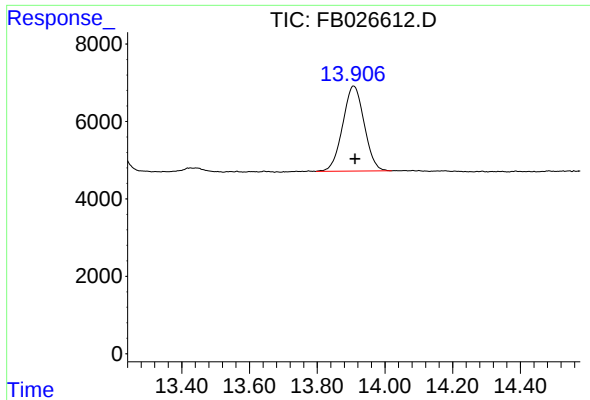

#9 O-Xylene

R.T.: 13.908 min
Delta R.T.: -0.003 min
Response: 97081
Conc: 4.91 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

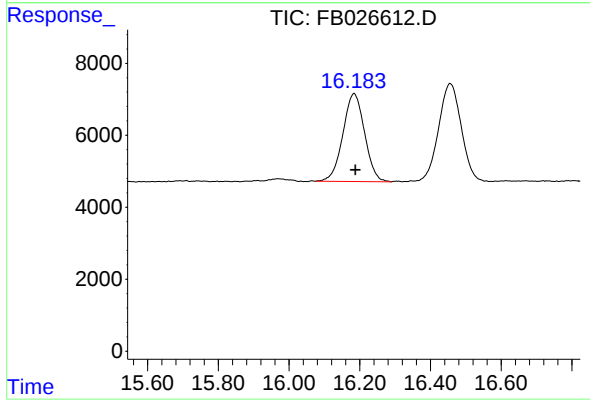

#10 1,2,4-Trimethylbenzene

R.T.: 16.184 min
Delta R.T.: -0.003 min
Response: 104054
Conc: 5.28 ng/ml