

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021122\
 Data File : FB026615.D
 Signal(s) : FID2B.CH
 Acq On : 11 Feb 2022 11:14
 Operator : AJ/MA
 Sample : 50 GRO STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 50 GRO STD

Integration File: Calibration.e
 Quant Time: Feb 11 12:13:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021122.M
 Quant Title :
 QLast Update : Fri Feb 11 12:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	587820	48.688 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	1359984	74.522 ng/ml
2) t 2,2,4-Trimethylpentane	7.433	1543623	76.012 ng/ml
3) t n-Heptane	7.745	504777	24.644 ng/ml
4) t Benzene	7.883	588494	25.017 ng/ml
6) t Toluene	10.615	1667421	74.850 ng/ml
7) t Ethylbenzene	13.053	508957	24.758 ng/ml
8) t m-Xylene	13.185	1012503	49.379 ng/ml
9) t O-Xylene	13.913	980528	49.616 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	971735	49.339 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021122\
Data File : FB026615.D
Signal(s) : FID2B.CH
Acq On : 11 Feb 2022 11:14
Operator : AJ/MA
Sample : 50 GRO STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
50 GRO STD

Integration File: Calibration.e
Quant Time: Feb 11 12:13:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021122.M
Quant Title :
QLast Update : Fri Feb 11 12:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

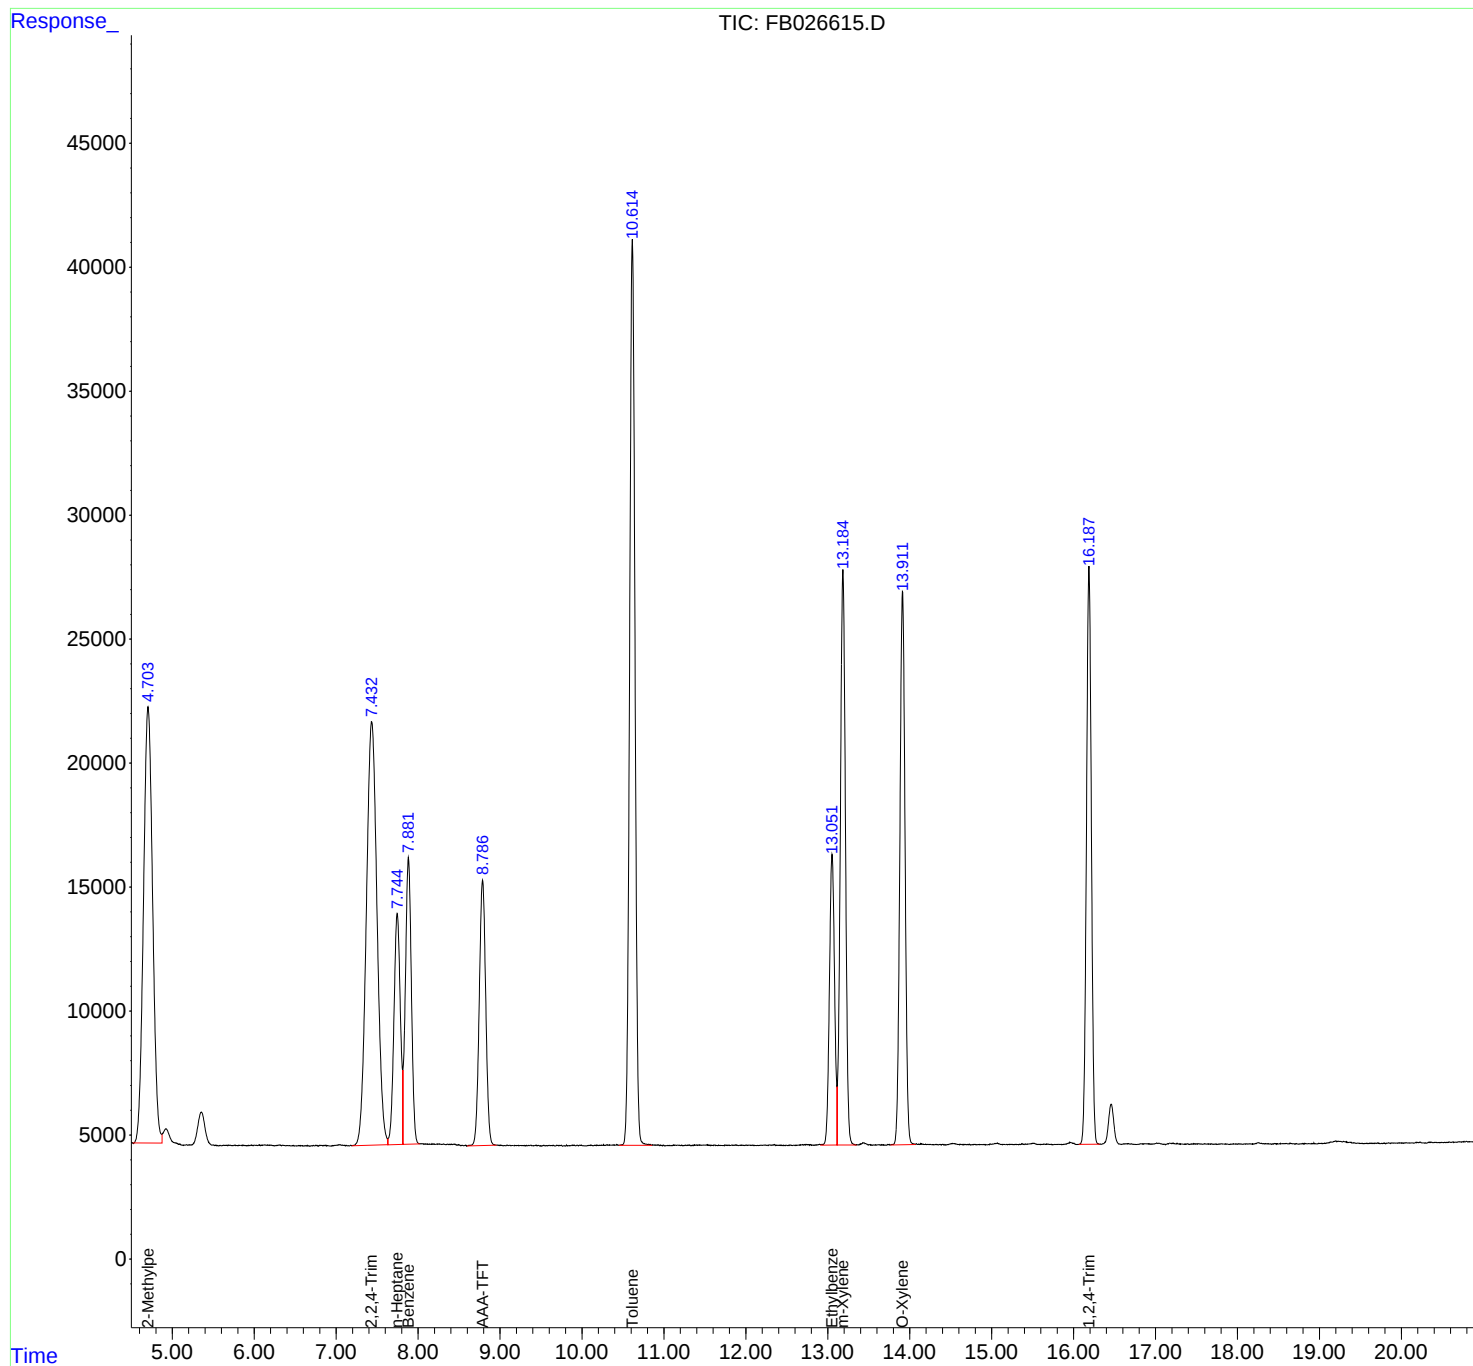


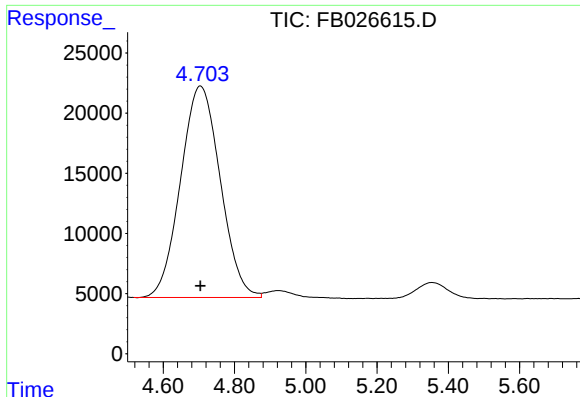

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: 0.000 min
Response: 1359984
Conc: 74.52 ng/ml

Instrument :
FID_B
ClientSampleId :
50 GRO STD

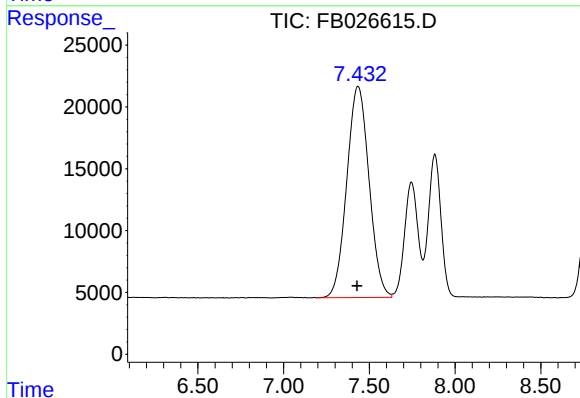


#2 2,2,4-Trimethylpentane

R.T.: 7.433 min
Delta R.T.: 0.005 min
Response: 1543623
Conc: 76.01 ng/ml

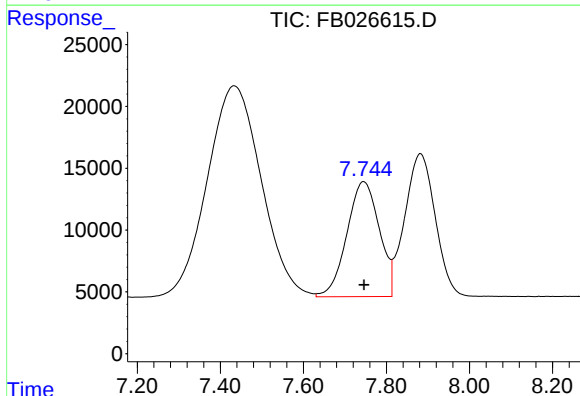


#3 n-Heptane

R.T.: 7.745 min
Delta R.T.: 0.000 min
Response: 504777
Conc: 24.64 ng/ml

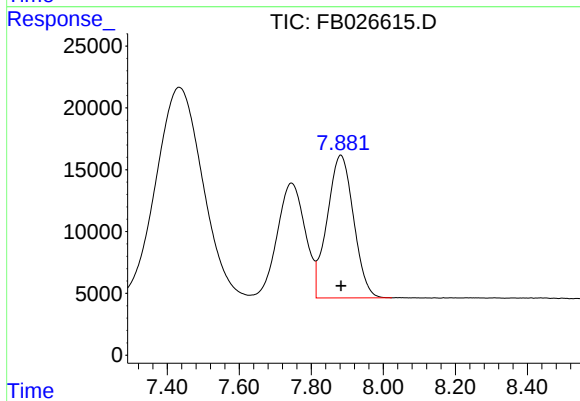

#4 Benzene


R.T.: 7.883 min
Delta R.T.: 0.000 min
Response: 588494
Conc: 25.02 ng/ml

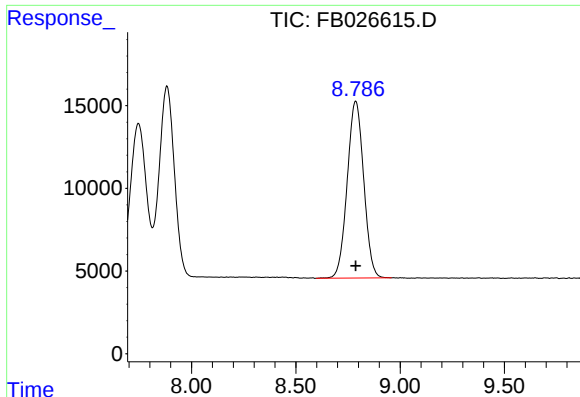

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: 0.000 min
Response: 587820
Conc: 48.69 ng/ml

Instrument :
FID_B
ClientSampleId :
50 GRO STD

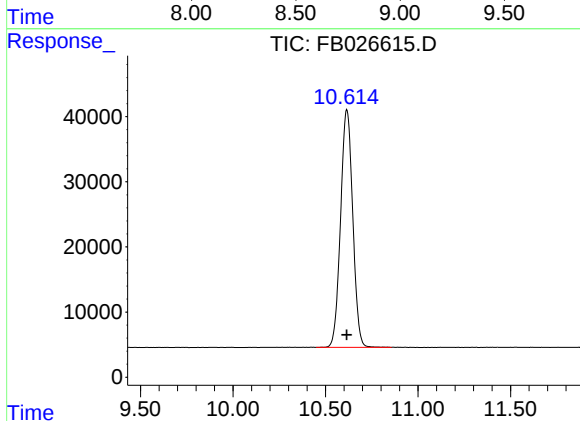


#6 Toluene

R.T.: 10.615 min
Delta R.T.: 0.000 min
Response: 1667421
Conc: 74.85 ng/ml

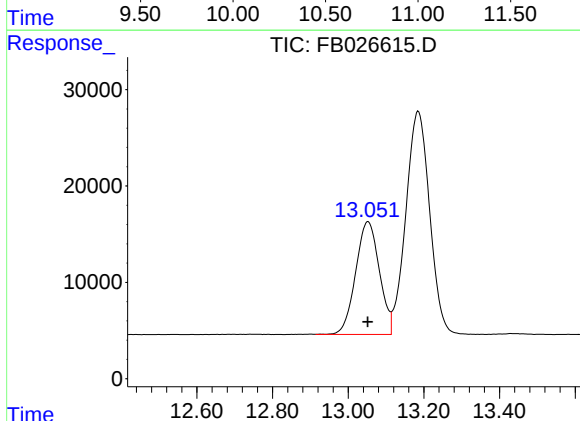


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: 0.000 min
Response: 508957
Conc: 24.76 ng/ml

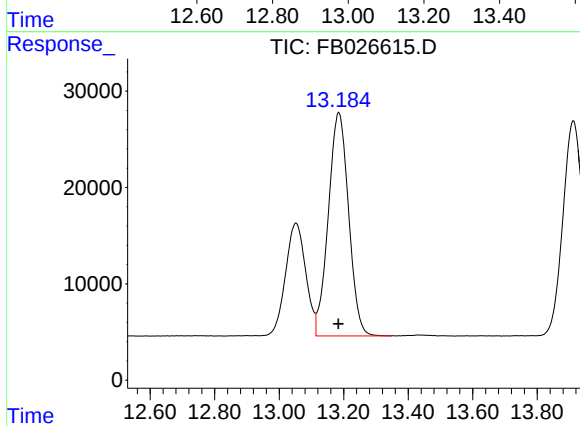

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: 0.001 min
Response: 1012503
Conc: 49.38 ng/ml

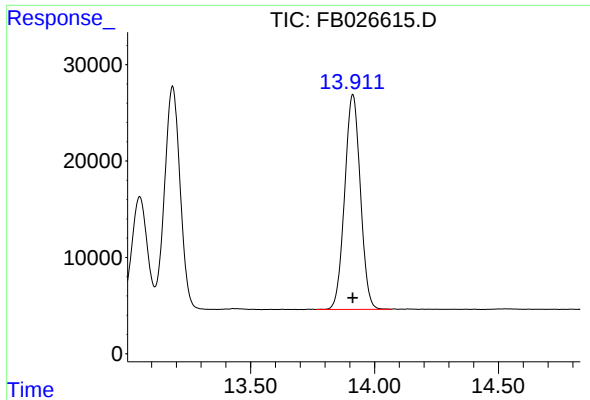

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: 0.001 min
Response: 980528
Conc: 49.62 ng/ml

Instrument :
FID_B
ClientSampleId :
50 GRO STD

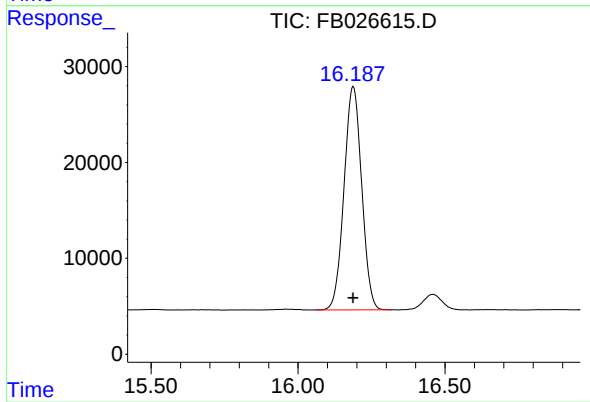

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: 0.000 min
Response: 971735
Conc: 49.34 ng/ml