

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021219\
 Data File : FB019722.D
 Signal(s) : FID2B.CH
 Acq On : 12 Feb 2019 13:51
 Operator : MJ/SJ
 Sample : K1345-01MS
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 13 00:46:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.043	215946	18.473 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.897	542451	31.332 ng/ml
2) t 2,2,4-Trimethylpentane	7.657	476763	28.749 ng/ml
3) t n-Heptane	7.997	149459	9.275 ng/ml
4) t Benzene	8.135	205840	10.913 ng/ml
6) t Toluene	10.890	498919	28.522 ng/ml
7) t Ethylbenzene	13.342	196939	8.974 ng/ml
8) t m-Xylene	13.475	408770	17.860 ng/ml
9) t O-Xylene	14.207	406749	18.211 ng/ml
10) t 1,2,4-Trimethylbenzene	16.493	396372	17.107 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021219\
Data File : FB019722.D
Signal(s) : FID2B.CH
Acq On : 12 Feb 2019 13:51
Operator : MJ/SJ
Sample : K1345-01MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 13 00:46:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

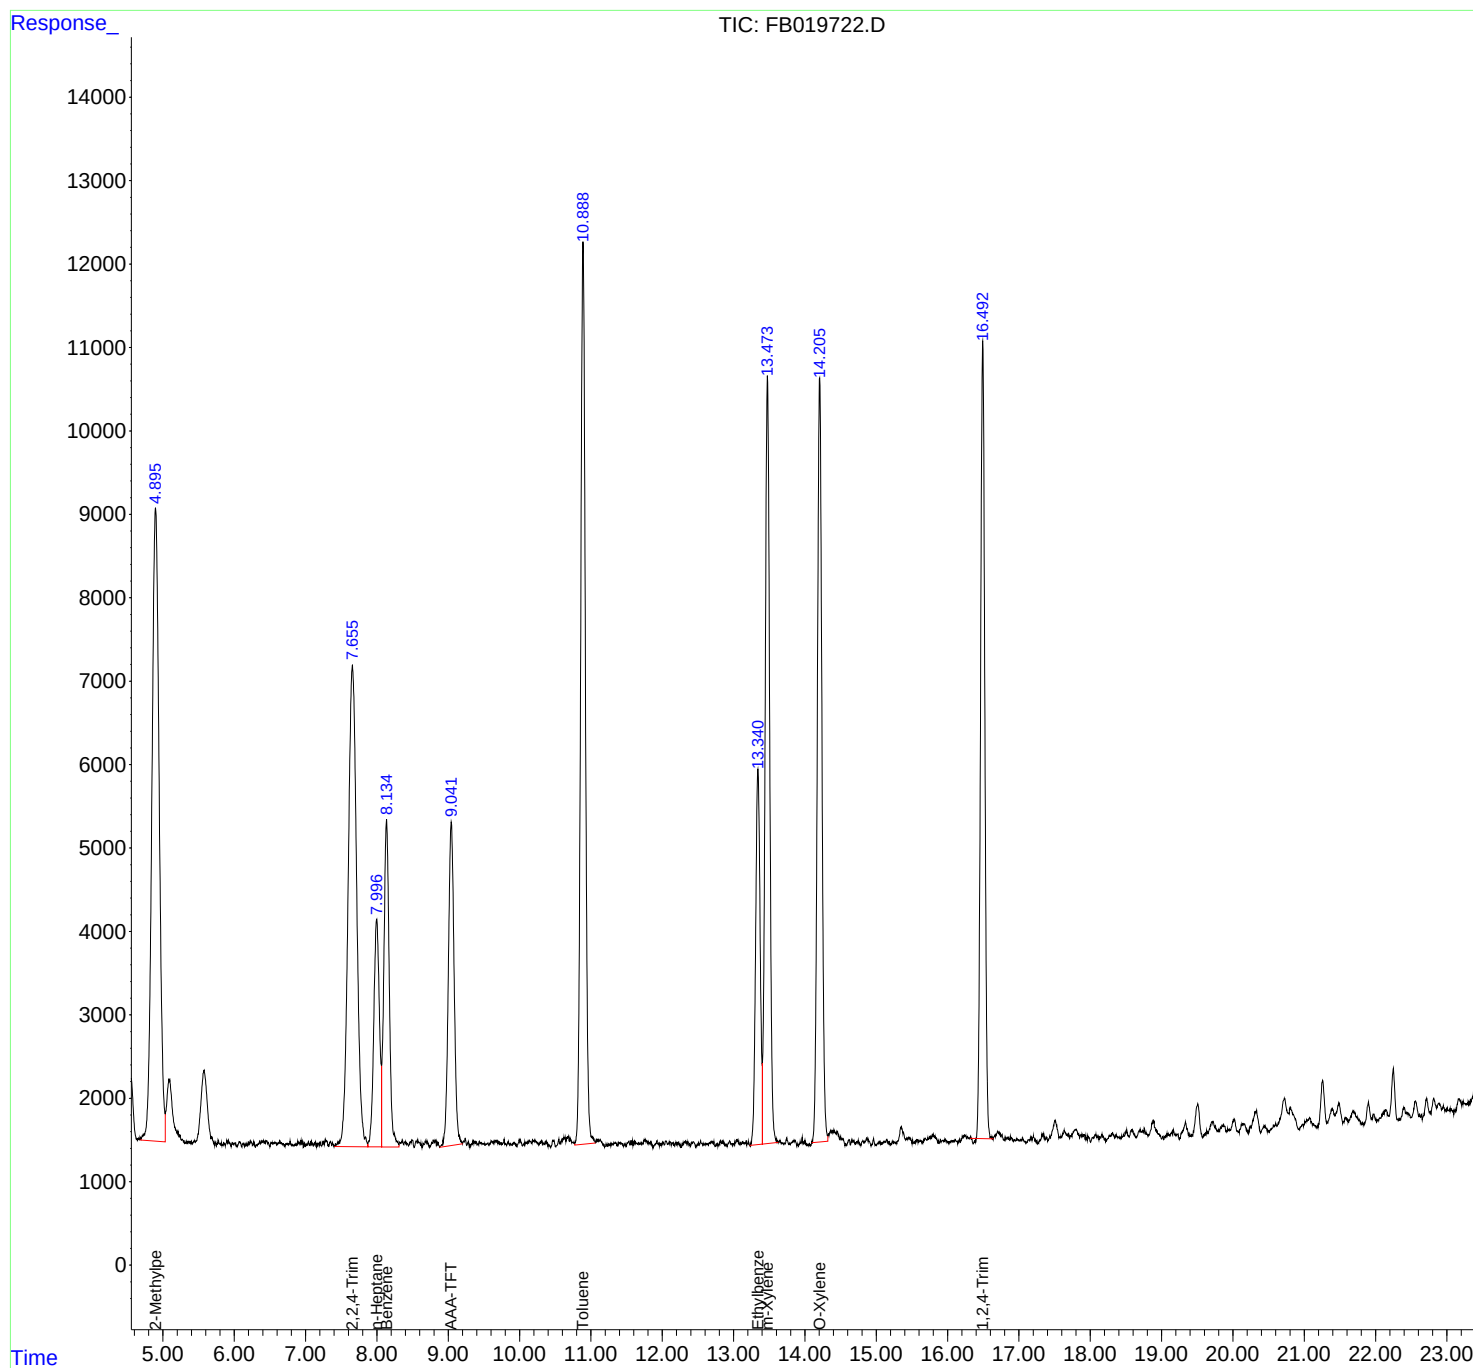

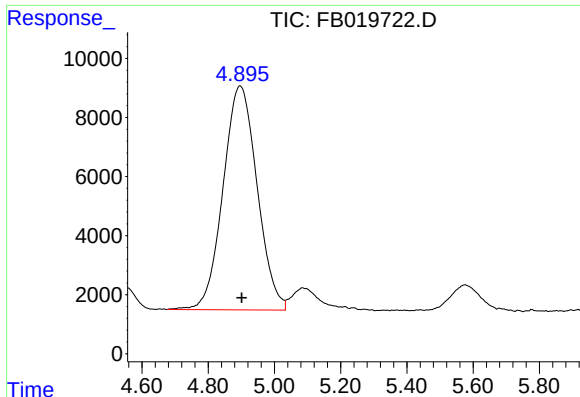


#1 2-Methylpentane

R.T.: 4.897 min
Delta R.T.: -0.005 min
Response: 542451
Conc: 31.33 ng/ml

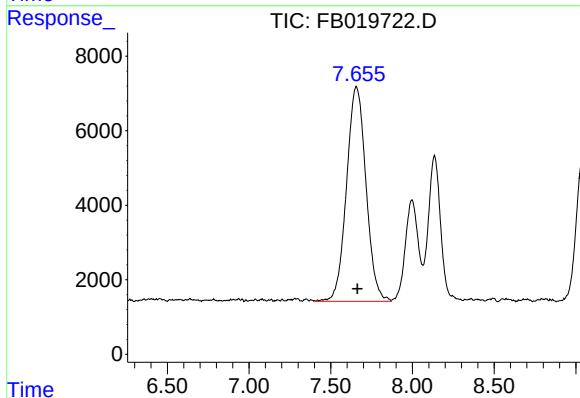


#2 2,2,4-Trimethylpentane

R.T.: 7.657 min
Delta R.T.: -0.008 min
Response: 476763
Conc: 28.75 ng/ml

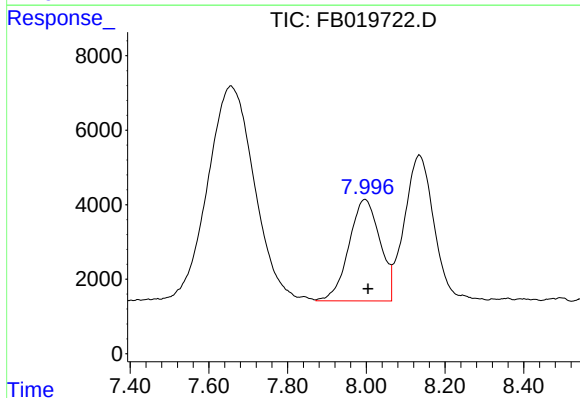


#3 n-Heptane

R.T.: 7.997 min
Delta R.T.: -0.008 min
Response: 149459
Conc: 9.27 ng/ml

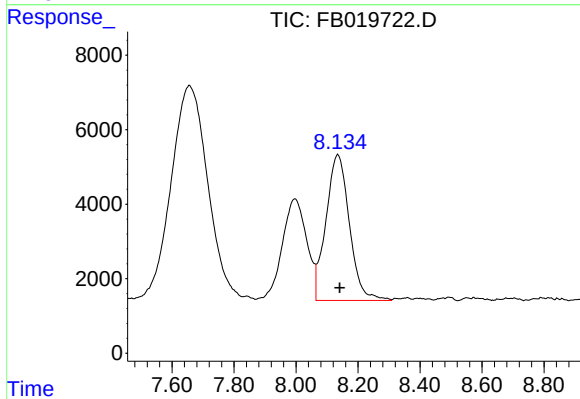


#4 Benzene

R.T.: 8.135 min
Delta R.T.: -0.006 min
Response: 205840
Conc: 10.91 ng/ml

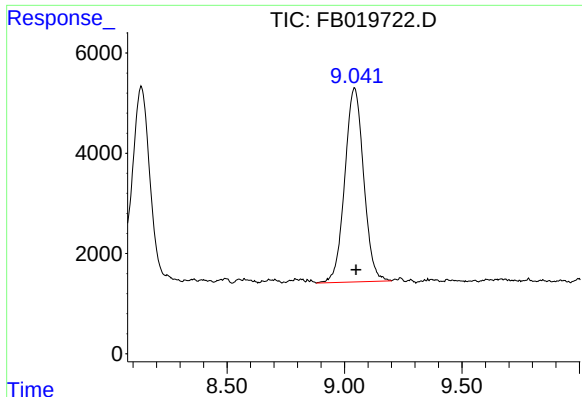


#5 AAA-TFT

R.T.: 9.043 min
Delta R.T.: -0.007 min
Response: 215946
Conc: 18.47 ng/ml

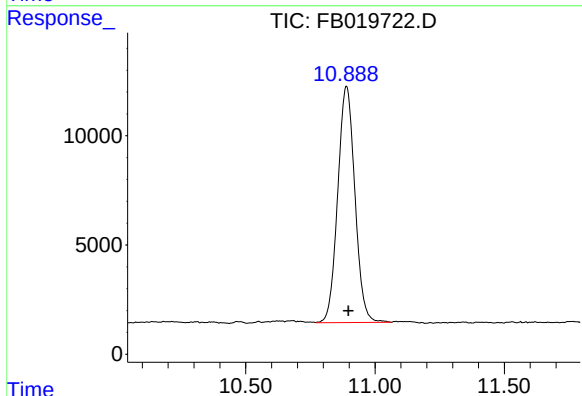


#6 Toluene

R.T.: 10.890 min
Delta R.T.: -0.007 min
Response: 498919
Conc: 28.52 ng/ml

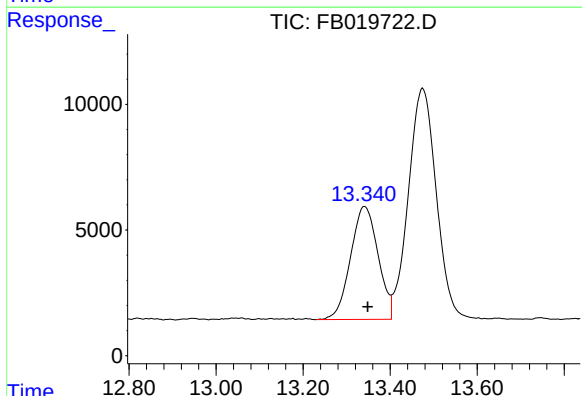


#7 Ethylbenzene

R.T.: 13.342 min
Delta R.T.: -0.007 min
Response: 196939
Conc: 8.97 ng/ml

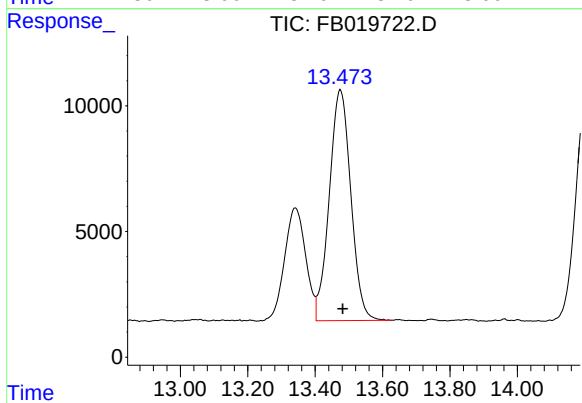

#8 m-Xylene

R.T.: 13.475 min
Delta R.T.: -0.007 min
Response: 408770
Conc: 17.86 ng/ml

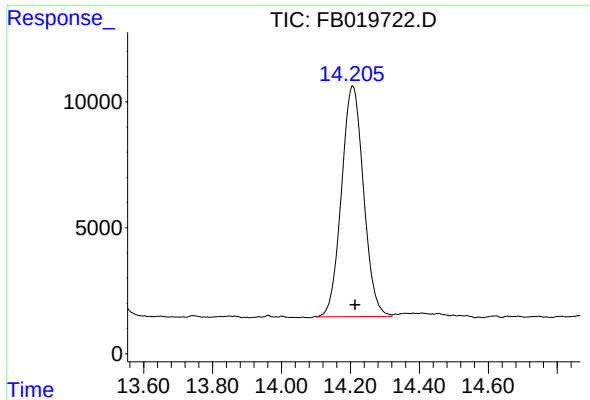


#9 O-Xylene

R.T.: 14.207 min

Delta R.T.: -0.007 min

Response: 406749

Conc: 18.21 ng/ml

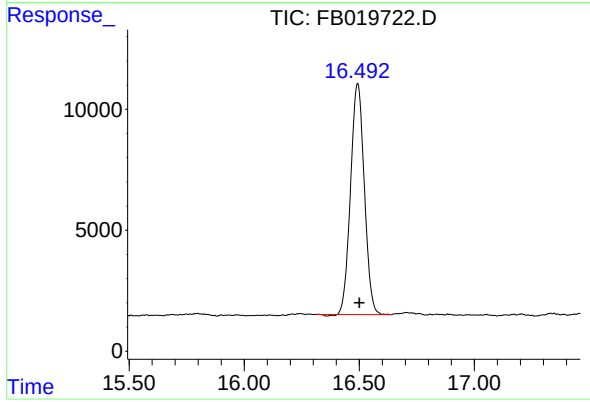

#10 1,2,4-Trimethylbenzene

R.T.: 16.493 min

Delta R.T.: -0.007 min

Response: 396372

Conc: 17.11 ng/ml