

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021319\
 Data File : FB019737.D
 Signal(s) : FID2B.CH
 Acq On : 13 Feb 2019 9:39
 Operator : MJ/SJ
 Sample : BSF0213S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 14 01:25:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.045	209939	17.959 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.899	564813	32.624 ng/ml
2) t 2,2,4-Trimethylpentane	7.659	555015	33.468 ng/ml
3) t n-Heptane	8.000	170720	10.594 ng/ml
4) t Benzene	8.138	186554	9.891 ng/ml
6) t Toluene	10.893	503668	28.793 ng/ml
7) t Ethylbenzene	13.345	203313	9.264 ng/ml
8) t m-Xylene	13.479	423633	18.509 ng/ml
9) t O-Xylene	14.210	425003	19.029 ng/ml
10) t 1,2,4-Trimethylbenzene	16.497	431037	18.603 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021319\
Data File : FB019737.D
Signal(s) : FID2B.CH
Acq On : 13 Feb 2019 9:39
Operator : MJ/SJ
Sample : BSF0213S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 14 01:25:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

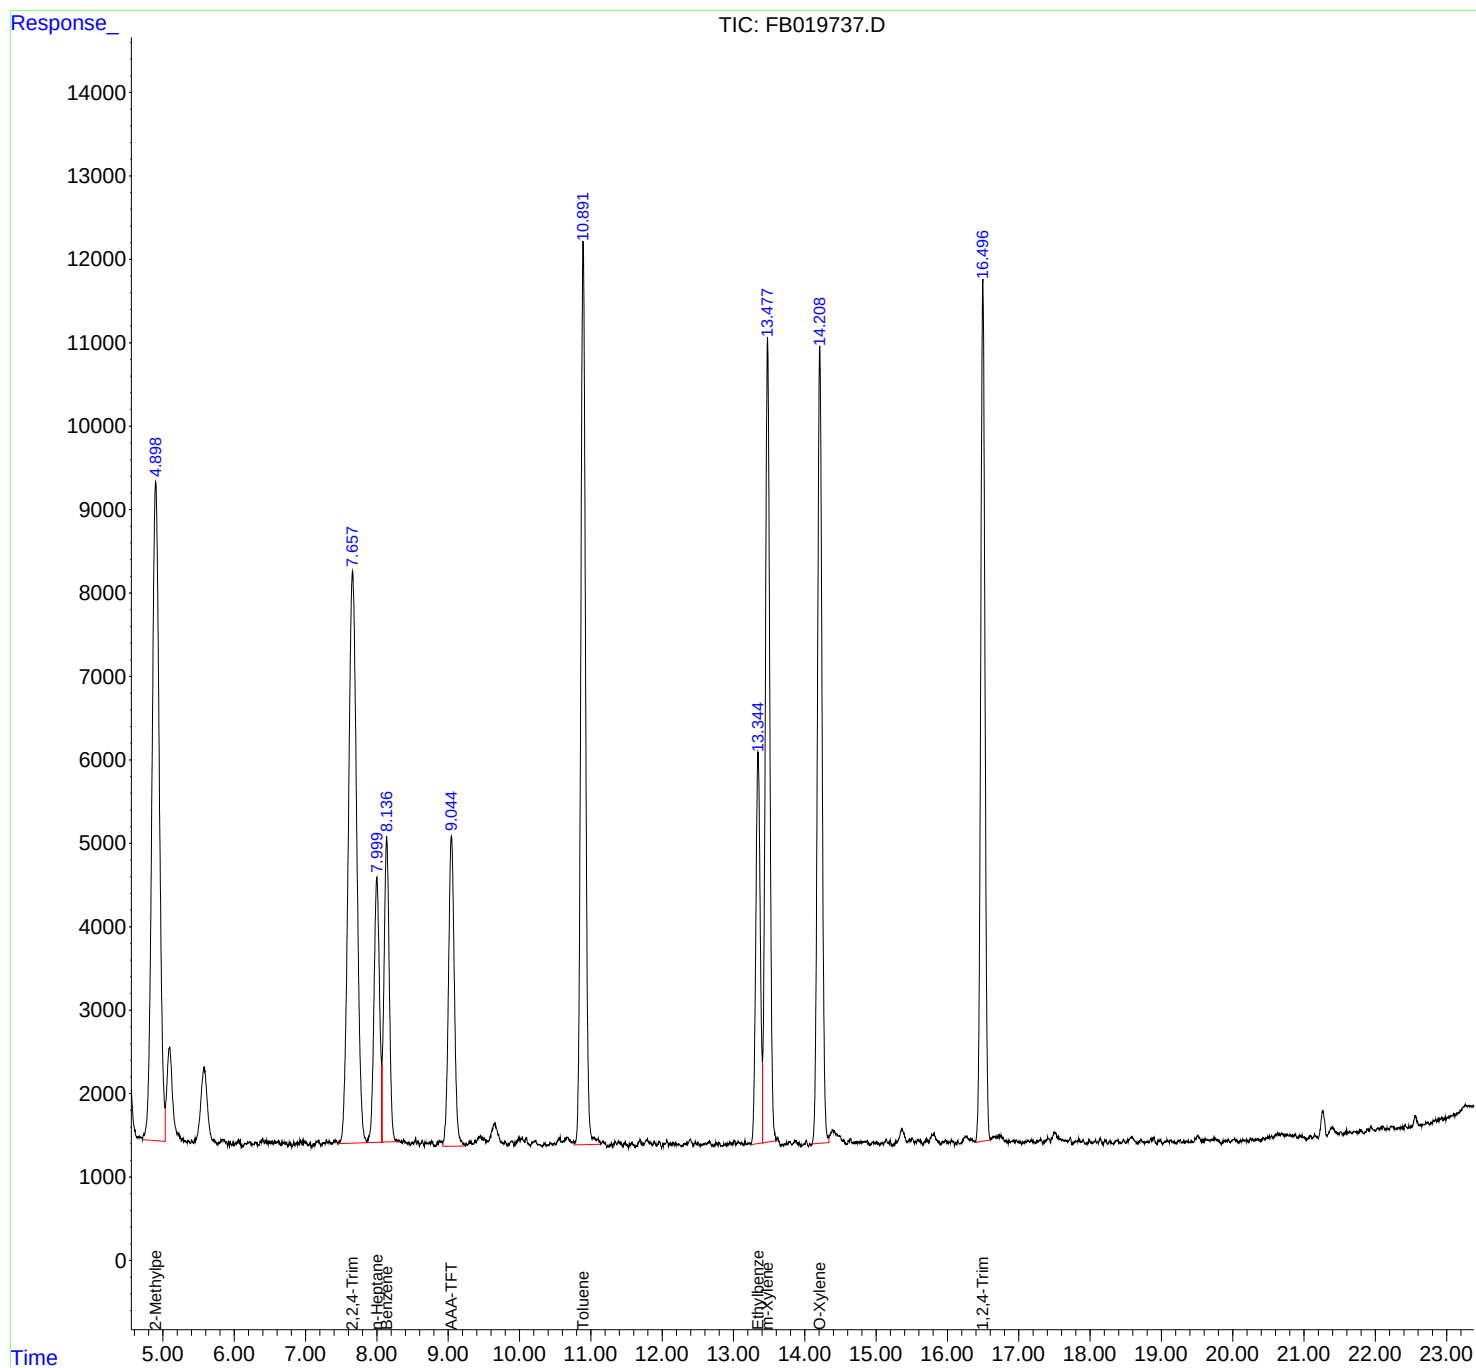

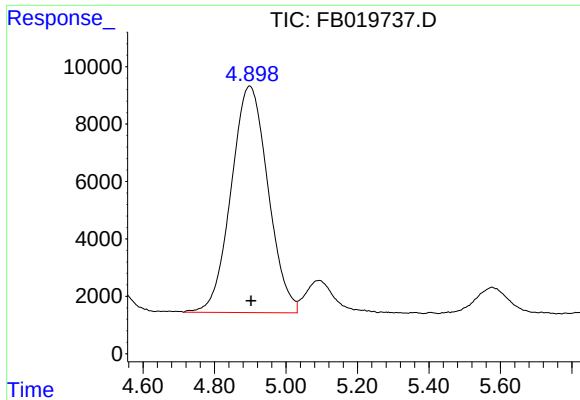


#1 2-Methylpentane

R.T.: 4.899 min
Delta R.T.: -0.003 min
Response: 564813
Conc: 32.62 ng/ml

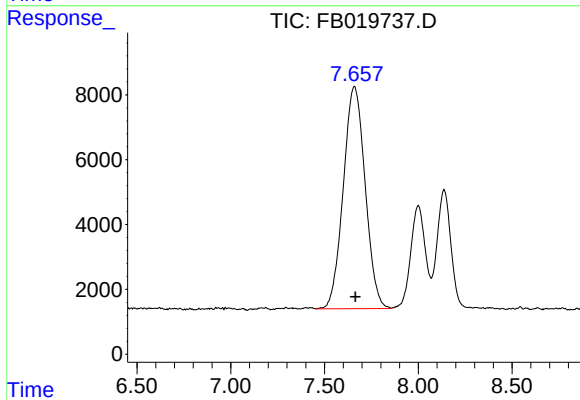


#2 2,2,4-Trimethylpentane

R.T.: 7.659 min
Delta R.T.: -0.005 min
Response: 555015
Conc: 33.47 ng/ml

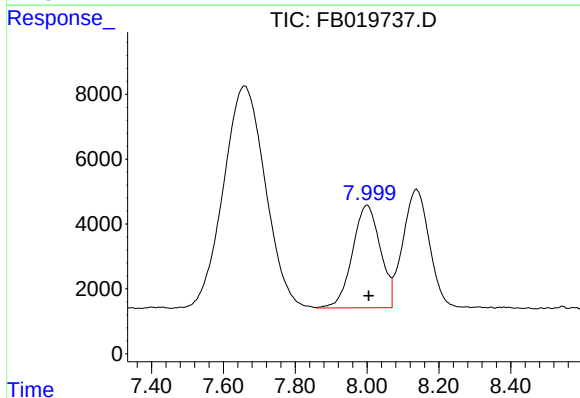


#3 n-Heptane

R.T.: 8.000 min
Delta R.T.: -0.005 min
Response: 170720
Conc: 10.59 ng/ml

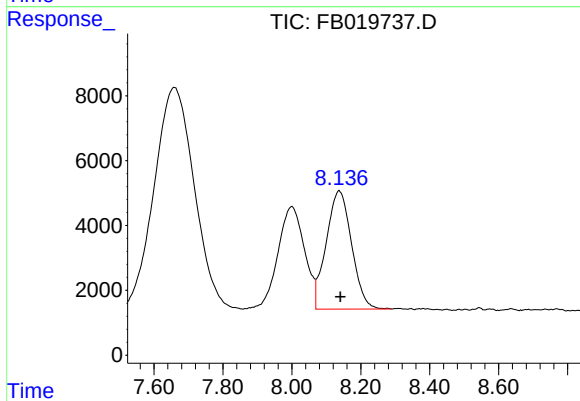


#4 Benzene

R.T.: 8.138 min
Delta R.T.: -0.003 min
Response: 186554
Conc: 9.89 ng/ml

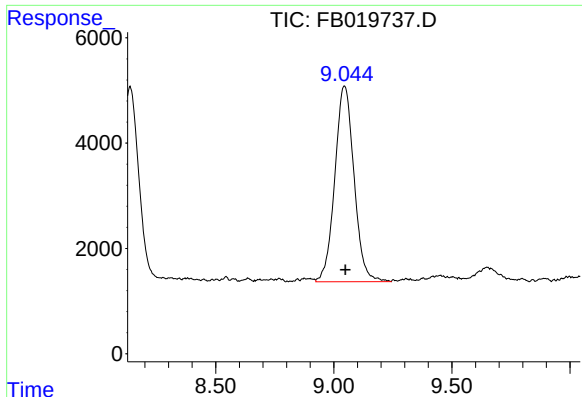


#5 AAA-TFT

R.T.: 9.045 min
Delta R.T.: -0.004 min
Response: 209939
Conc: 17.96 ng/ml

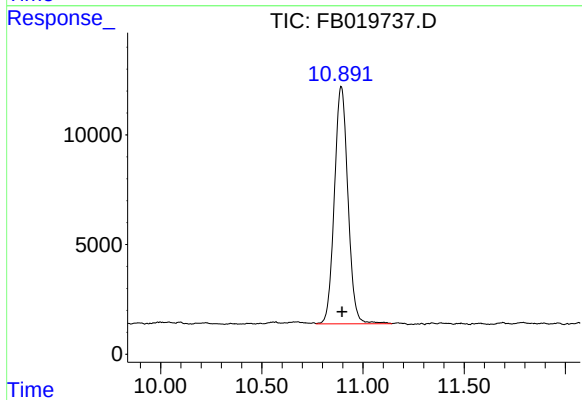


#6 Toluene

R.T.: 10.893 min
Delta R.T.: -0.004 min
Response: 503668
Conc: 28.79 ng/ml

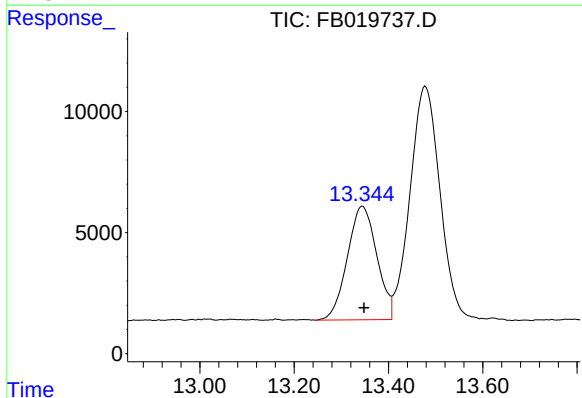


#7 Ethylbenzene

R.T.: 13.345 min
Delta R.T.: -0.004 min
Response: 203313
Conc: 9.26 ng/ml

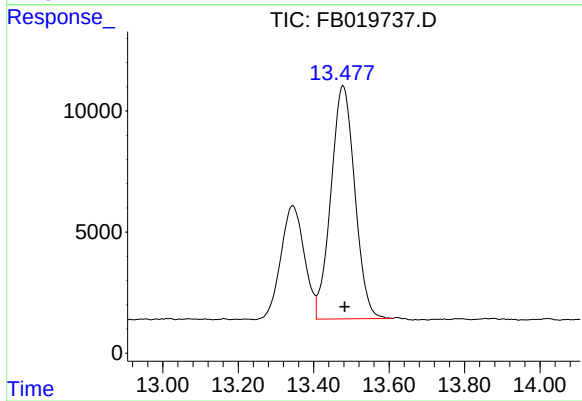


#8 m-Xylene

R.T.: 13.479 min
Delta R.T.: -0.004 min
Response: 423633
Conc: 18.51 ng/ml

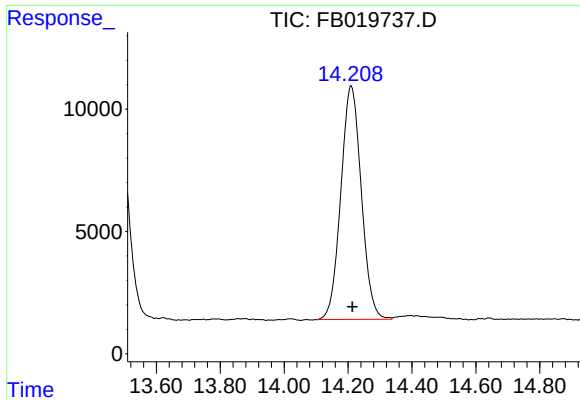

#9 O-Xylene

R.T.: 14.210 min
Delta R.T.: -0.004 min
Response: 425003
Conc: 19.03 ng/ml

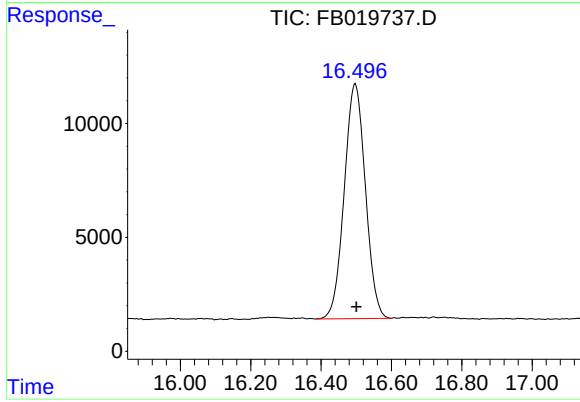

#10 1,2,4-Trimethylbenzene

R.T.: 16.497 min
Delta R.T.: -0.003 min
Response: 431037
Conc: 18.60 ng/ml