

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021319\
Data File : FB019744.D
Signal(s) : FID2B.CH
Acq On : 13 Feb 2019 14:45
Operator : MJ/SJ
Sample : K1462-01MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 14 01:26:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.046	221443	18.944 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.897	565683	32.674 ng/ml
2) t	2,2,4-Trimethylpentane	7.659	554847	33.458 ng/ml
3) t	n-Heptane	7.999	169445	10.515 ng/ml
4) t	Benzene	8.139	195664	10.374 ng/ml
6) t	Toluene	10.893	496871	28.405 ng/ml
7) t	Ethylbenzene	13.345	202819	9.242 ng/ml
8) t	m-Xylene	13.478	425205	18.578 ng/ml
9) t	O-Xylene	14.210	416976	18.669 ng/ml
10) t	1,2,4-Trimethylbenzene	16.497	435239	18.785 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021319\
Data File : FB019744.D
Signal(s) : FID2B.CH
Acq On : 13 Feb 2019 14:45
Operator : MJ/SJ
Sample : K1462-01MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 14 01:26:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

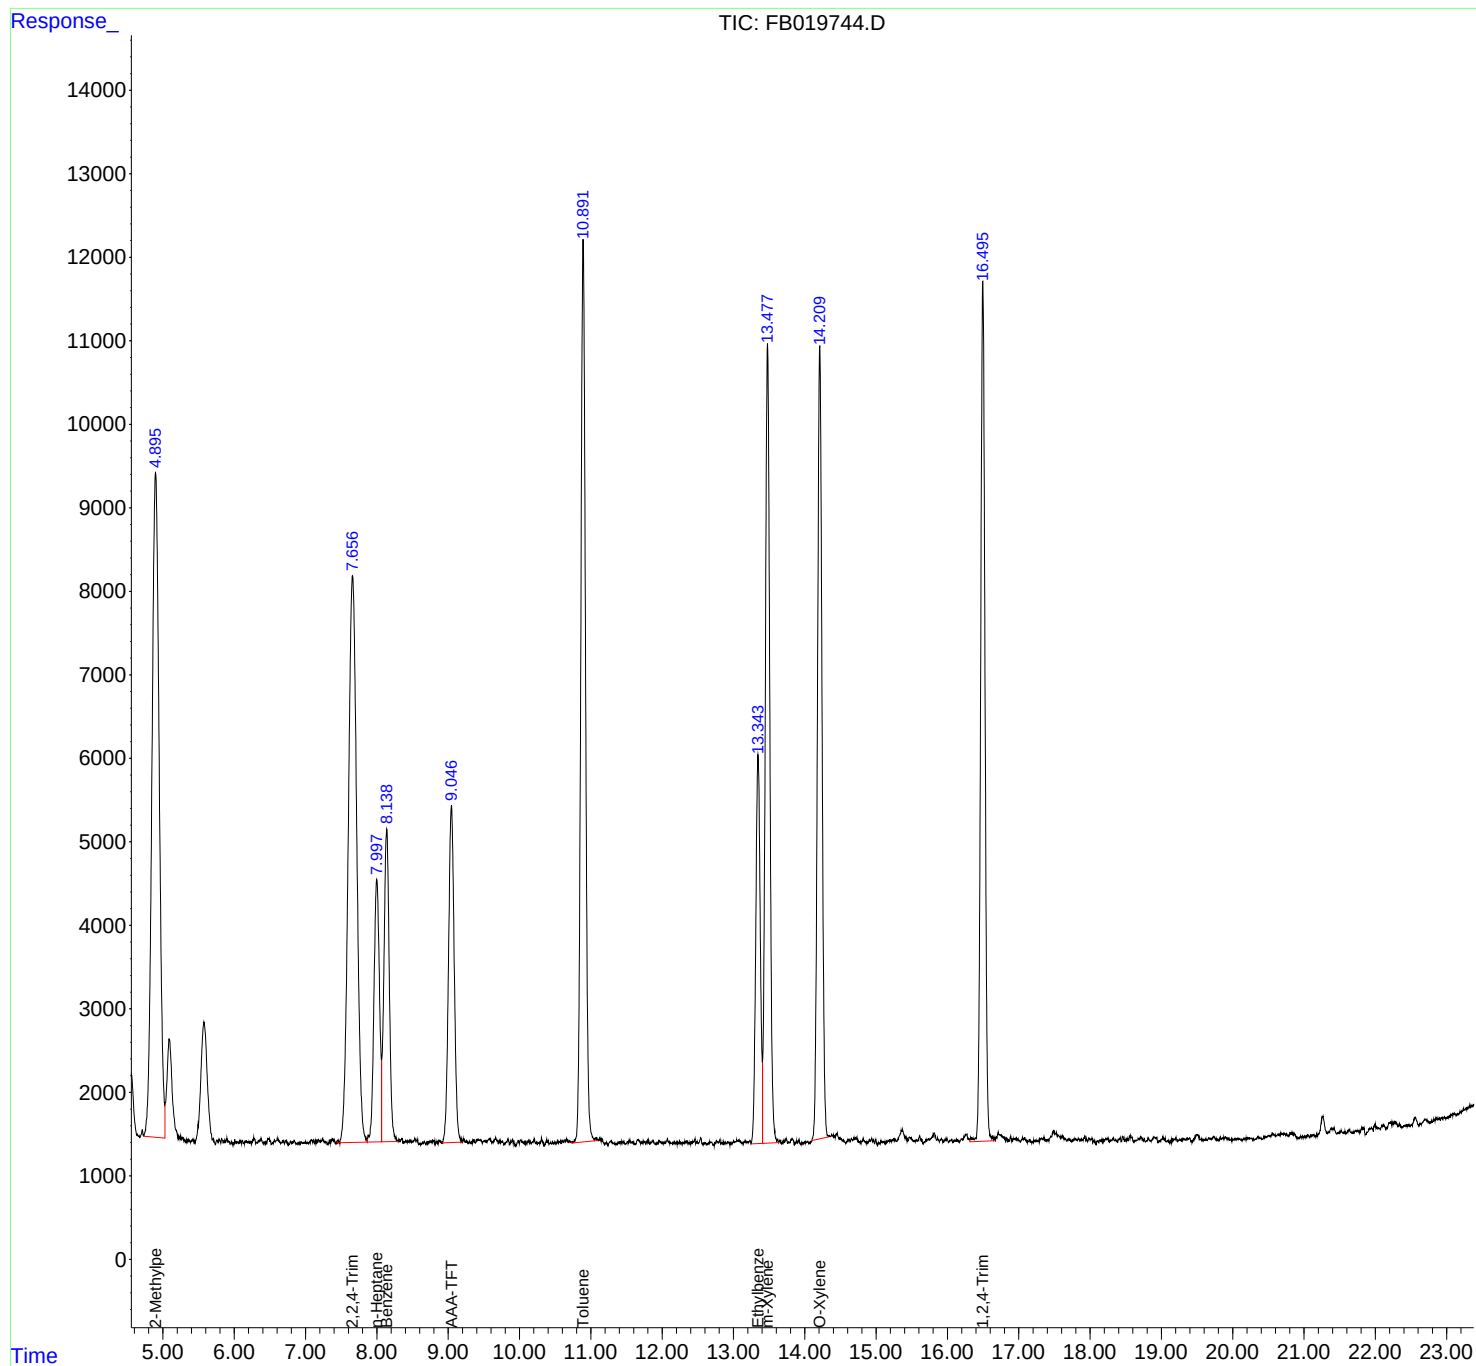

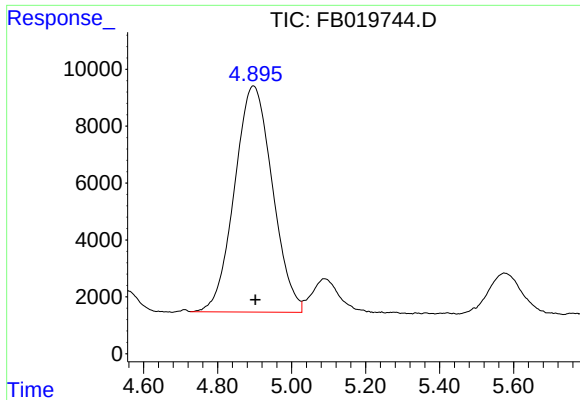


#1 2-Methylpentane

R.T.: 4.897 min
Delta R.T.: -0.005 min
Response: 565683
Conc: 32.67 ng/ml

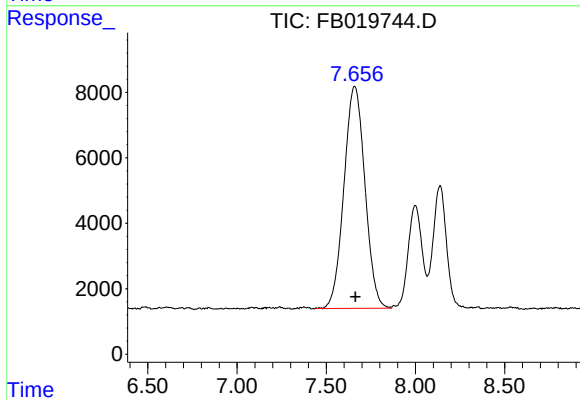


#2 2,2,4-Trimethylpentane

R.T.: 7.659 min
Delta R.T.: -0.005 min
Response: 554847
Conc: 33.46 ng/ml

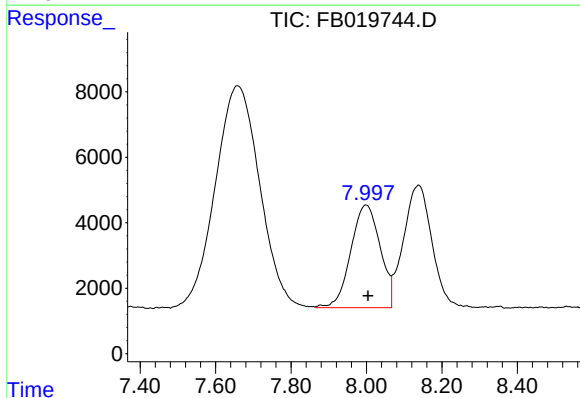


#3 n-Heptane

R.T.: 7.999 min
Delta R.T.: -0.005 min
Response: 169445
Conc: 10.51 ng/ml

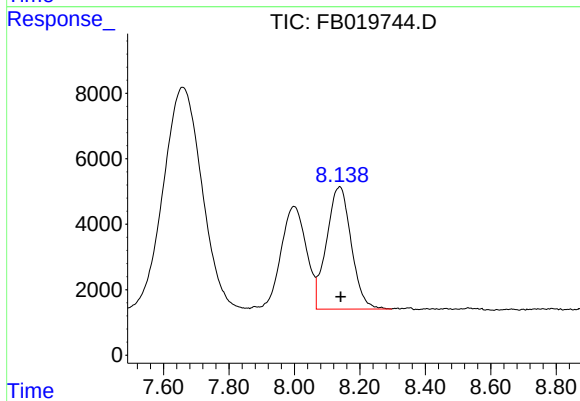


#4 Benzene

R.T.: 8.139 min
Delta R.T.: -0.003 min
Response: 195664
Conc: 10.37 ng/ml

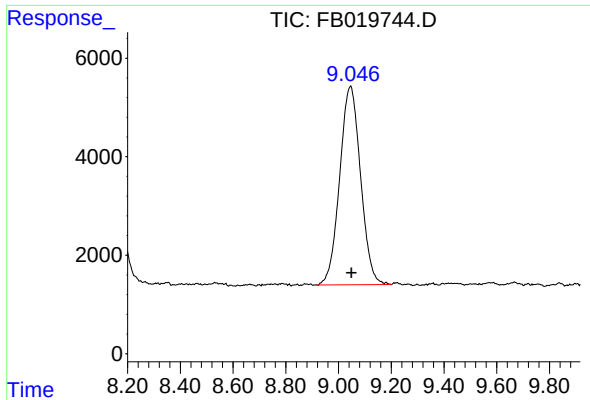


#5 AAA-TFT

R.T.: 9.046 min
Delta R.T.: -0.004 min
Response: 221443
Conc: 18.94 ng/ml

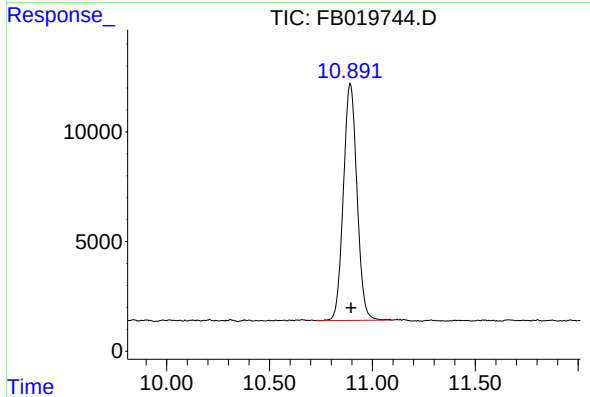


#6 Toluene

R.T.: 10.893 min
Delta R.T.: -0.004 min
Response: 496871
Conc: 28.40 ng/ml

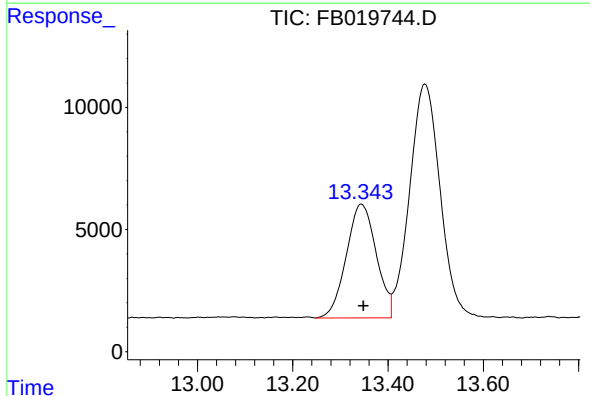


#7 Ethylbenzene

R.T.: 13.345 min
Delta R.T.: -0.004 min
Response: 202819
Conc: 9.24 ng/ml

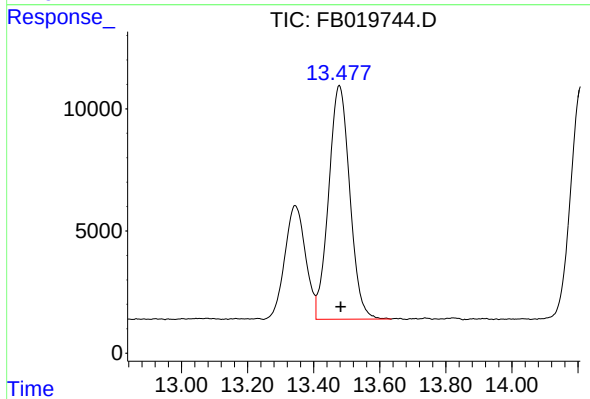


#8 m-Xylene

R.T.: 13.478 min
Delta R.T.: -0.004 min
Response: 425205
Conc: 18.58 ng/ml

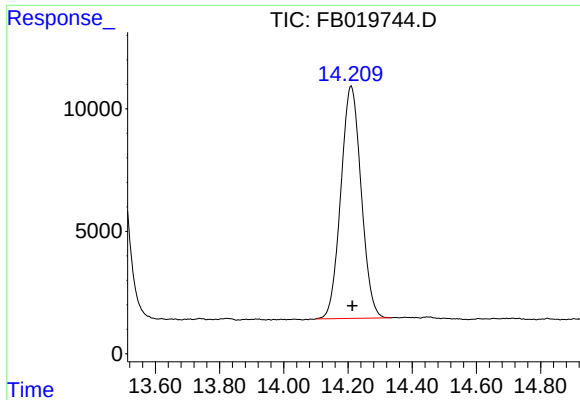

#9 O-Xylene

R.T.: 14.210 min
Delta R.T.: -0.004 min
Response: 416976
Conc: 18.67 ng/ml

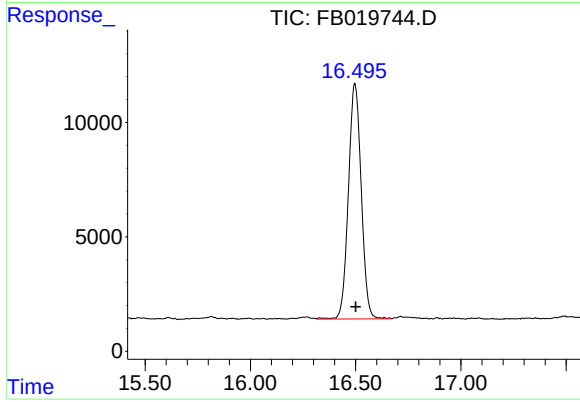

#10 1,2,4-Trimethylbenzene

R.T.: 16.497 min
Delta R.T.: -0.003 min
Response: 435239
Conc: 18.78 ng/ml