

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021320\
 Data File : FB023667.D
 Signal(s) : FID2B.CH
 Acq On : 13 Feb 2020 11:35
 Operator : DD/AJ
 Sample : BSF0213S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 14 01:30:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.798	429257	21.084 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.690	946451	31.454 ng/ml
2) t	2,2,4-Trimethylpentane	7.417	1061398	32.527 ng/ml
3) t	n-Heptane	7.757	349200	10.853 ng/ml
4) t	Benzene	7.891	420164	10.273 ng/ml
6) t	Toluene	10.630	1225764	30.880 ng/ml
7) t	Ethylbenzene	13.070	382909	10.300 ng/ml
8) t	m-Xylene	13.203	733950	20.552 ng/ml
9) t	O-Xylene	13.931	700623	20.314 ng/ml
10) t	1,2,4-Trimethylbenzene	16.209	595491	20.339 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021320\
Data File : FB023667.D
Signal(s) : FID2B.CH
Acq On : 13 Feb 2020 11:35
Operator : DD/AJ
Sample : BSF0213S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 14 01:30:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

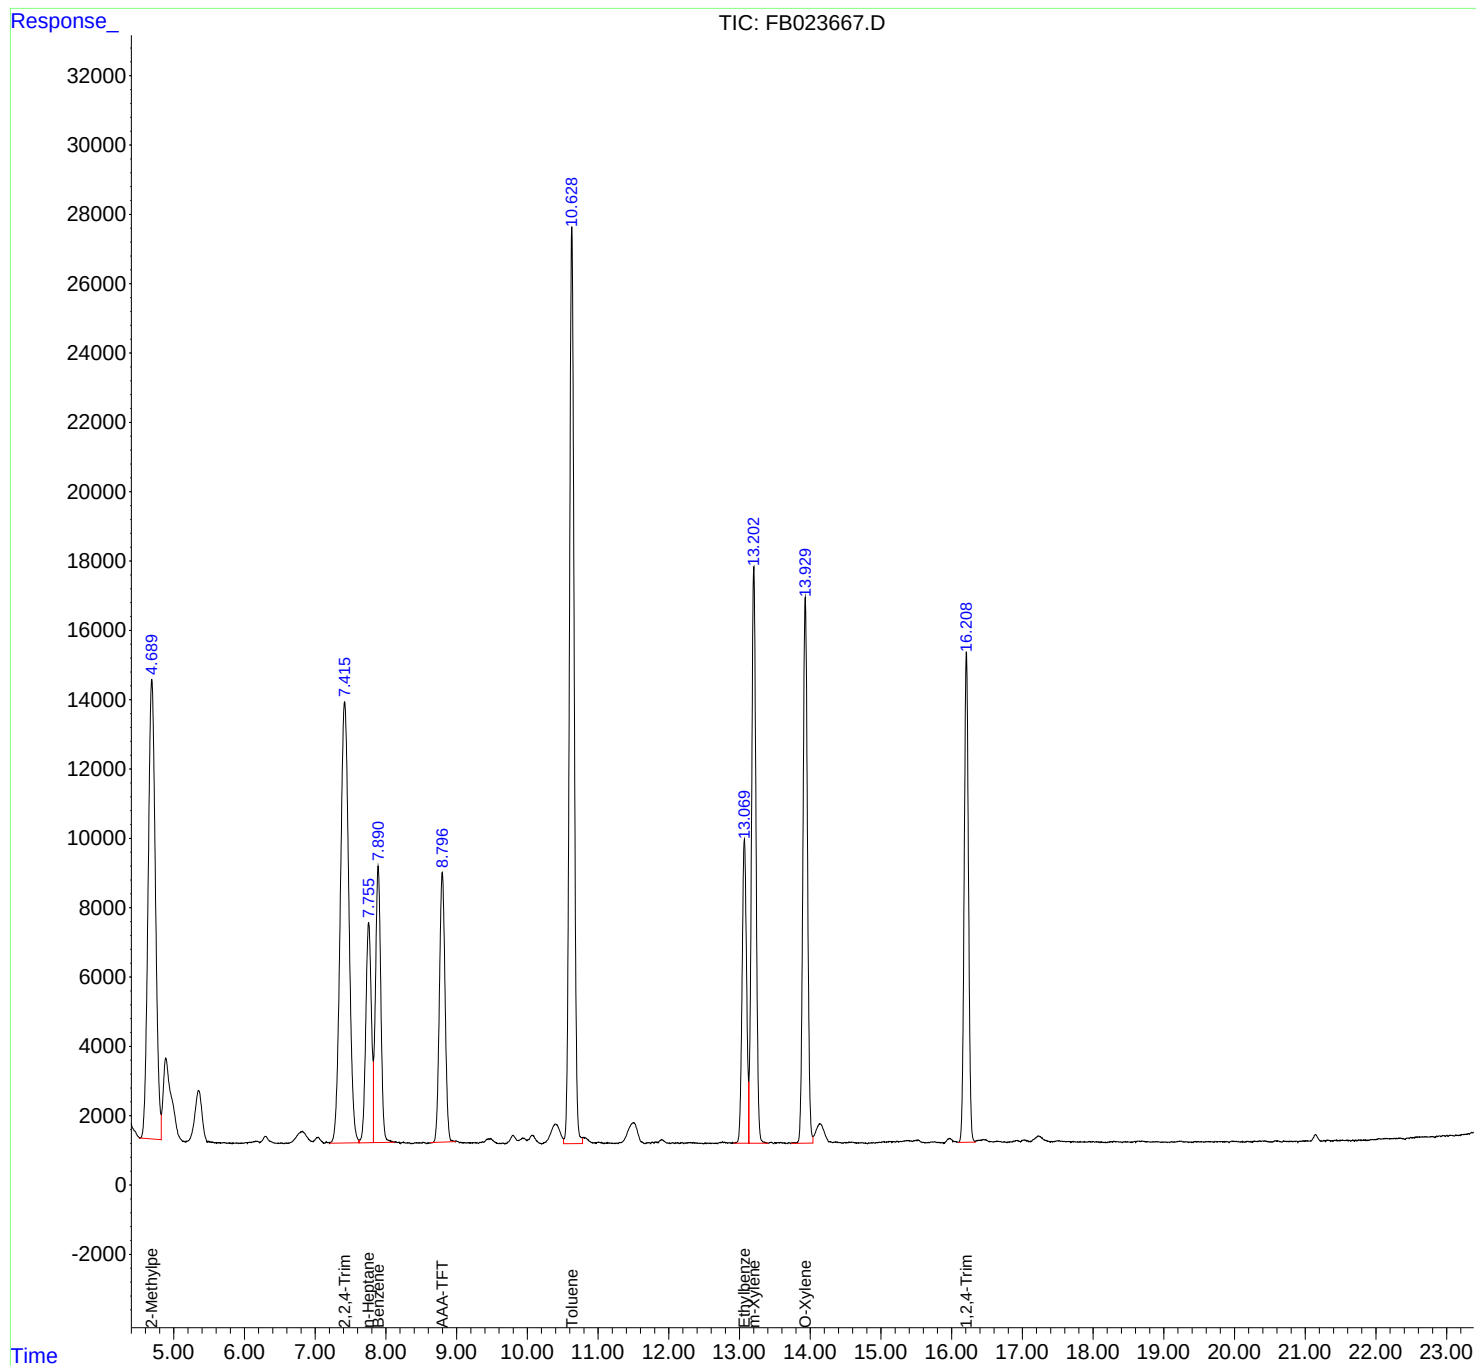

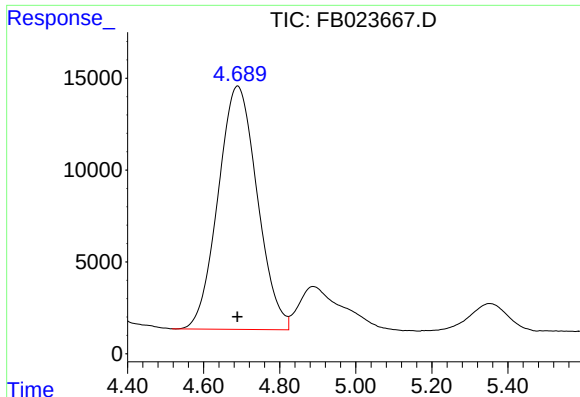


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.001 min
Response: 946451
Conc: 31.45 ng/ml

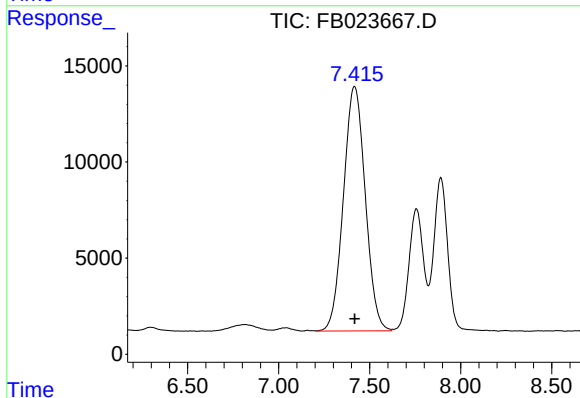


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.001 min
Response: 1061398
Conc: 32.53 ng/ml

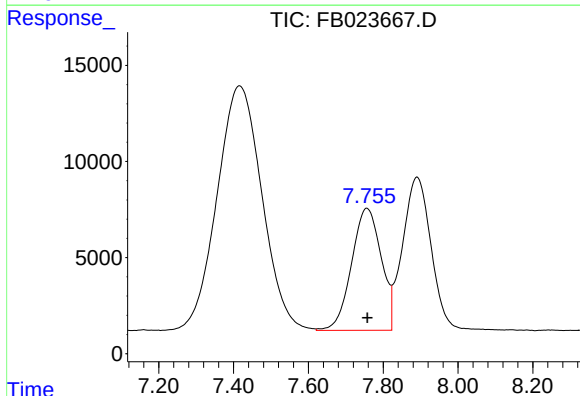


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.001 min
Response: 349200
Conc: 10.85 ng/ml

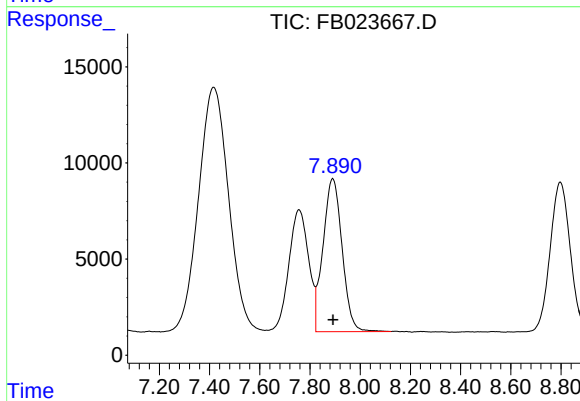


#4 Benzene

R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 420164
Conc: 10.27 ng/ml

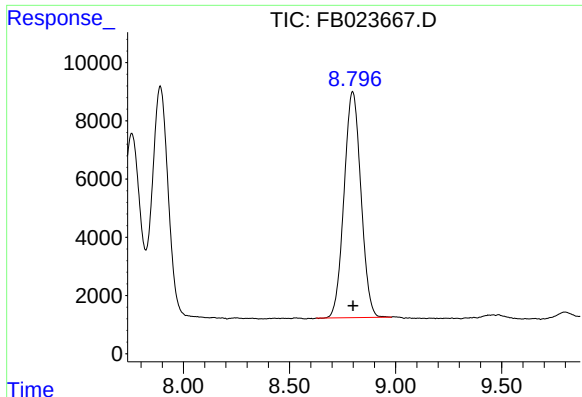


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 429257
Conc: 21.08 ng/ml

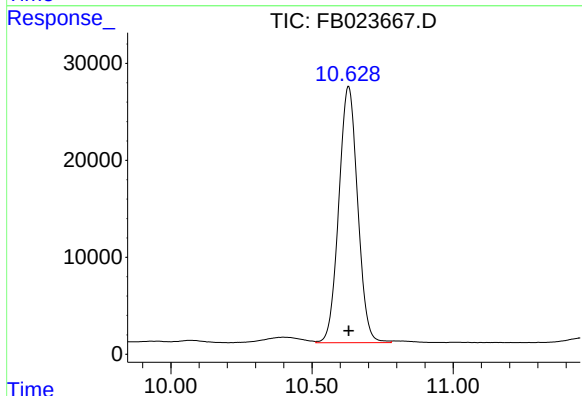


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 1225764
Conc: 30.88 ng/ml

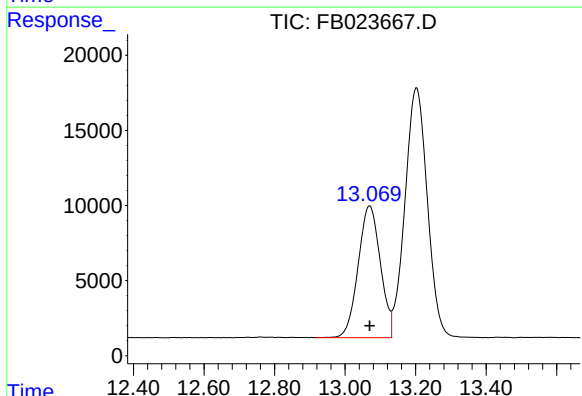


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 382909
Conc: 10.30 ng/ml

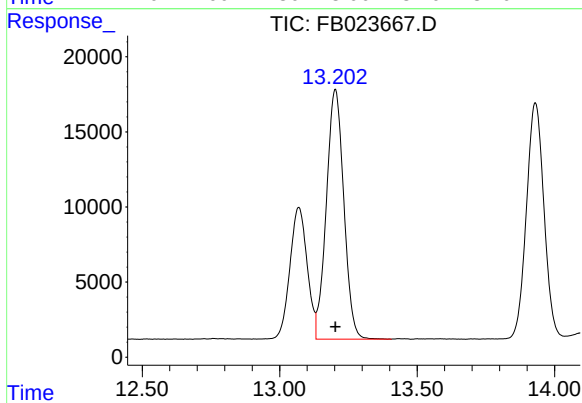


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 733950
Conc: 20.55 ng/ml

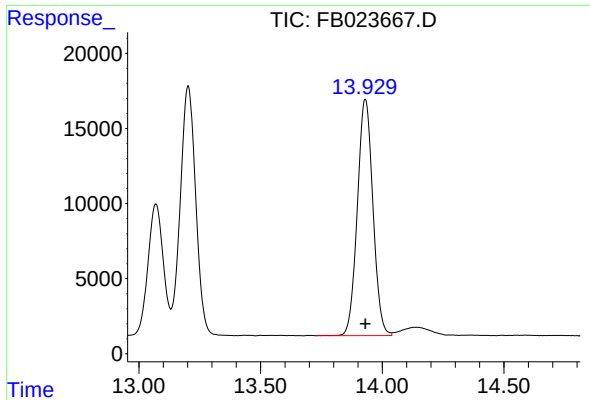

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 700623
Conc: 20.31 ng/ml

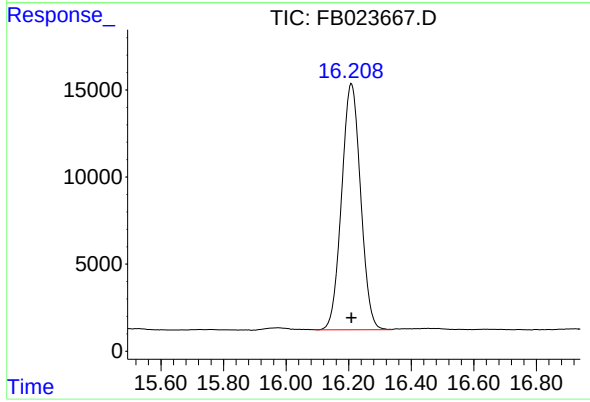

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 595491
Conc: 20.34 ng/ml