

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB021419\  
Data File : FB019759.D  
Signal(s) : FID2B.CH  
Acq On : 14 Feb 2019 12:34  
Operator : MJ/SJ  
Sample : K1349-05  
Misc : 5.00g/5.00ml DI WATER  
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Feb 14 22:37:44 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB012919.M  
Quant Title :  
QLast Update : Tue Jan 29 12:07:12 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 9.040  | 207721   | 17.770 ng/ml |
| Target Compounds             |        |          |              |
| 6) t Toluene                 | 10.891 | 9423     | 0.539 ng/ml  |
| 8) t m-Xylene                | 13.468 | 9817     | 0.429 ng/ml  |
| 9) t O-Xylene                | 14.207 | 5833     | 0.261 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.491 | 21796    | 0.941 ng/ml  |
| -----                        |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB021419\  
Data File : FB019759.D  
Signal(s) : FID2B.CH  
Acq On : 14 Feb 2019 12:34  
Operator : MJ/SJ  
Sample : K1349-05  
Misc : 5.00g/5.00ml DI WATER  
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Feb 14 22:37:44 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB012919.M  
Quant Title :  
QLast Update : Tue Jan 29 12:07:12 2019  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

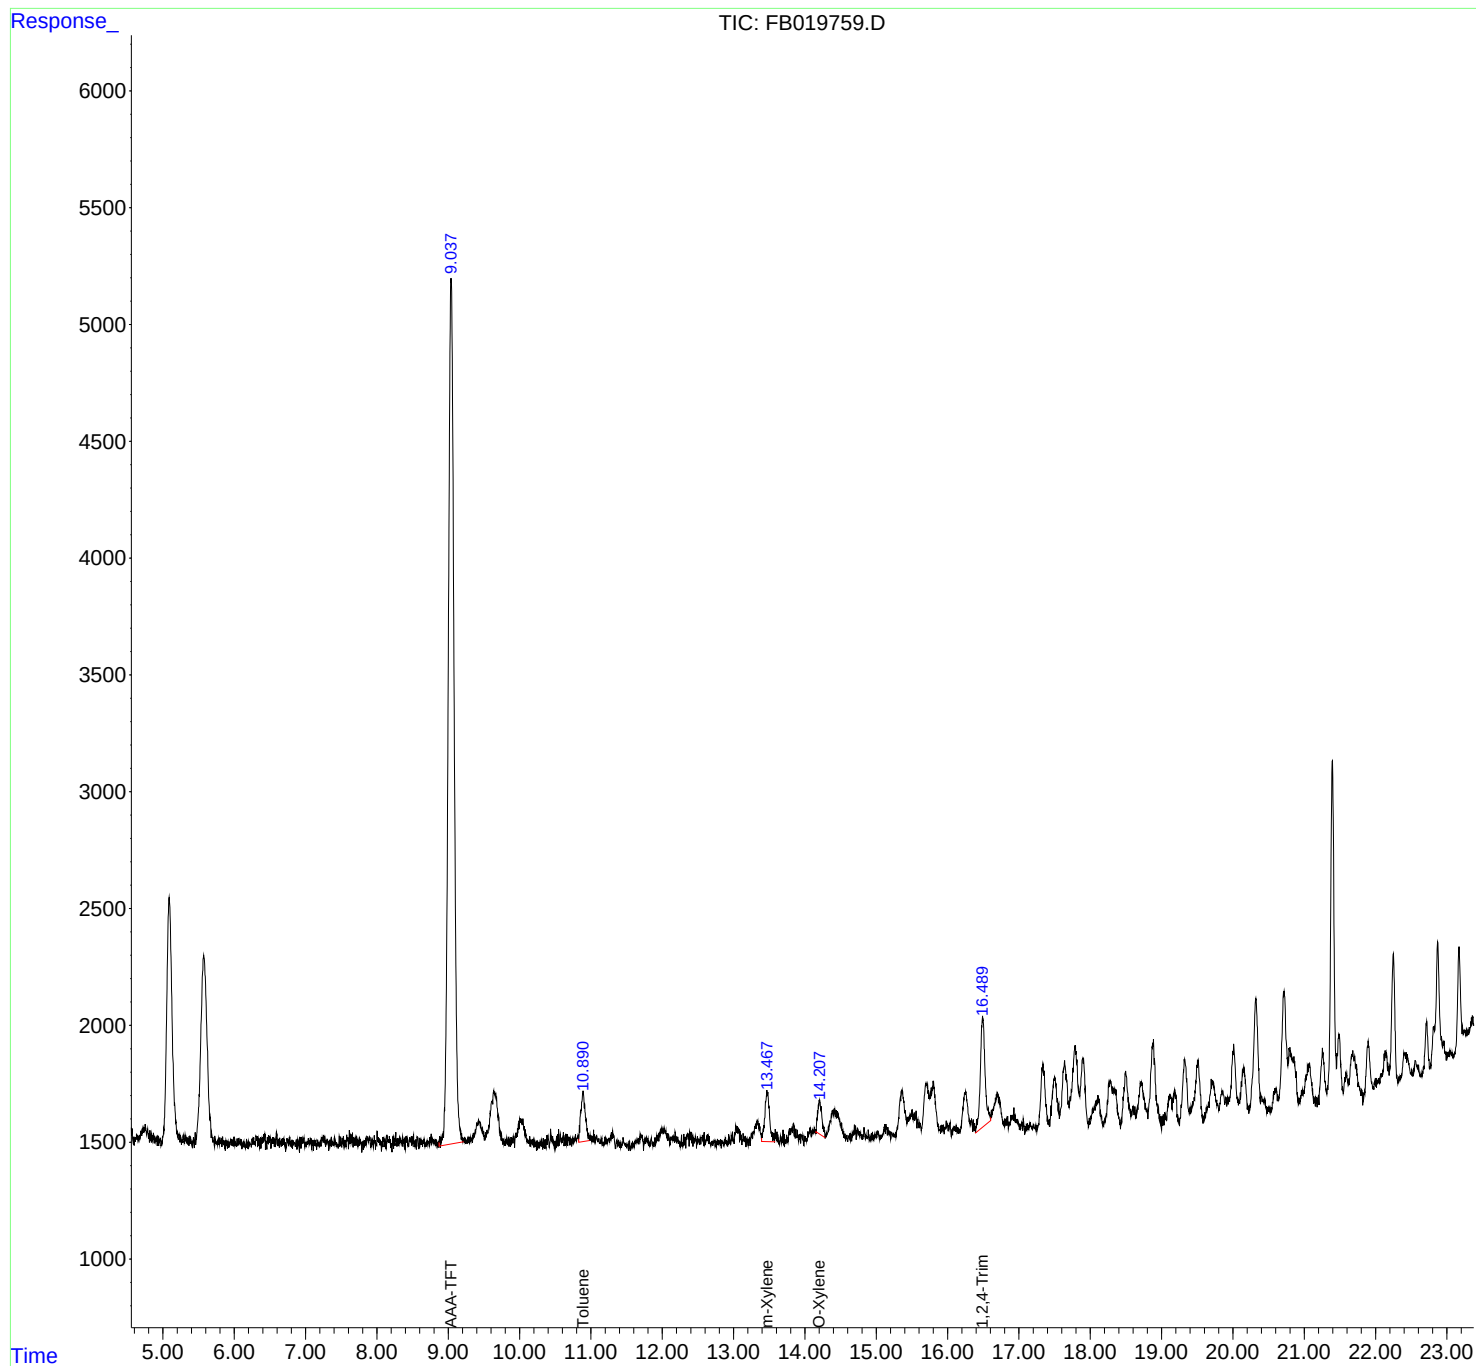

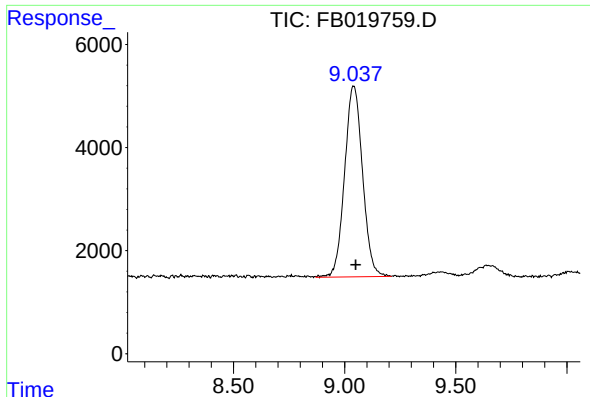


#5 AAA-TFT

R.T.: 9.040 min  
Delta R.T.: -0.009 min  
Response: 207721  
Conc: 17.77 ng/ml

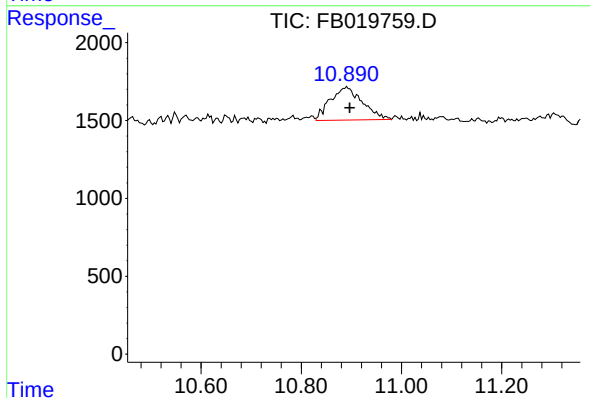


#6 Toluene

R.T.: 10.891 min  
Delta R.T.: -0.005 min  
Response: 9423  
Conc: 0.54 ng/ml

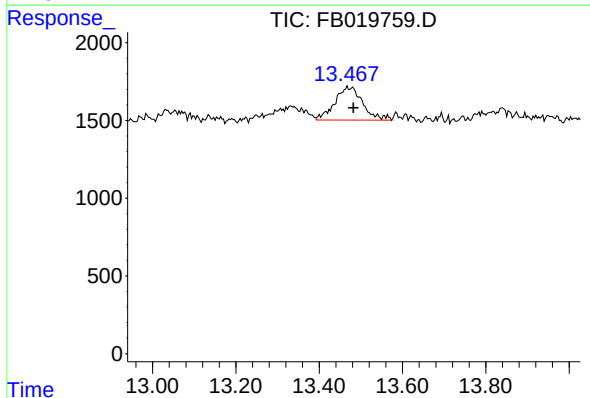


#8 m-Xylene

R.T.: 13.468 min  
Delta R.T.: -0.014 min  
Response: 9817  
Conc: 0.43 ng/ml

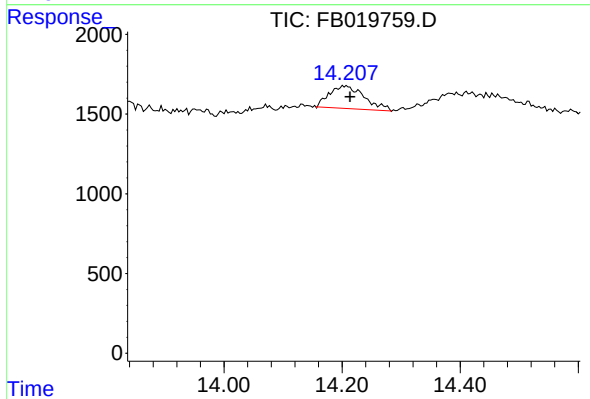

#9 O-Xylene

R.T.: 14.207 min  
Delta R.T.: -0.007 min  
Response: 5833  
Conc: 0.26 ng/ml

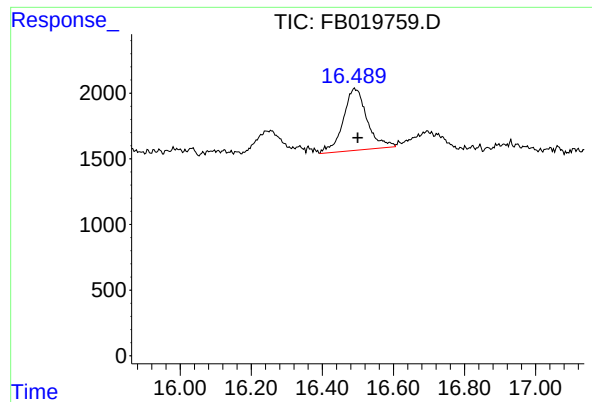

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min  
Delta R.T.: -0.009 min  
Response: 21796  
Conc: 0.94 ng/ml