

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021419\
 Data File : FB019762.D
 Signal(s) : FID2B.CH
 Acq On : 14 Feb 2019 14:04
 Operator : MJ/SJ
 Sample : K1349-07MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 14 22:38:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.041	198630	16.992 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.898	464651	26.838 ng/ml
2) t	2,2,4-Trimethylpentane	7.656	389094	23.463 ng/ml
3) t	n-Heptane	7.997	113166	7.022 ng/ml
4) t	Benzene	8.134	180776	9.584 ng/ml
6) t	Toluene	10.889	459041	26.242 ng/ml
7) t	Ethylbenzene	13.340	176501	8.043 ng/ml
8) t	m-Xylene	13.474	359678	15.715 ng/ml
9) t	O-Xylene	14.206	358956	16.072 ng/ml
10) t	1,2,4-Trimethylbenzene	16.492	343917	14.843 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021419\
Data File : FB019762.D
Signal(s) : FID2B.CH
Acq On : 14 Feb 2019 14:04
Operator : MJ/SJ
Sample : K1349-07MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 14 22:38:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

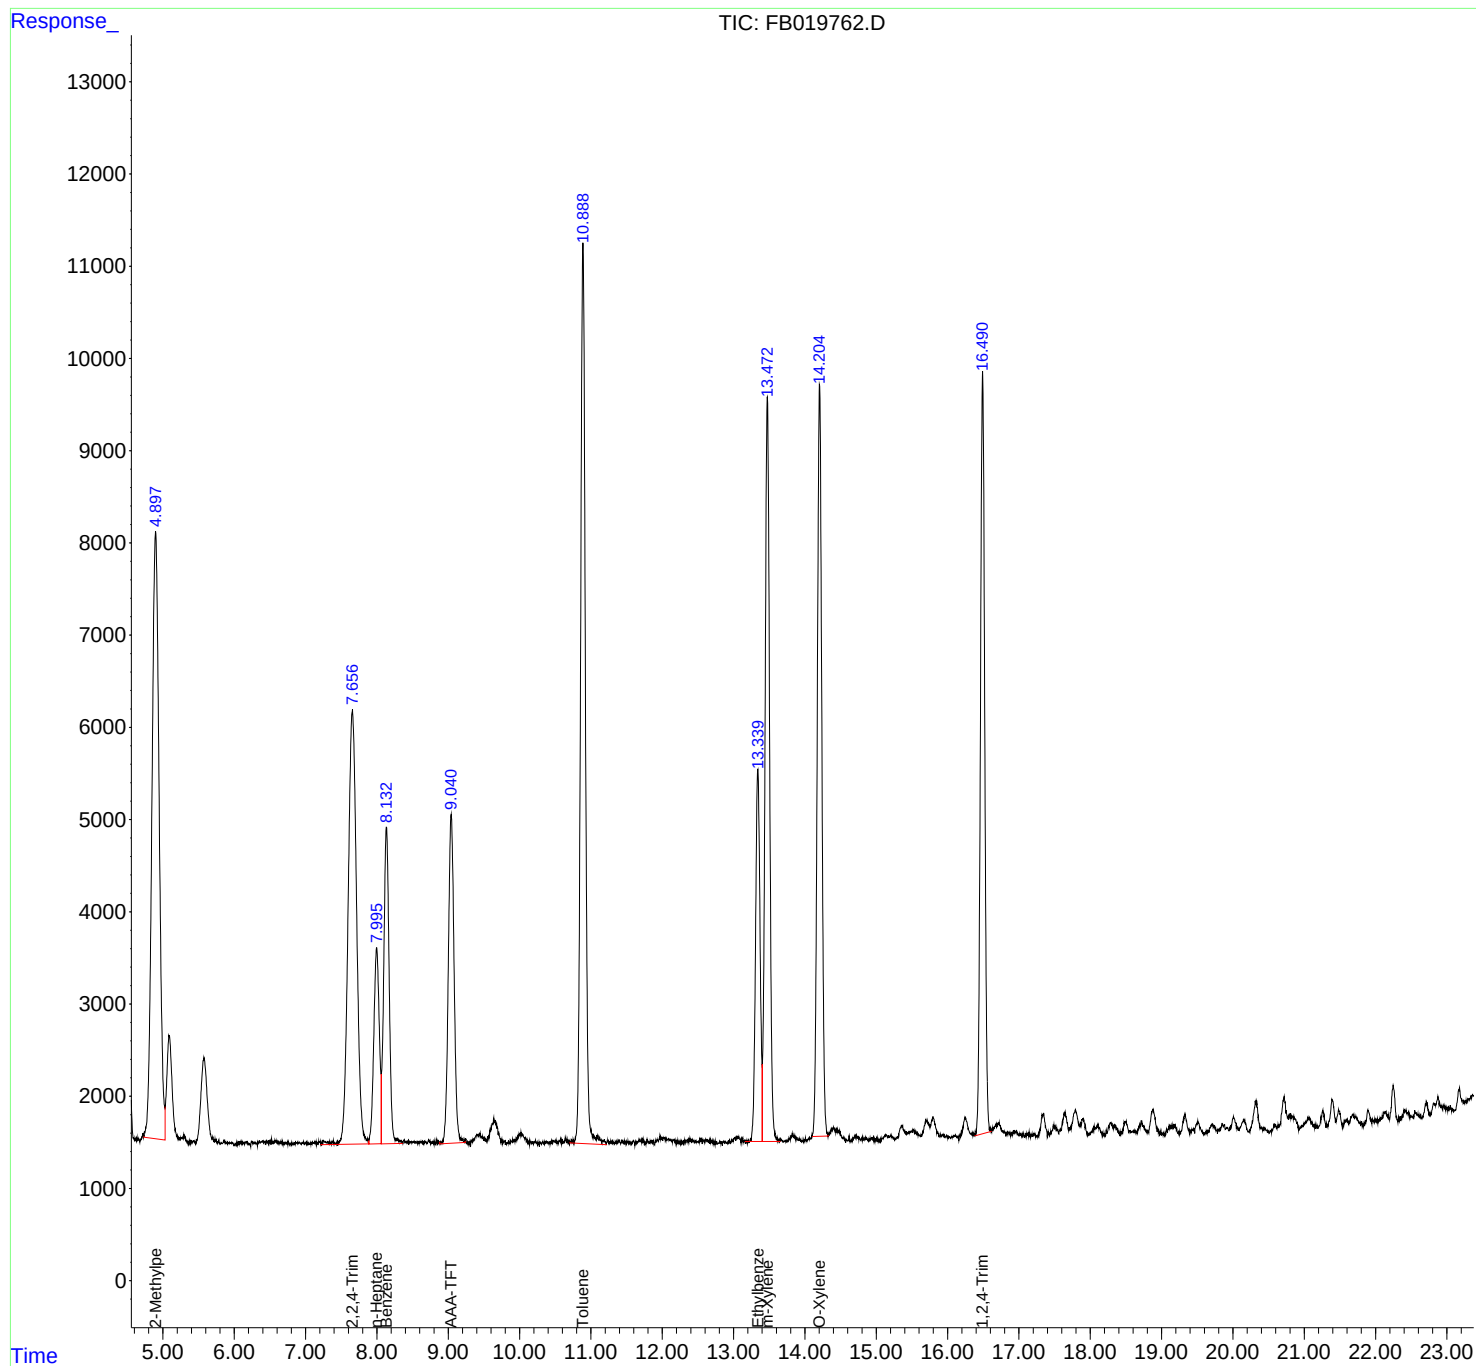

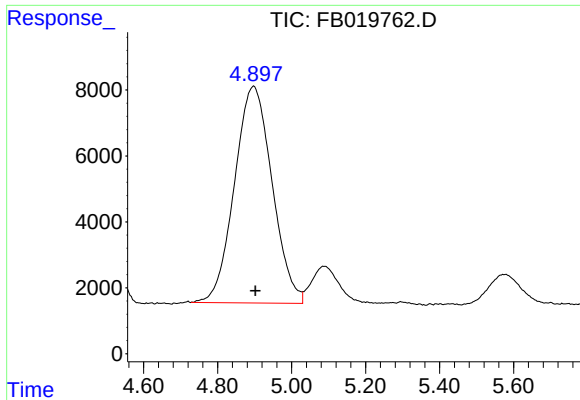


#1 2-Methylpentane

R.T.: 4.898 min
Delta R.T.: -0.004 min
Response: 464651
Conc: 26.84 ng/ml

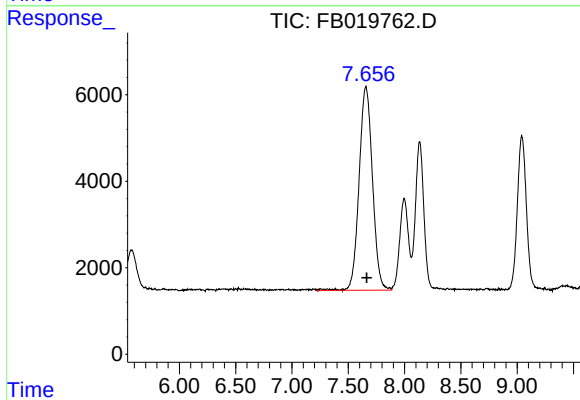


#2 2,2,4-Trimethylpentane

R.T.: 7.656 min
Delta R.T.: -0.008 min
Response: 389094
Conc: 23.46 ng/ml

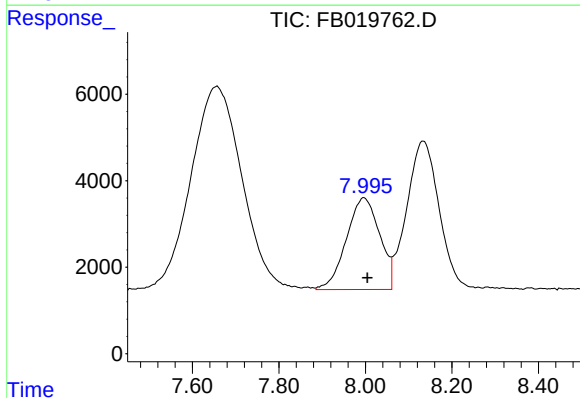


#3 n-Heptane

R.T.: 7.997 min
Delta R.T.: -0.008 min
Response: 113166
Conc: 7.02 ng/ml

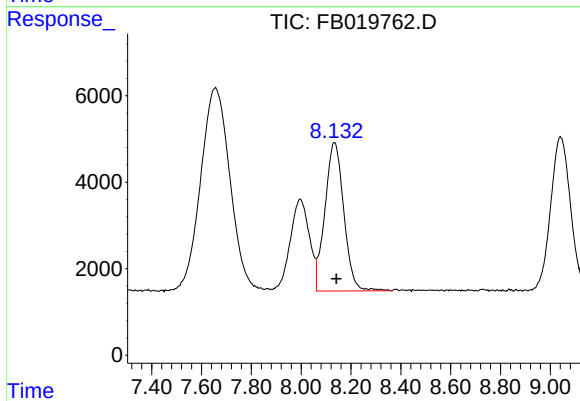


#4 Benzene

R.T.: 8.134 min
Delta R.T.: -0.007 min
Response: 180776
Conc: 9.58 ng/ml

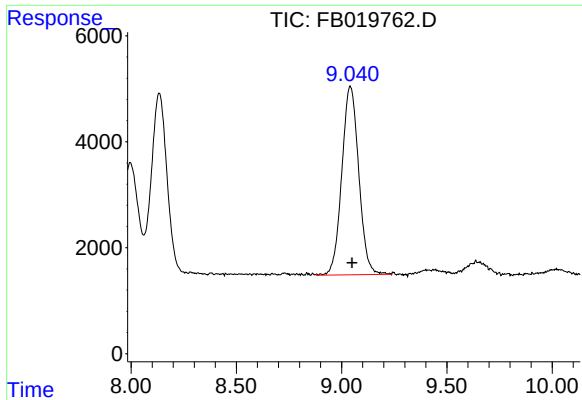


#5 AAA-TFT

R.T.: 9.041 min
Delta R.T.: -0.008 min
Response: 198630
Conc: 16.99 ng/ml

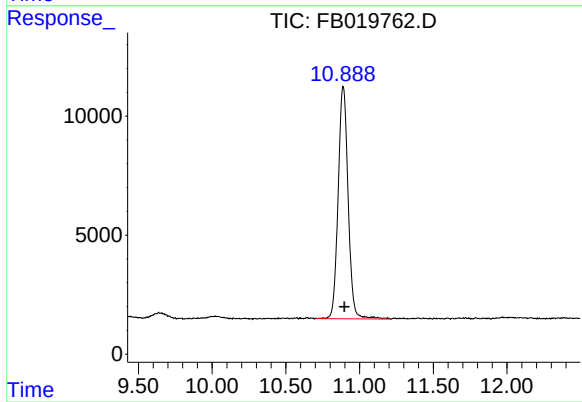


#6 Toluene

R.T.: 10.889 min
Delta R.T.: -0.008 min
Response: 459041
Conc: 26.24 ng/ml

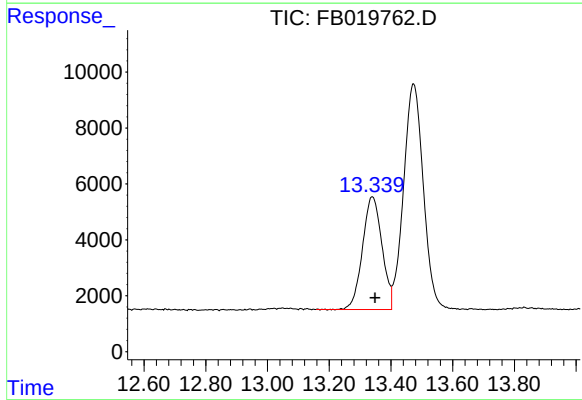


#7 Ethylbenzene

R.T.: 13.340 min
Delta R.T.: -0.008 min
Response: 176501
Conc: 8.04 ng/ml

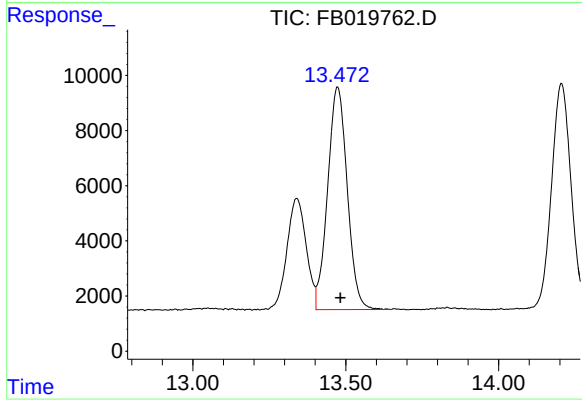


#8 m-Xylene

R.T.: 13.474 min
Delta R.T.: -0.008 min
Response: 359678
Conc: 15.71 ng/ml

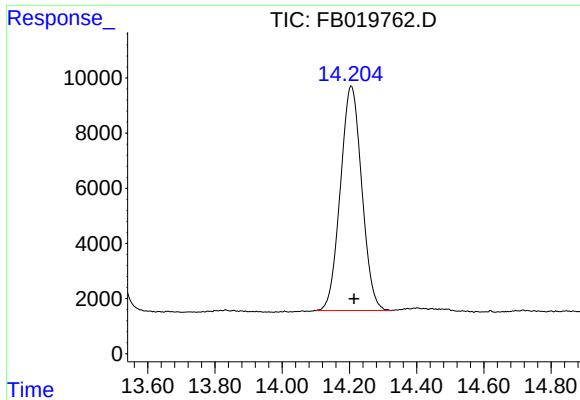

#9 O-Xylene

R.T.: 14.206 min
Delta R.T.: -0.008 min
Response: 358956
Conc: 16.07 ng/ml

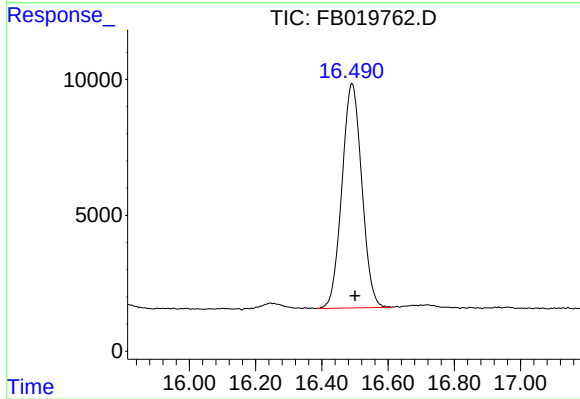

#10 1,2,4-Trimethylbenzene

R.T.: 16.492 min
Delta R.T.: -0.008 min
Response: 343917
Conc: 14.84 ng/ml