

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021419\
 Data File : FB019755.D
 Signal(s) : FID2B.CH
 Acq On : 14 Feb 2019 9:53
 Operator : MJ/SJ
 Sample : BSF0214S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 14 22:37:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	210603	18.016 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.896	568714	32.849 ng/ml
2) t 2,2,4-Trimethylpentane	7.656	556166	33.537 ng/ml
3) t n-Heptane	7.995	169519	10.519 ng/ml
4) t Benzene	8.133	191873	10.173 ng/ml
6) t Toluene	10.887	535646	30.622 ng/ml
7) t Ethylbenzene	13.340	210652	9.599 ng/ml
8) t m-Xylene	13.473	439225	19.190 ng/ml
9) t O-Xylene	14.204	426445	19.093 ng/ml
10) t 1,2,4-Trimethylbenzene	16.491	433889	18.726 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021419\
Data File : FB019755.D
Signal(s) : FID2B.CH
Acq On : 14 Feb 2019 9:53
Operator : MJ/SJ
Sample : BSF0214S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 14 22:37:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

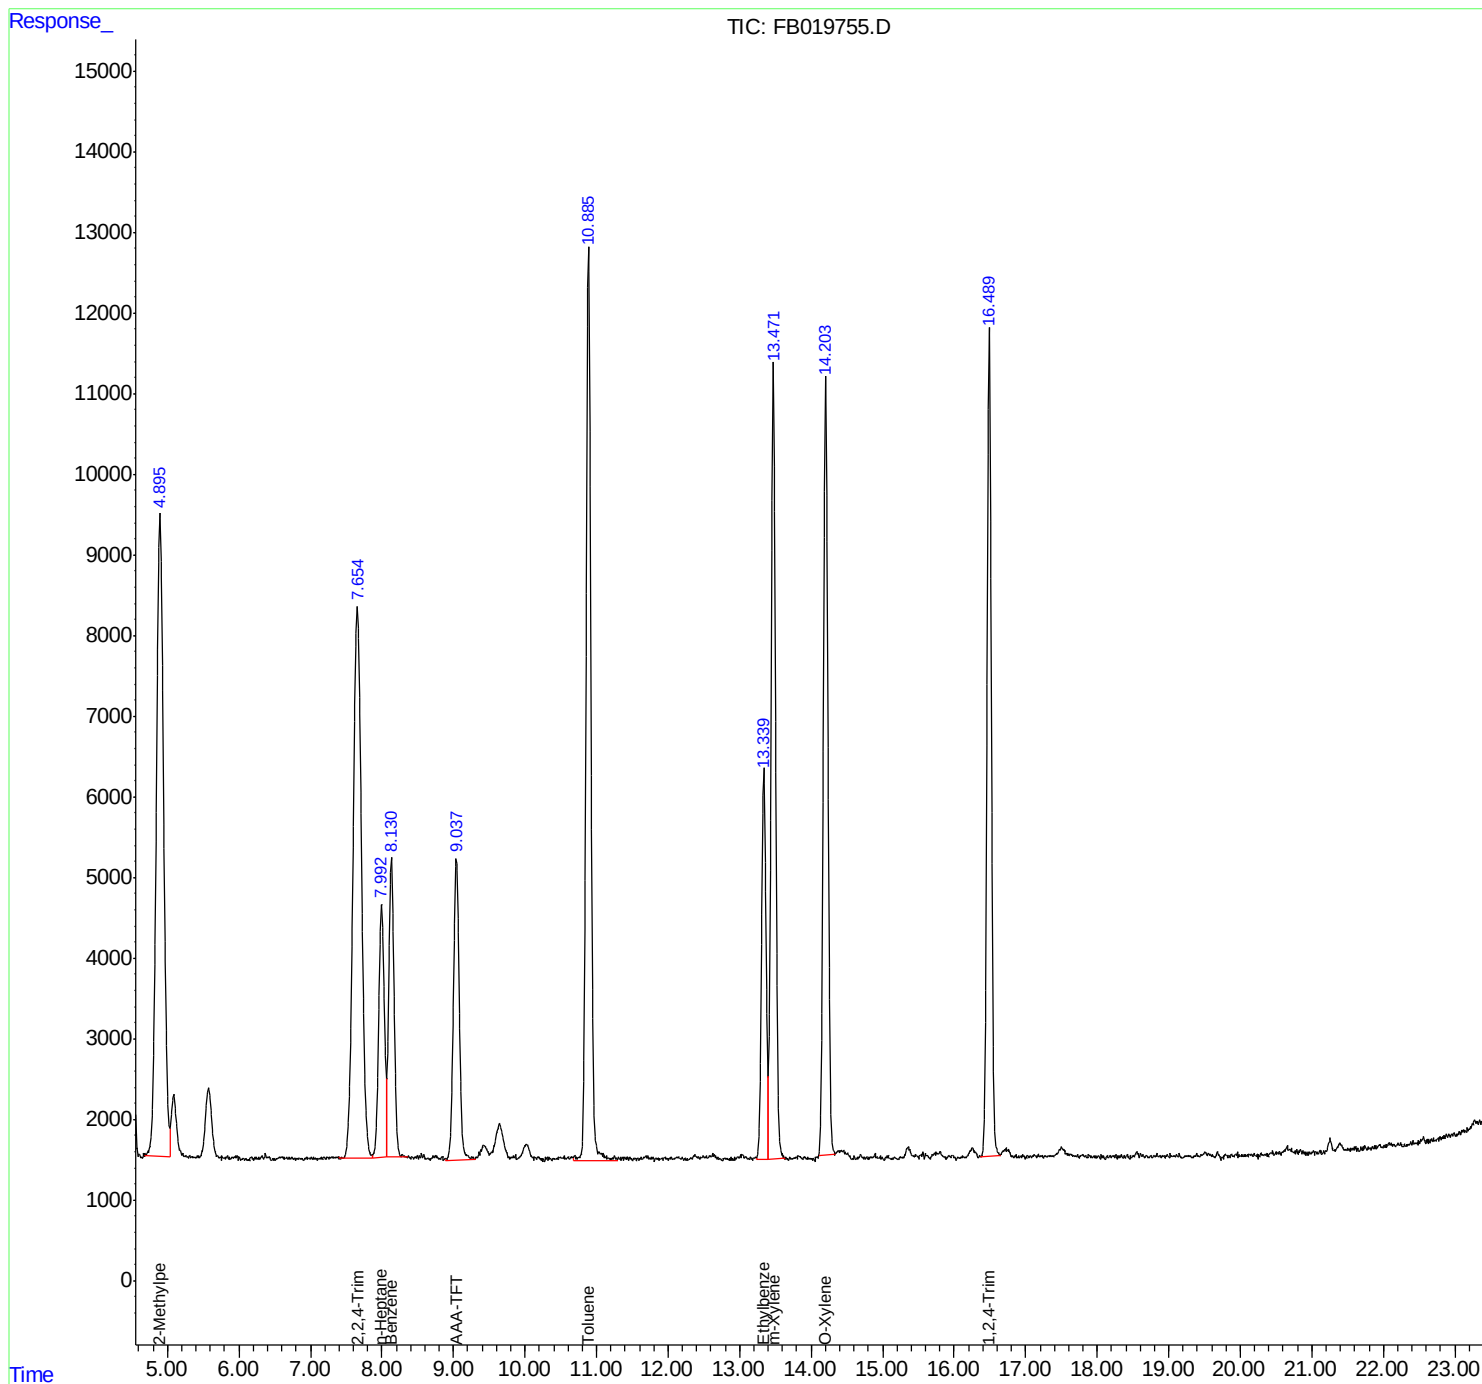

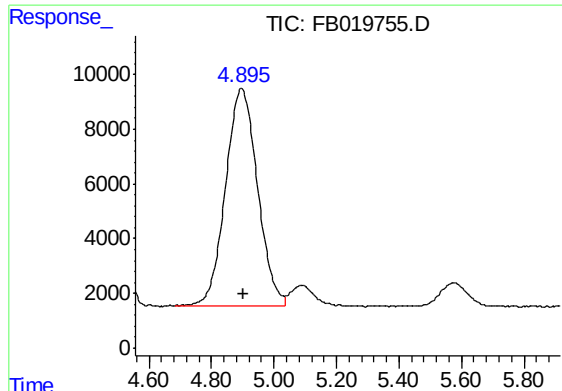


#1 2-Methylpentane

R.T.: 4.896 min
Delta R.T.: -0.006 min
Response: 568714
Conc: 32.85 ng/ml

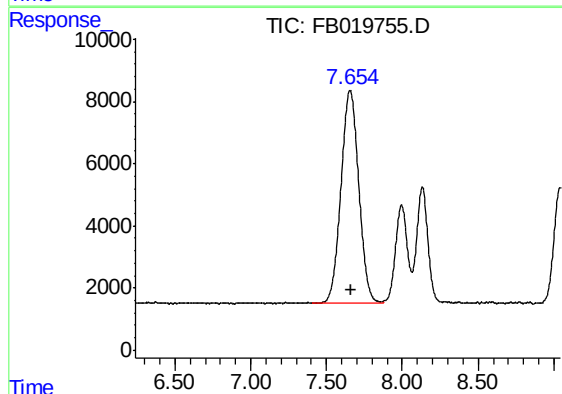


#2 2,2,4-Trimethylpentane

R.T.: 7.656 min
Delta R.T.: -0.008 min
Response: 556166
Conc: 33.54 ng/ml

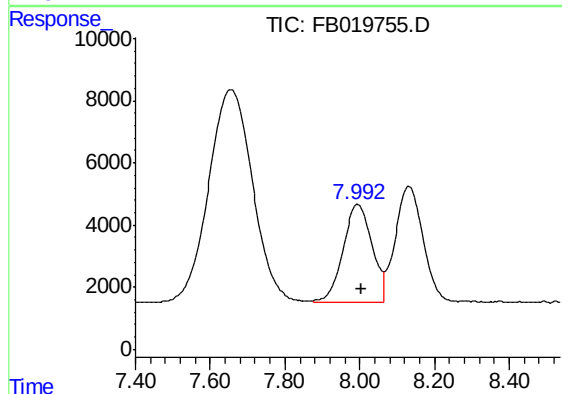


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: -0.010 min
Response: 169519
Conc: 10.52 ng/ml

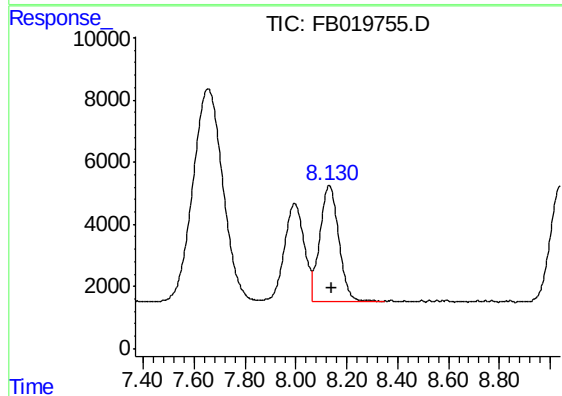


#4 Benzene

R.T.: 8.133 min
Delta R.T.: -0.008 min
Response: 191873
Conc: 10.17 ng/ml

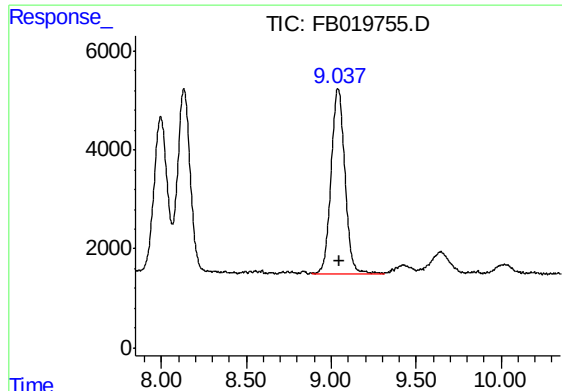


#5 AAA-TFT

R.T.: 9.040 min
Delta R.T.: -0.009 min
Response: 210603
Conc: 18.02 ng/ml

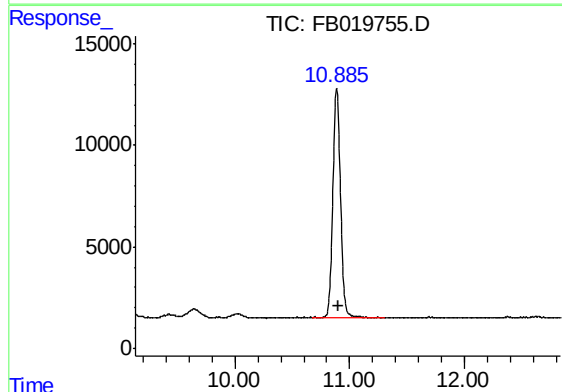


#6 Toluene

R.T.: 10.887 min
Delta R.T.: -0.009 min
Response: 535646
Conc: 30.62 ng/ml

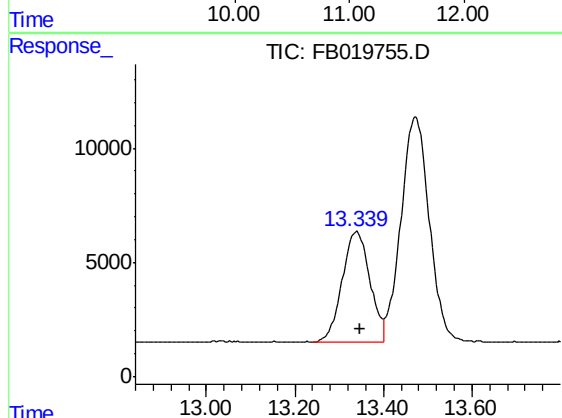


#7 Ethylbenzene

R.T.: 13.340 min
Delta R.T.: -0.009 min
Response: 210652
Conc: 9.60 ng/ml

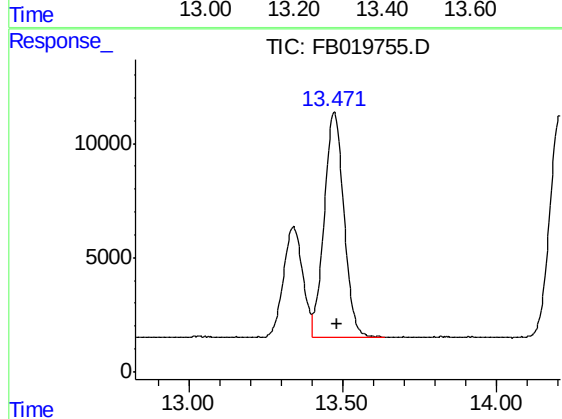


#8 m-Xylene

R.T.: 13.473 min
Delta R.T.: -0.009 min
Response: 439225
Conc: 19.19 ng/ml

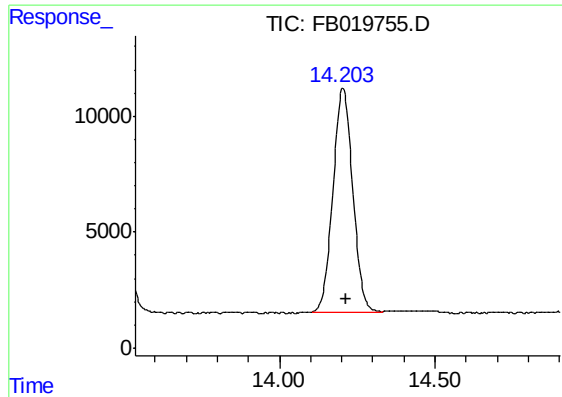

#9 O-Xylene

R.T.: 14.204 min
Delta R.T.: -0.009 min
Response: 426445
Conc: 19.09 ng/ml

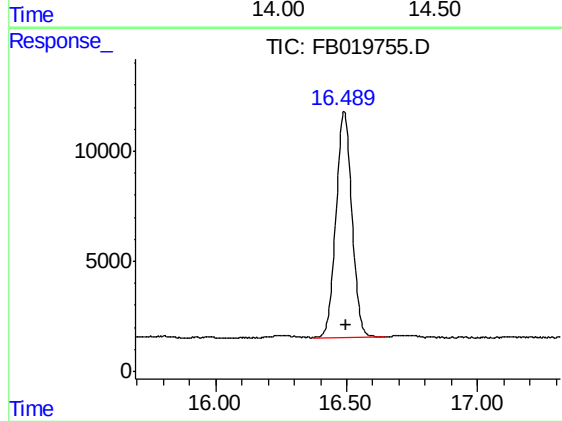

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min
Delta R.T.: -0.009 min
Response: 433889
Conc: 18.73 ng/ml