

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021519\
 Data File : FB019766.D
 Signal(s) : FID2B.CH
 Acq On : 15 Feb 2019 9:21
 Operator : MJ/SJ
 Sample : BSF0215S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 15 23:14:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.043	209908	17.957 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.896	567024	32.751 ng/ml
2) t 2,2,4-Trimethylpentane	7.656	571416	34.457 ng/ml
3) t n-Heptane	7.997	172054	10.677 ng/ml
4) t Benzene	8.134	193959	10.283 ng/ml
6) t Toluene	10.889	526448	30.096 ng/ml
7) t Ethylbenzene	13.341	210630	9.598 ng/ml
8) t m-Xylene	13.474	437244	19.104 ng/ml
9) t O-Xylene	14.206	427091	19.122 ng/ml
10) t 1,2,4-Trimethylbenzene	16.493	432986	18.687 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021519\
Data File : FB019766.D
Signal(s) : FID2B.CH
Acq On : 15 Feb 2019 9:21
Operator : MJ/SJ
Sample : BSF021551
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 15 23:14:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

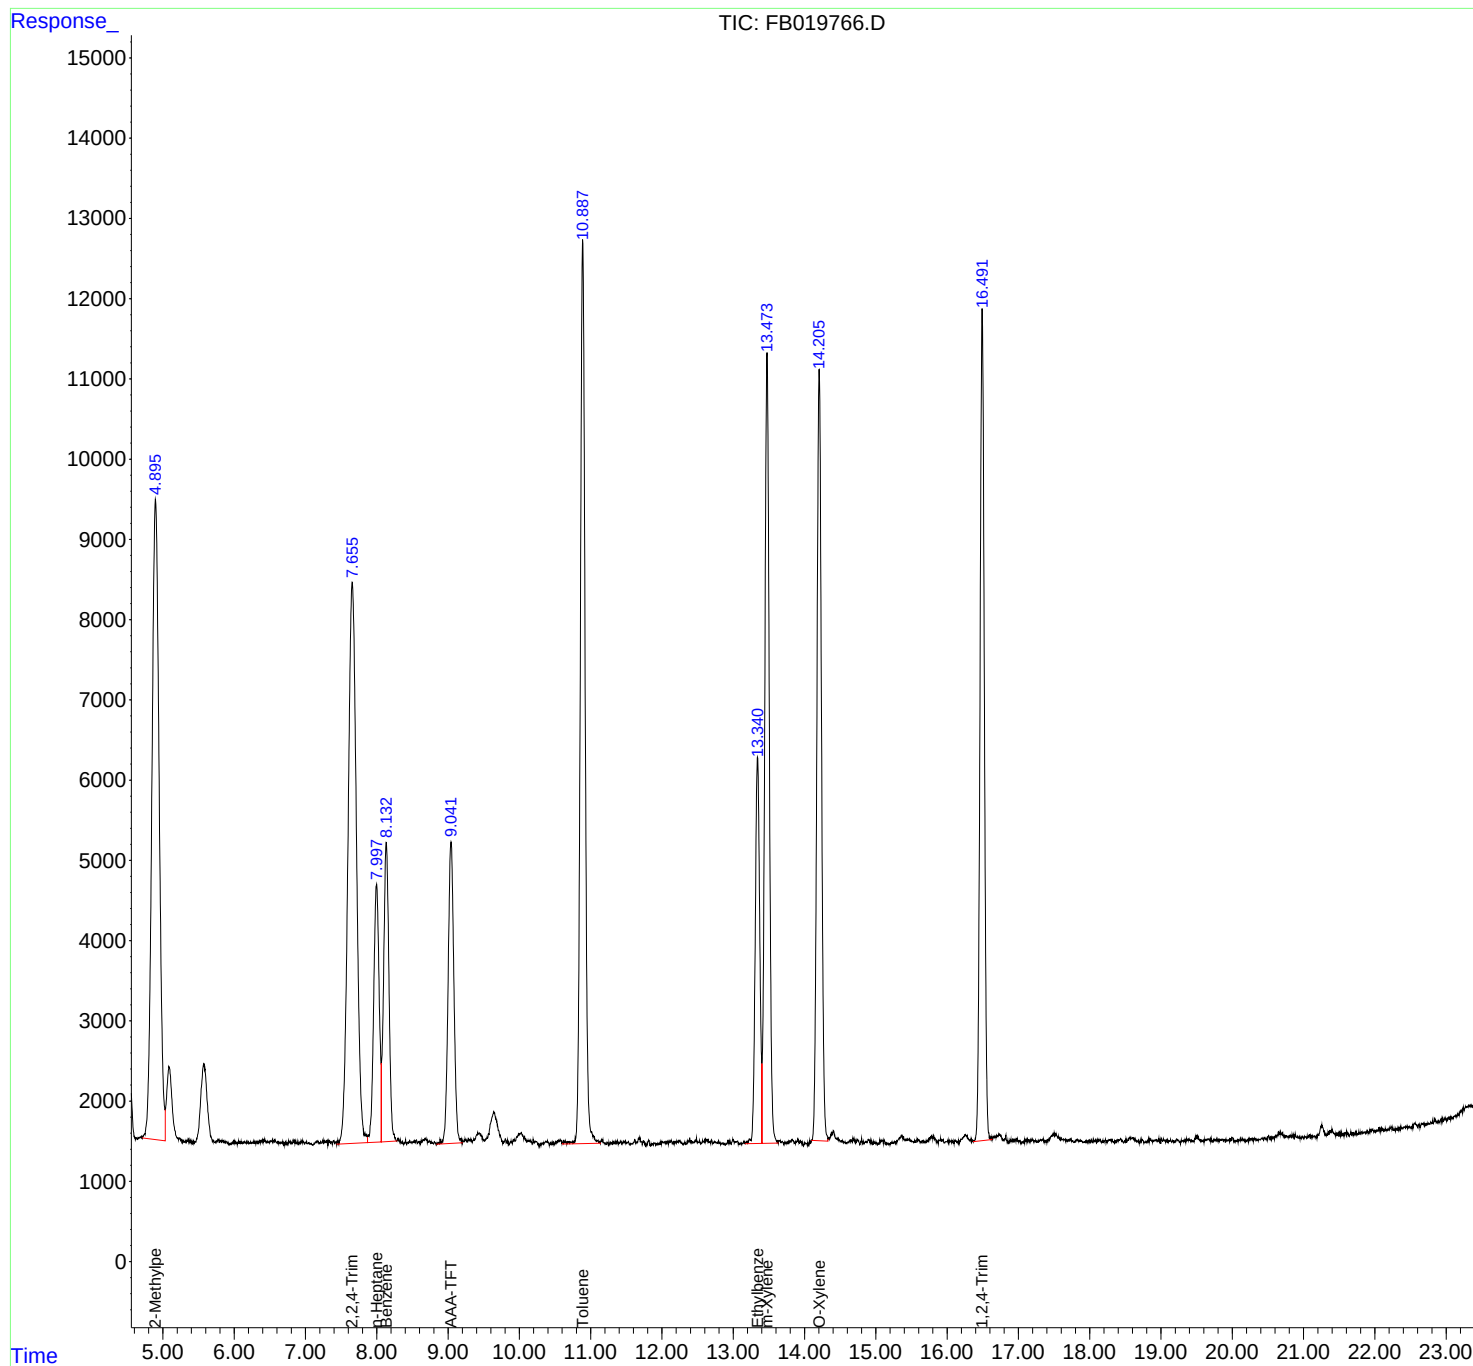

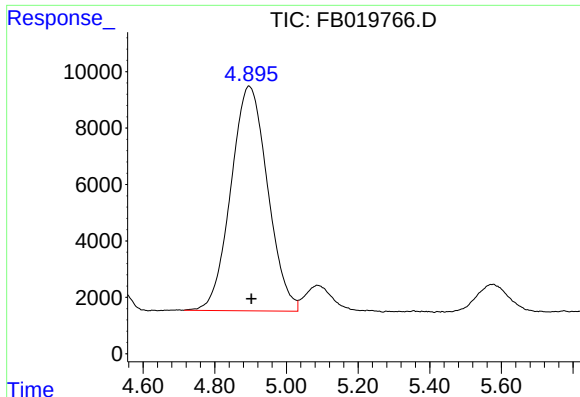


#1 2-Methylpentane

R.T.: 4.896 min
Delta R.T.: -0.006 min
Response: 567024
Conc: 32.75 ng/ml

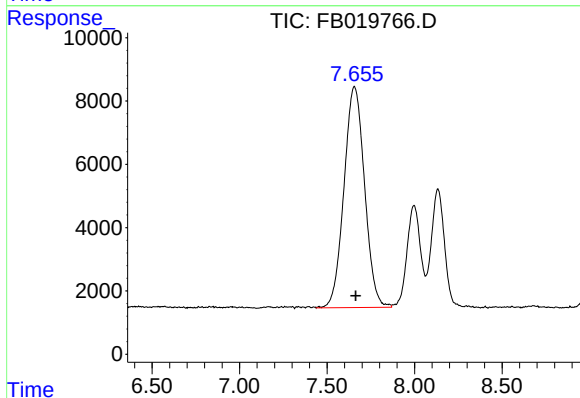


#2 2,2,4-Trimethylpentane

R.T.: 7.656 min
Delta R.T.: -0.008 min
Response: 571416
Conc: 34.46 ng/ml

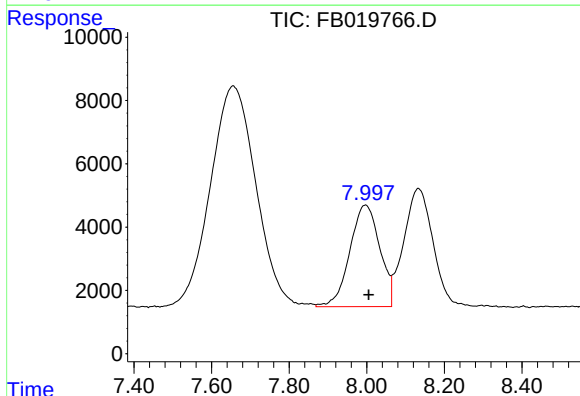


#3 n-Heptane

R.T.: 7.997 min
Delta R.T.: -0.008 min
Response: 172054
Conc: 10.68 ng/ml

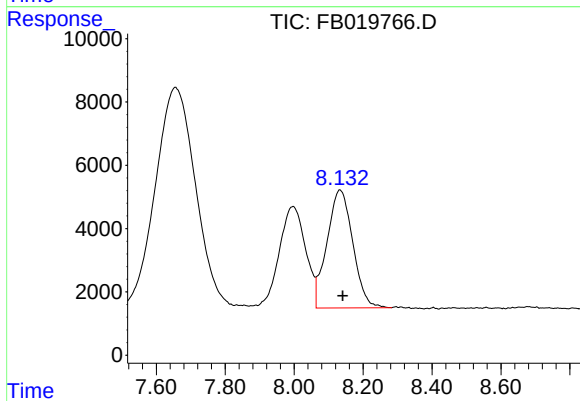


#4 Benzene

R.T.: 8.134 min
Delta R.T.: -0.008 min
Response: 193959
Conc: 10.28 ng/ml

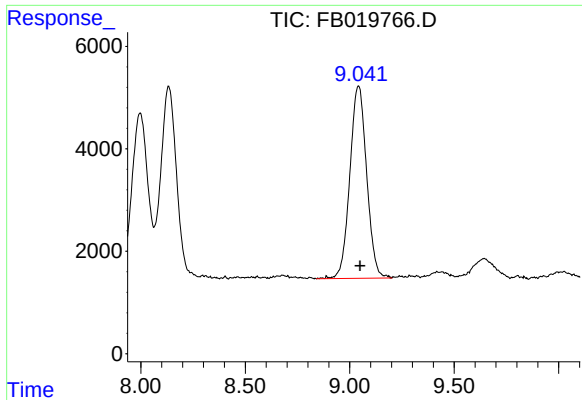


#5 AAA-TFT

R.T.: 9.043 min
Delta R.T.: -0.007 min
Response: 209908
Conc: 17.96 ng/ml

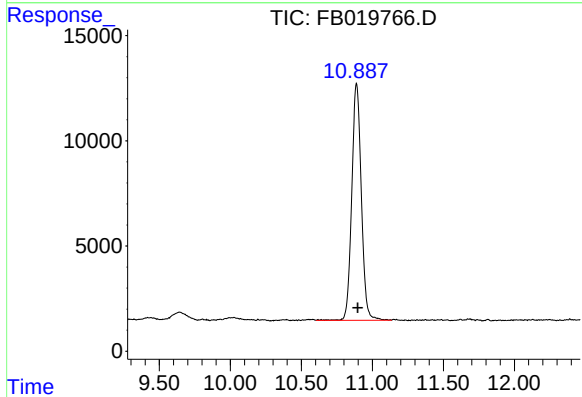


#6 Toluene

R.T.: 10.889 min
Delta R.T.: -0.008 min
Response: 526448
Conc: 30.10 ng/ml

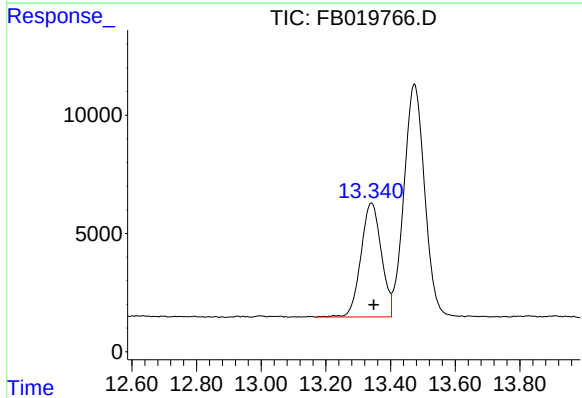


#7 Ethylbenzene

R.T.: 13.341 min
Delta R.T.: -0.007 min
Response: 210630
Conc: 9.60 ng/ml

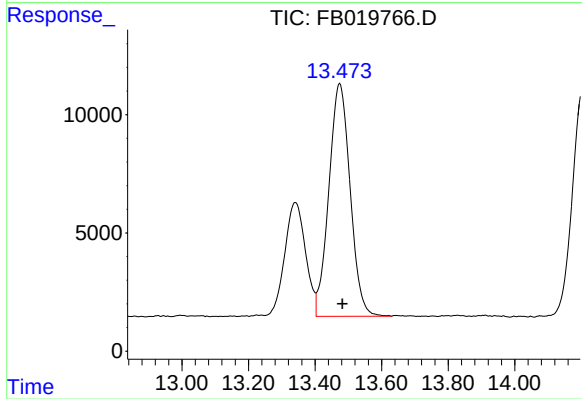

#8 m-Xylene

R.T.: 13.474 min
Delta R.T.: -0.008 min
Response: 437244
Conc: 19.10 ng/ml

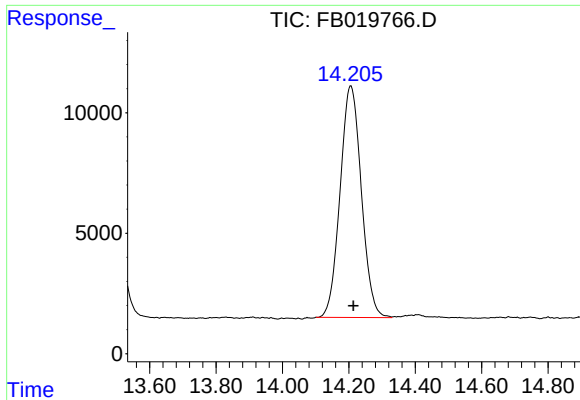


#9 O-Xylene

R.T.: 14.206 min

Delta R.T.: -0.008 min

Response: 427091

Conc: 19.12 ng/ml

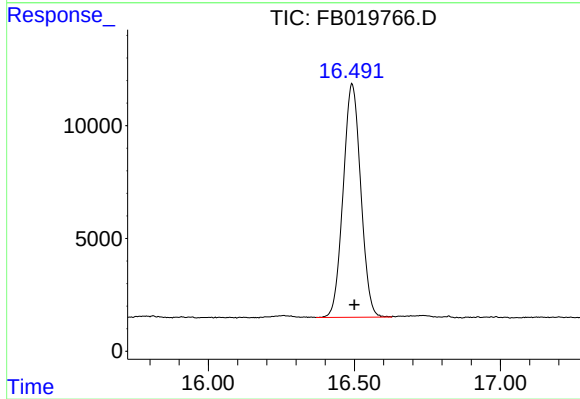

#10 1,2,4-Trimethylbenzene

R.T.: 16.493 min

Delta R.T.: -0.007 min

Response: 432986

Conc: 18.69 ng/ml