

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021519\
 Data File : FB019772.D
 Signal(s) : FID2B.CH
 Acq On : 15 Feb 2019 12:19
 Operator : MJ/SJ
 Sample : K1484-01MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 15 23:15:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.043	217405	18.598 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.897	546701	31.577 ng/ml
2) t 2,2,4-Trimethylpentane	7.657	521257	31.432 ng/ml
3) t n-Heptane	7.998	158324	9.825 ng/ml
4) t Benzene	8.135	195182	10.348 ng/ml
6) t Toluene	10.891	509236	29.112 ng/ml
7) t Ethylbenzene	13.343	207173	9.440 ng/ml
8) t m-Xylene	13.476	436871	19.088 ng/ml
9) t O-Xylene	14.208	417534	18.694 ng/ml
10) t 1,2,4-Trimethylbenzene	16.495	421674	18.199 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021519\
Data File : FB019772.D
Signal(s) : FID2B.CH
Acq On : 15 Feb 2019 12:19
Operator : MJ/SJ
Sample : K1484-01MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 15 23:15:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

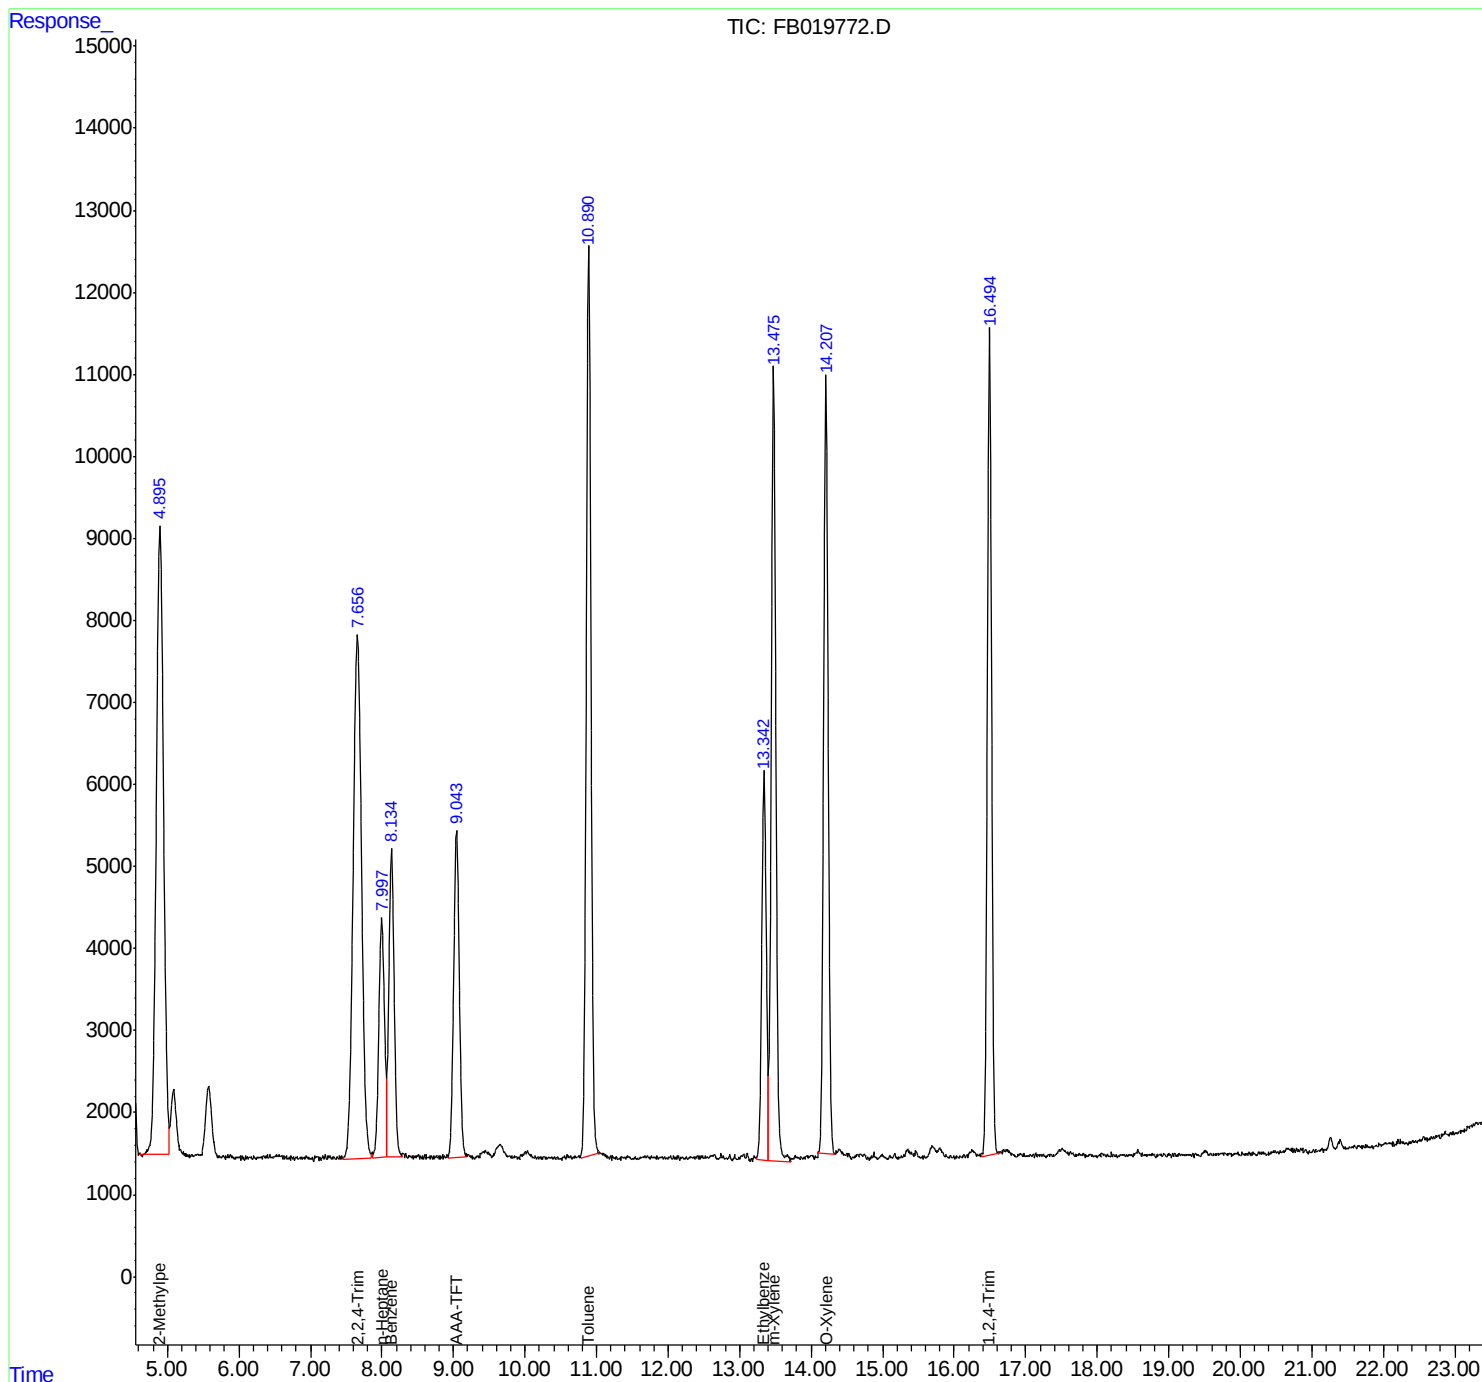

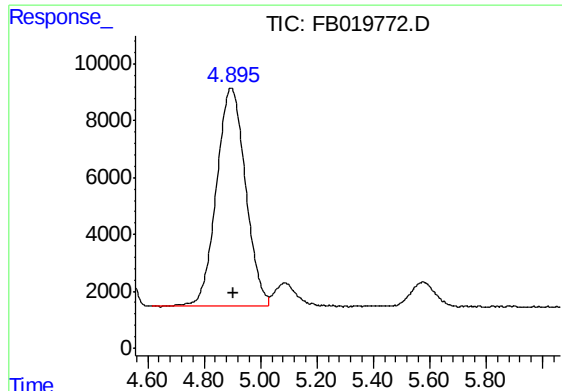


#1 2-Methylpentane

R.T.: 4.897 min
Delta R.T.: -0.005 min
Response: 546701
Conc: 31.58 ng/ml

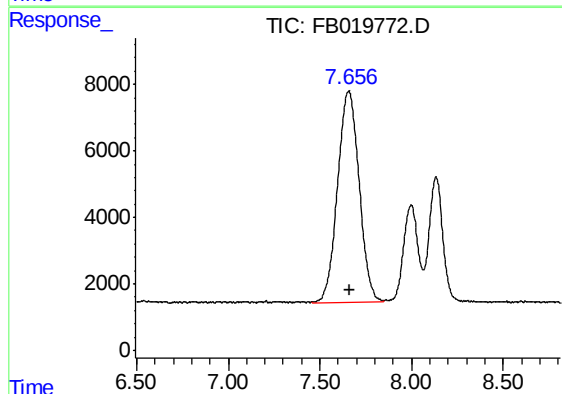


#2 2,2,4-Trimethylpentane

R.T.: 7.657 min
Delta R.T.: -0.007 min
Response: 521257
Conc: 31.43 ng/ml

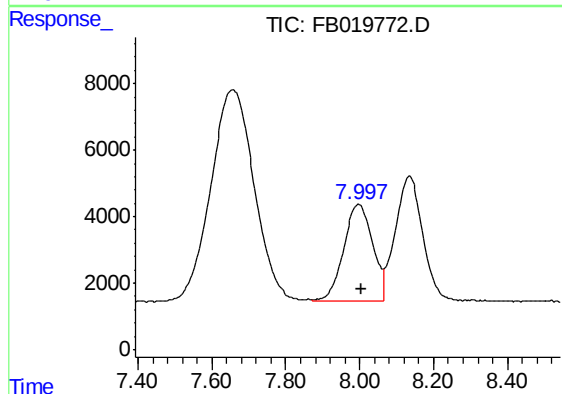


#3 n-Heptane

R.T.: 7.998 min
Delta R.T.: -0.006 min
Response: 158324
Conc: 9.82 ng/ml

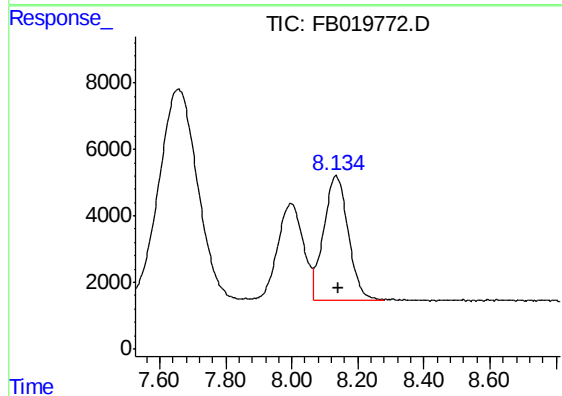


#4 Benzene

R.T.: 8.135 min
Delta R.T.: -0.006 min
Response: 195182
Conc: 10.35 ng/ml

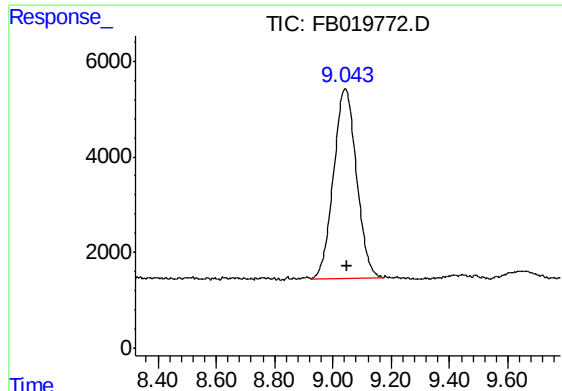


#5 AAA-TFT

R.T.: 9.043 min
Delta R.T.: -0.006 min
Response: 217405
Conc: 18.60 ng/ml

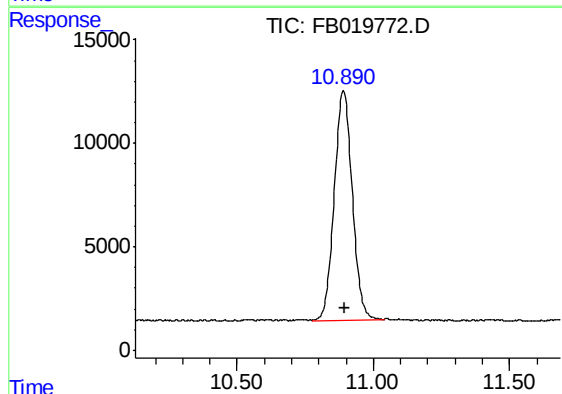


#6 Toluene

R.T.: 10.891 min
Delta R.T.: -0.006 min
Response: 509236
Conc: 29.11 ng/ml

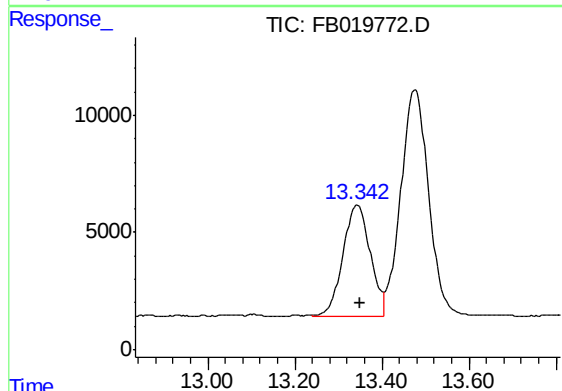


#7 Ethylbenzene

R.T.: 13.343 min
Delta R.T.: -0.005 min
Response: 207173
Conc: 9.44 ng/ml

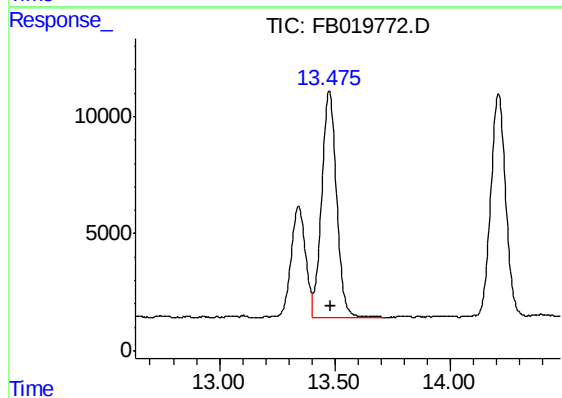


#8 m-Xylene

R.T.: 13.476 min
Delta R.T.: -0.006 min
Response: 436871
Conc: 19.09 ng/ml

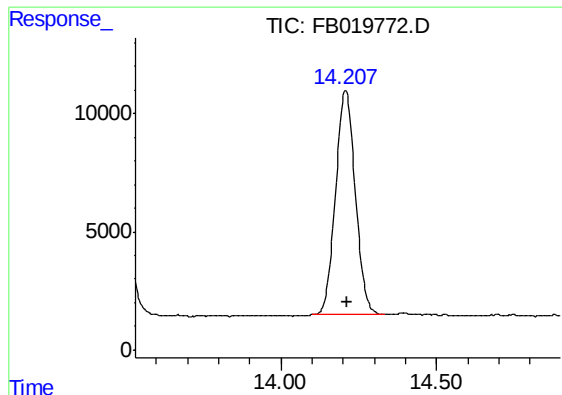

#9 O-Xylene

R.T.: 14.208 min
Delta R.T.: -0.006 min
Response: 417534
Conc: 18.69 ng/ml

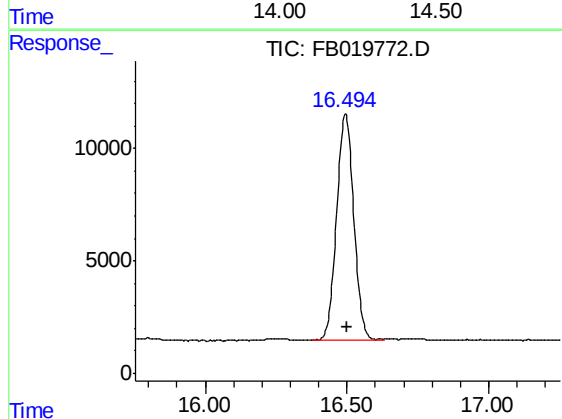

#10 1,2,4-Trimethylbenzene

R.T.: 16.495 min
Delta R.T.: -0.005 min
Response: 421674
Conc: 18.20 ng/ml