

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021523\
 Data File : FB029314.D
 Signal(s) : FID2B.CH
 Acq On : 15 Feb 2023 16:17
 Operator : YP/AJ
 Sample : 01552-19MSD
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 16 03:56:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	180603	18.777 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	441595	27.831 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	480463	27.896 ng/ml
3) t n-Heptane	7.755	173655	9.597 ng/ml
4) t Benzene	7.891	197682	9.490 ng/ml
6) t Toluene	10.624	599108	29.564 ng/ml
7) t Ethylbenzene	13.061	187098	9.803 ng/ml
8) t m-Xylene	13.193	368159	19.420 ng/ml
9) t O-Xylene	13.920	351084	19.242 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	331006	17.589 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021523\
Data File : FB029314.D
Signal(s) : FID2B.CH
Acq On : 15 Feb 2023 16:17
Operator : YP/AJ
Sample : 01552-19MSD
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 16 03:56:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

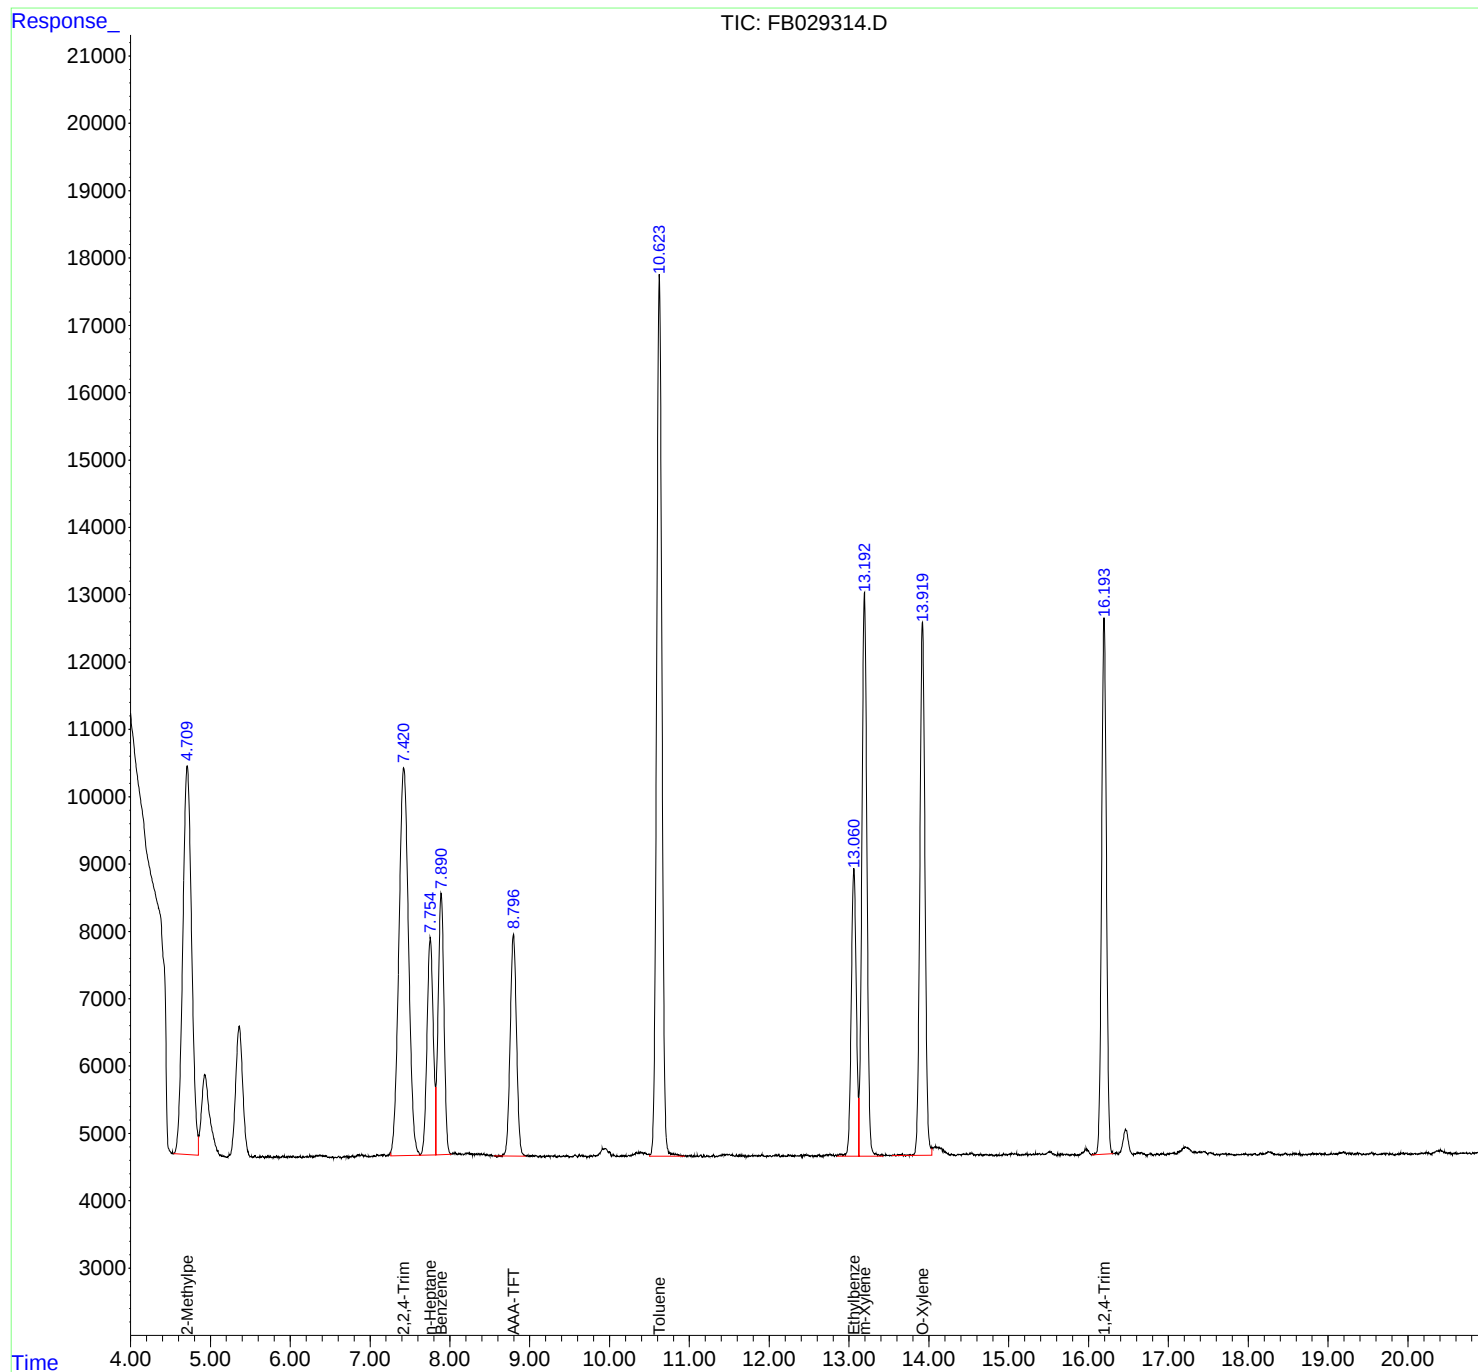

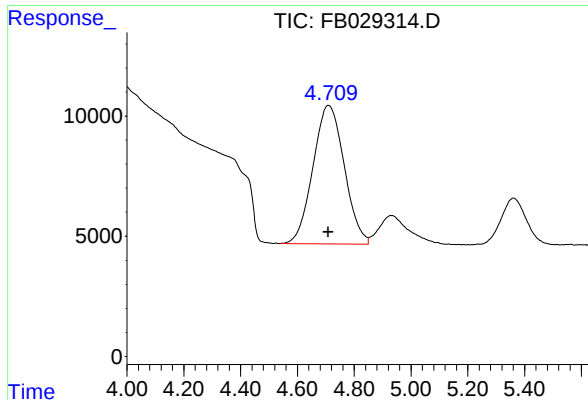


#1 2-Methylpentane

R.T.: 4.711 min
Delta R.T.: 0.002 min
Response: 441595
Conc: 27.83 ng/ml

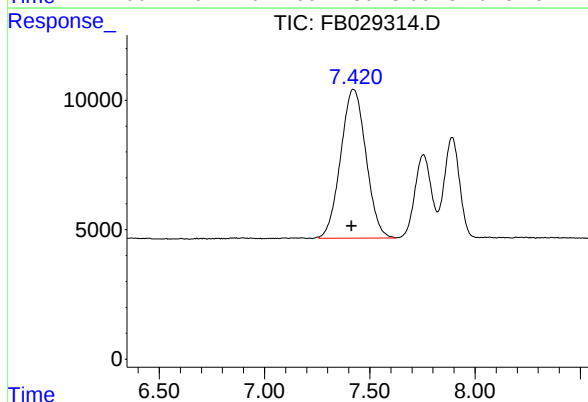


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.007 min
Response: 480463
Conc: 27.90 ng/ml

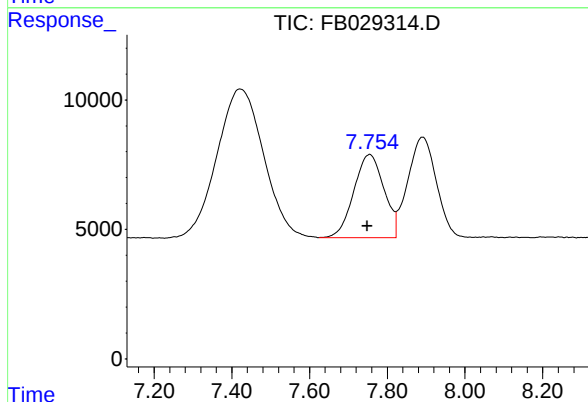


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.006 min
Response: 173655
Conc: 9.60 ng/ml

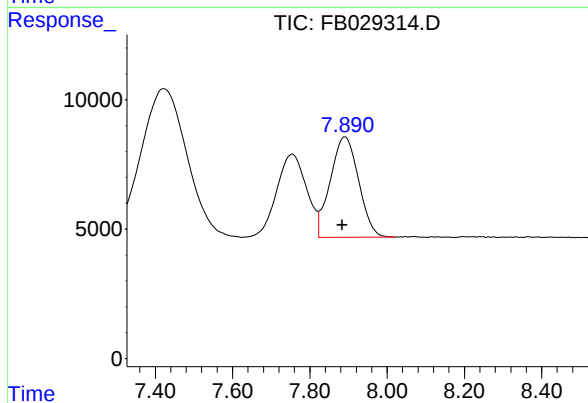


#4 Benzene

R.T.: 7.891 min
Delta R.T.: 0.006 min
Response: 197682
Conc: 9.49 ng/ml

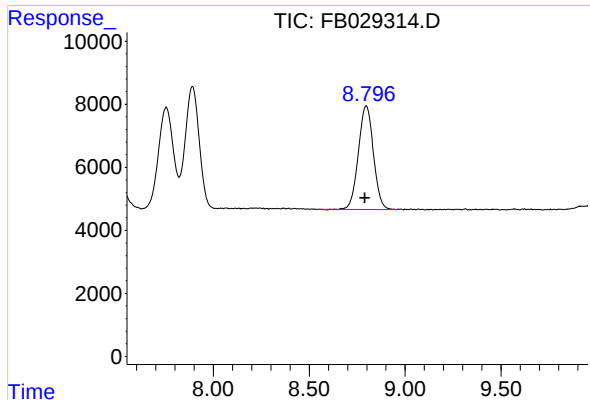


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.008 min
Response: 180603
Conc: 18.78 ng/ml

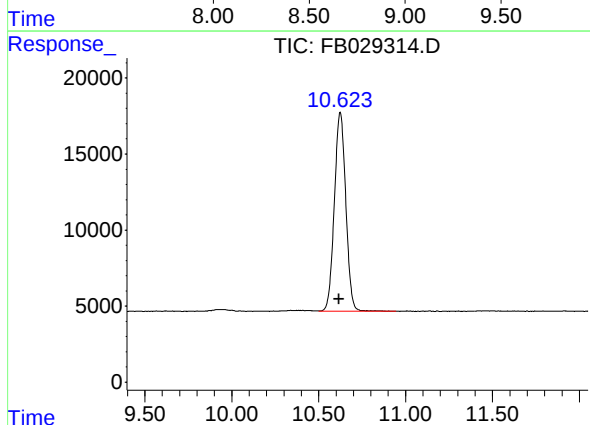


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.007 min
Response: 599108
Conc: 29.56 ng/ml

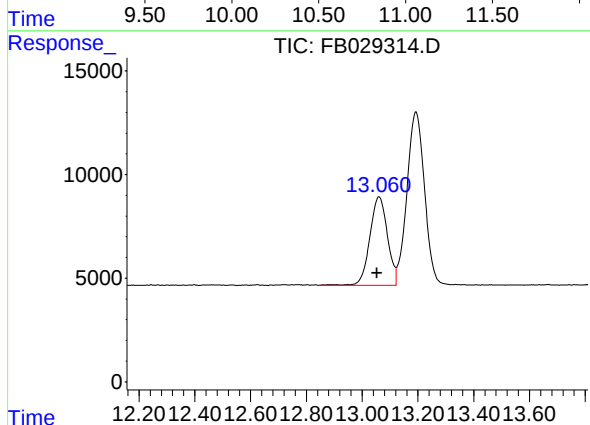


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: 0.007 min
Response: 187098
Conc: 9.80 ng/ml

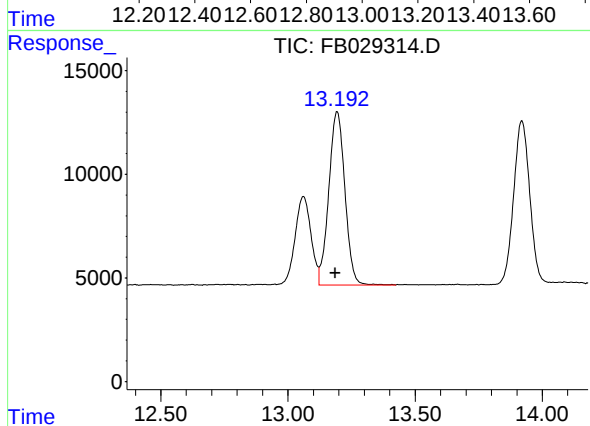


#8 m-Xylene

R.T.: 13.193 min
Delta R.T.: 0.007 min
Response: 368159
Conc: 19.42 ng/ml

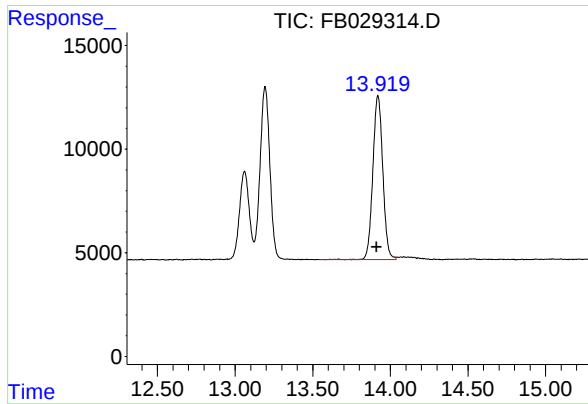

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.007 min
Response: 351084
Conc: 19.24 ng/ml

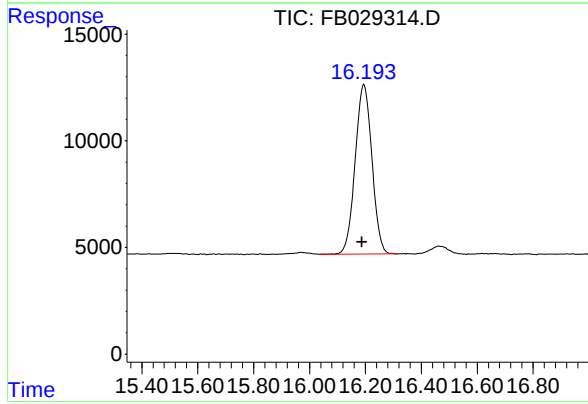

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.007 min
Response: 331006
Conc: 17.59 ng/ml