

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021523\
 Data File : FB029306.D
 Signal(s) : FID2B.CH
 Acq On : 15 Feb 2023 11:19
 Operator : YP/AJ
 Sample : BSF0215S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 16 03:55:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	195380	20.313 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	461542	29.088 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	504604	29.297 ng/ml
3) t n-Heptane	7.749	174664	9.653 ng/ml
4) t Benzene	7.886	202164	9.706 ng/ml
6) t Toluene	10.618	603378	29.774 ng/ml
7) t Ethylbenzene	13.055	190925	10.003 ng/ml
8) t m-Xylene	13.187	376999	19.886 ng/ml
9) t O-Xylene	13.914	364455	19.975 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	370379	19.681 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021523\
Data File : FB029306.D
Signal(s) : FID2B.CH
Acq On : 15 Feb 2023 11:19
Operator : YP/AJ
Sample : BSF0215S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 16 03:55:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

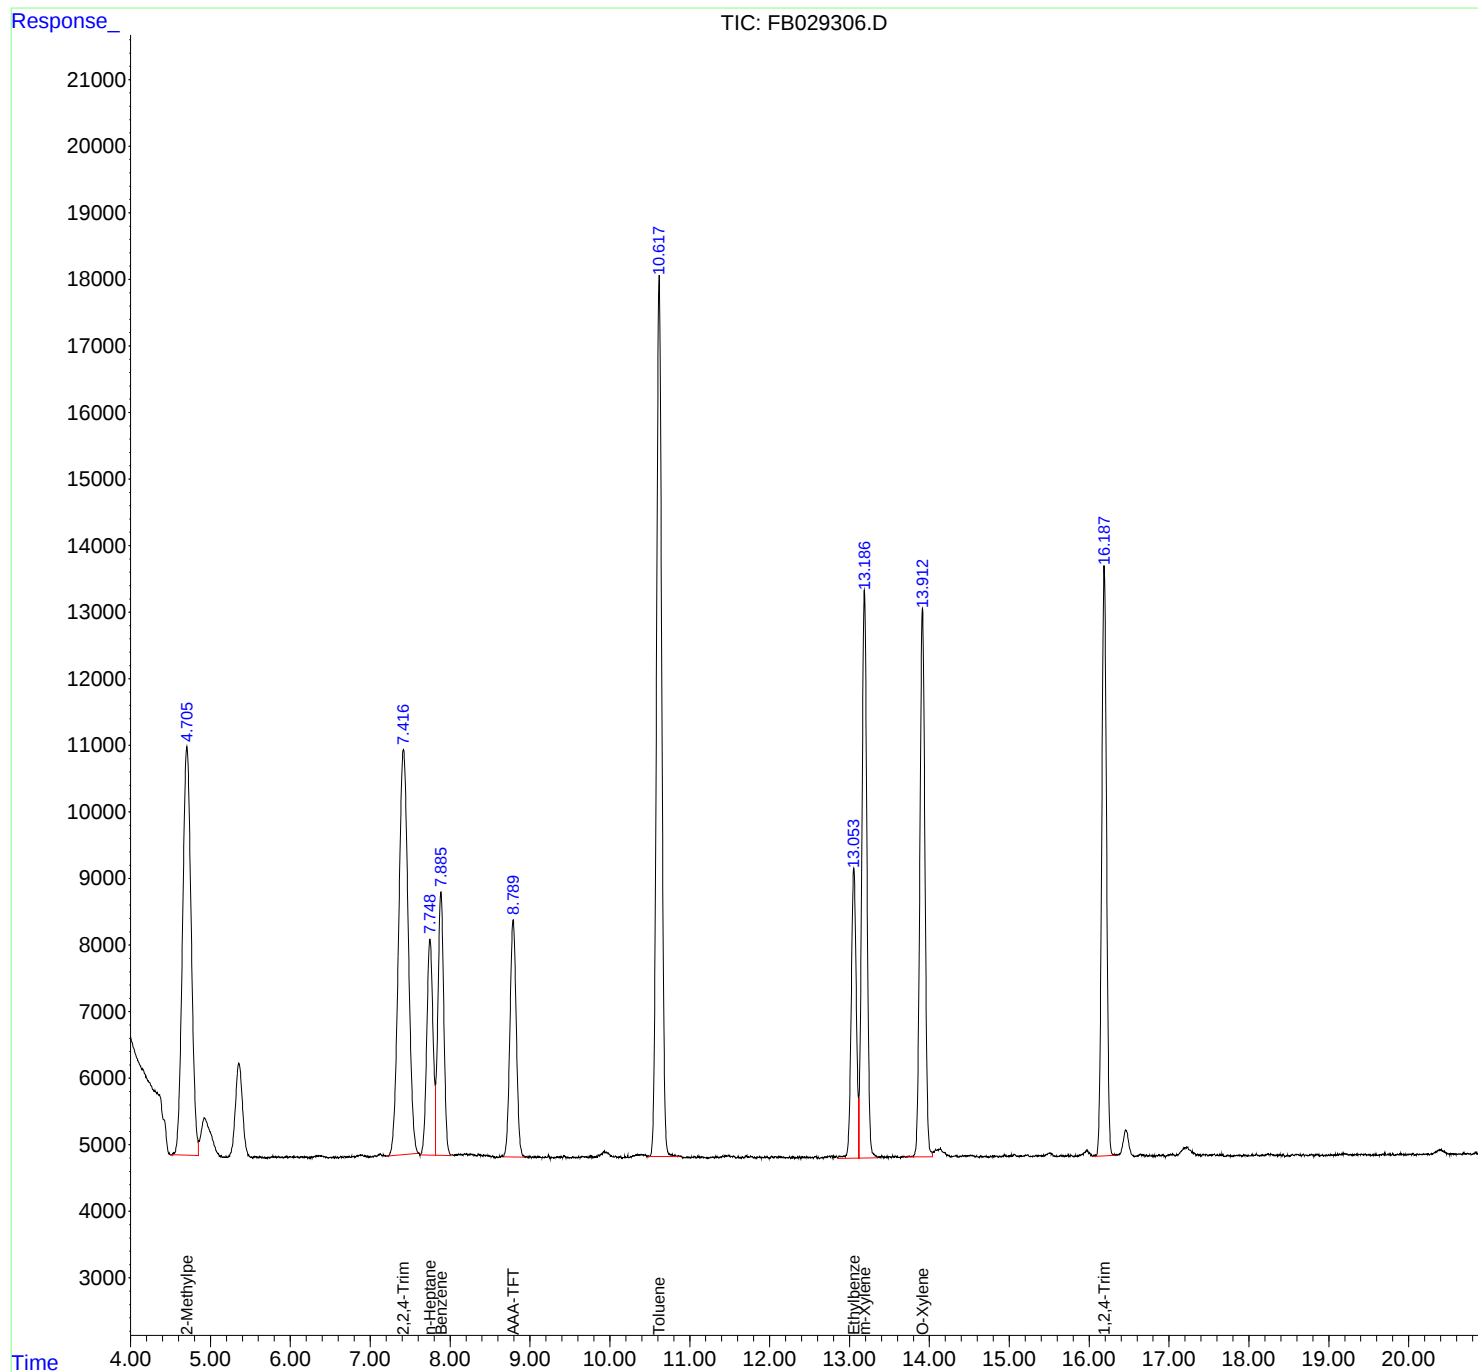

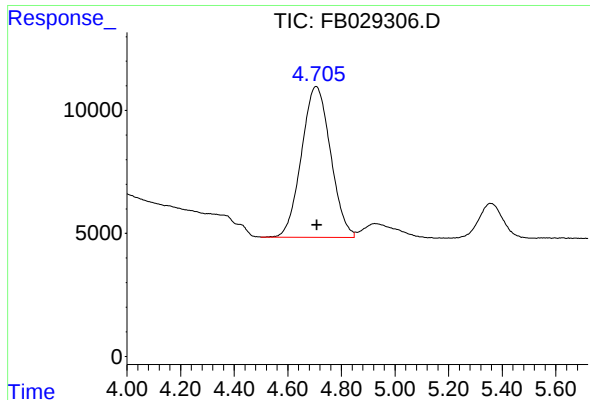


#1 2-Methylpentane

R.T.: 4.706 min
Delta R.T.: -0.003 min
Response: 461542
Conc: 29.09 ng/ml

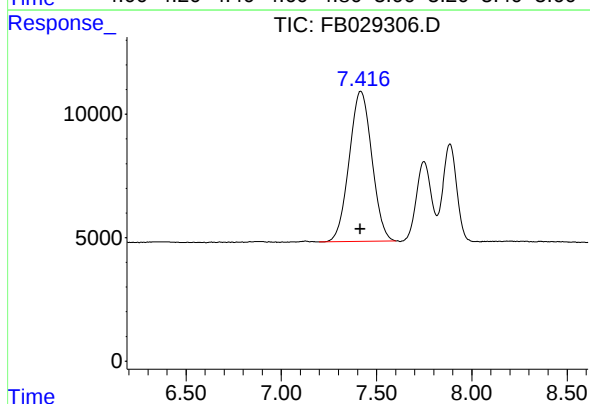


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.003 min
Response: 504604
Conc: 29.30 ng/ml

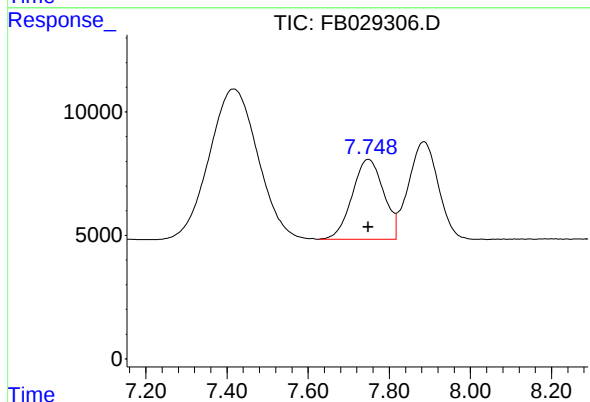


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 174664
Conc: 9.65 ng/ml

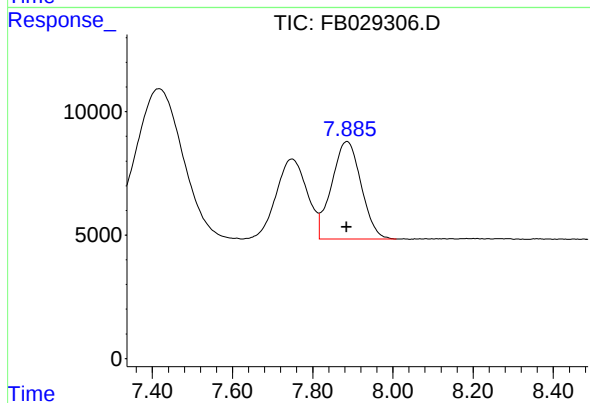


#4 Benzene

R.T.: 7.886 min
Delta R.T.: 0.001 min
Response: 202164
Conc: 9.71 ng/ml

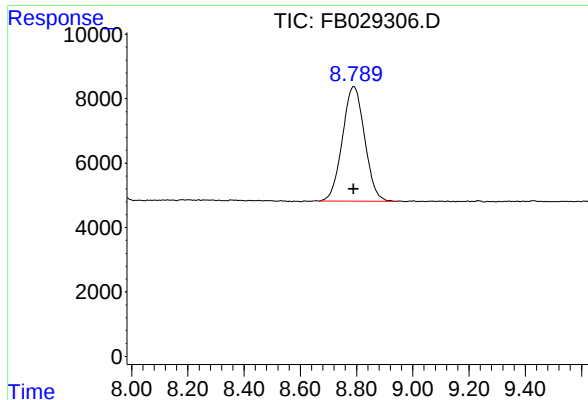


#5 AAA-TFT

R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 195380
Conc: 20.31 ng/ml

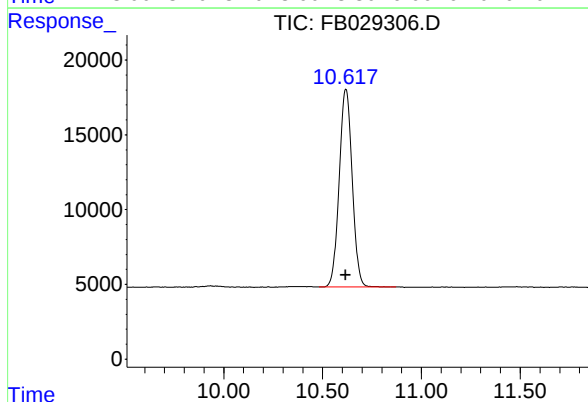


#6 Toluene

R.T.: 10.618 min
Delta R.T.: 0.000 min
Response: 603378
Conc: 29.77 ng/ml

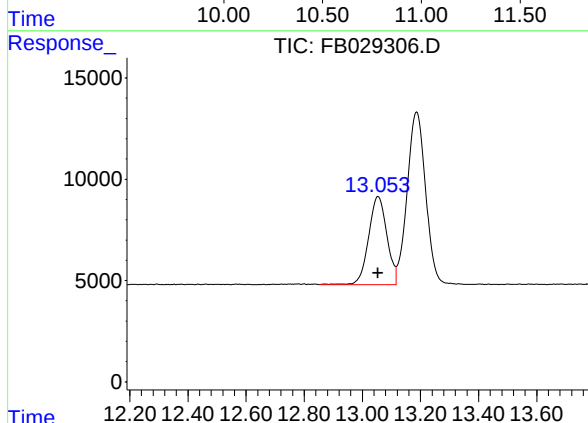


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: 0.000 min
Response: 190925
Conc: 10.00 ng/ml

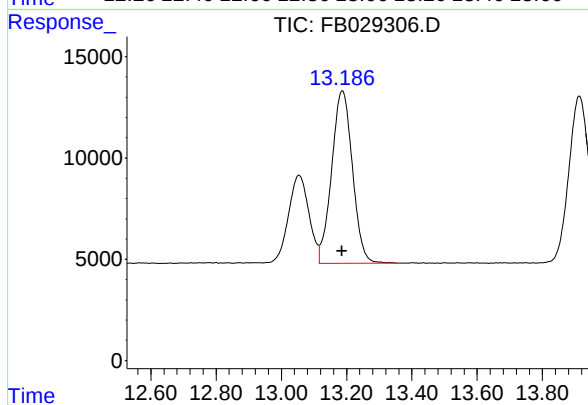


#8 m-Xylene

R.T.: 13.187 min
Delta R.T.: 0.001 min
Response: 376999
Conc: 19.89 ng/ml

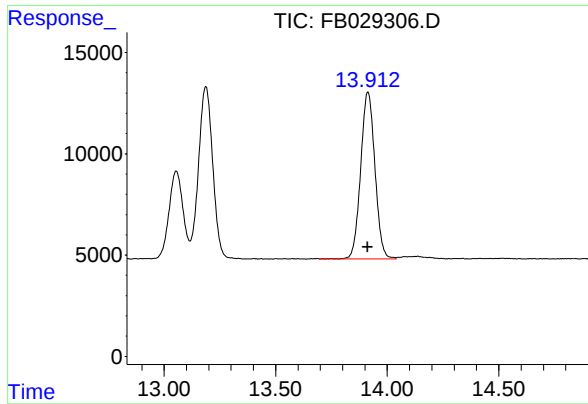

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: 0.001 min
Response: 364455
Conc: 19.97 ng/ml

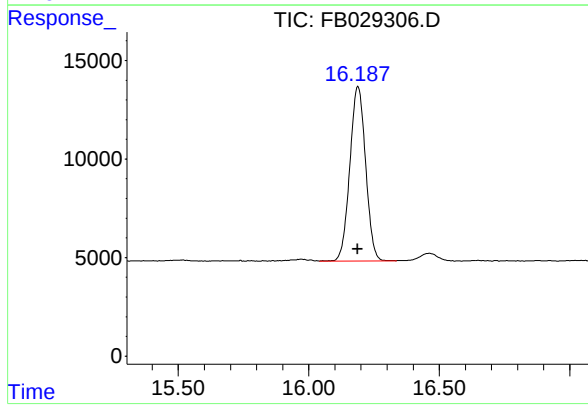

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: 0.000 min
Response: 370379
Conc: 19.68 ng/ml