

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021524\
 Data File : FB030594.D
 Signal(s) : FID2B.CH
 Acq On : 15 Feb 2024 17:39
 Operator : YP/AJ
 Sample : BSF021553
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 16 05:48:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021324.M
 Quant Title :
 QLast Update : Wed Feb 14 09:51:13 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	209112	18.947 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	317369	23.205 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	373100	23.828 ng/ml
3) t n-Heptane	7.744	114756	8.120 ng/ml
4) t Benzene	7.881	173651	8.636 ng/ml
6) t Toluene	10.613	510510	25.751 ng/ml
7) t Ethylbenzene	13.051	160771	8.480 ng/ml
8) t m-Xylene	13.183	319136	16.781 ng/ml
9) t O-Xylene	13.910	308147	16.246 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	302161	15.941 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021524\
Data File : FB030594.D
Signal(s) : FID2B.CH
Acq On : 15 Feb 2024 17:39
Operator : YP/AJ
Sample : BSF0215S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 16 05:48:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021324.M
Quant Title :
QLast Update : Wed Feb 14 09:51:13 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

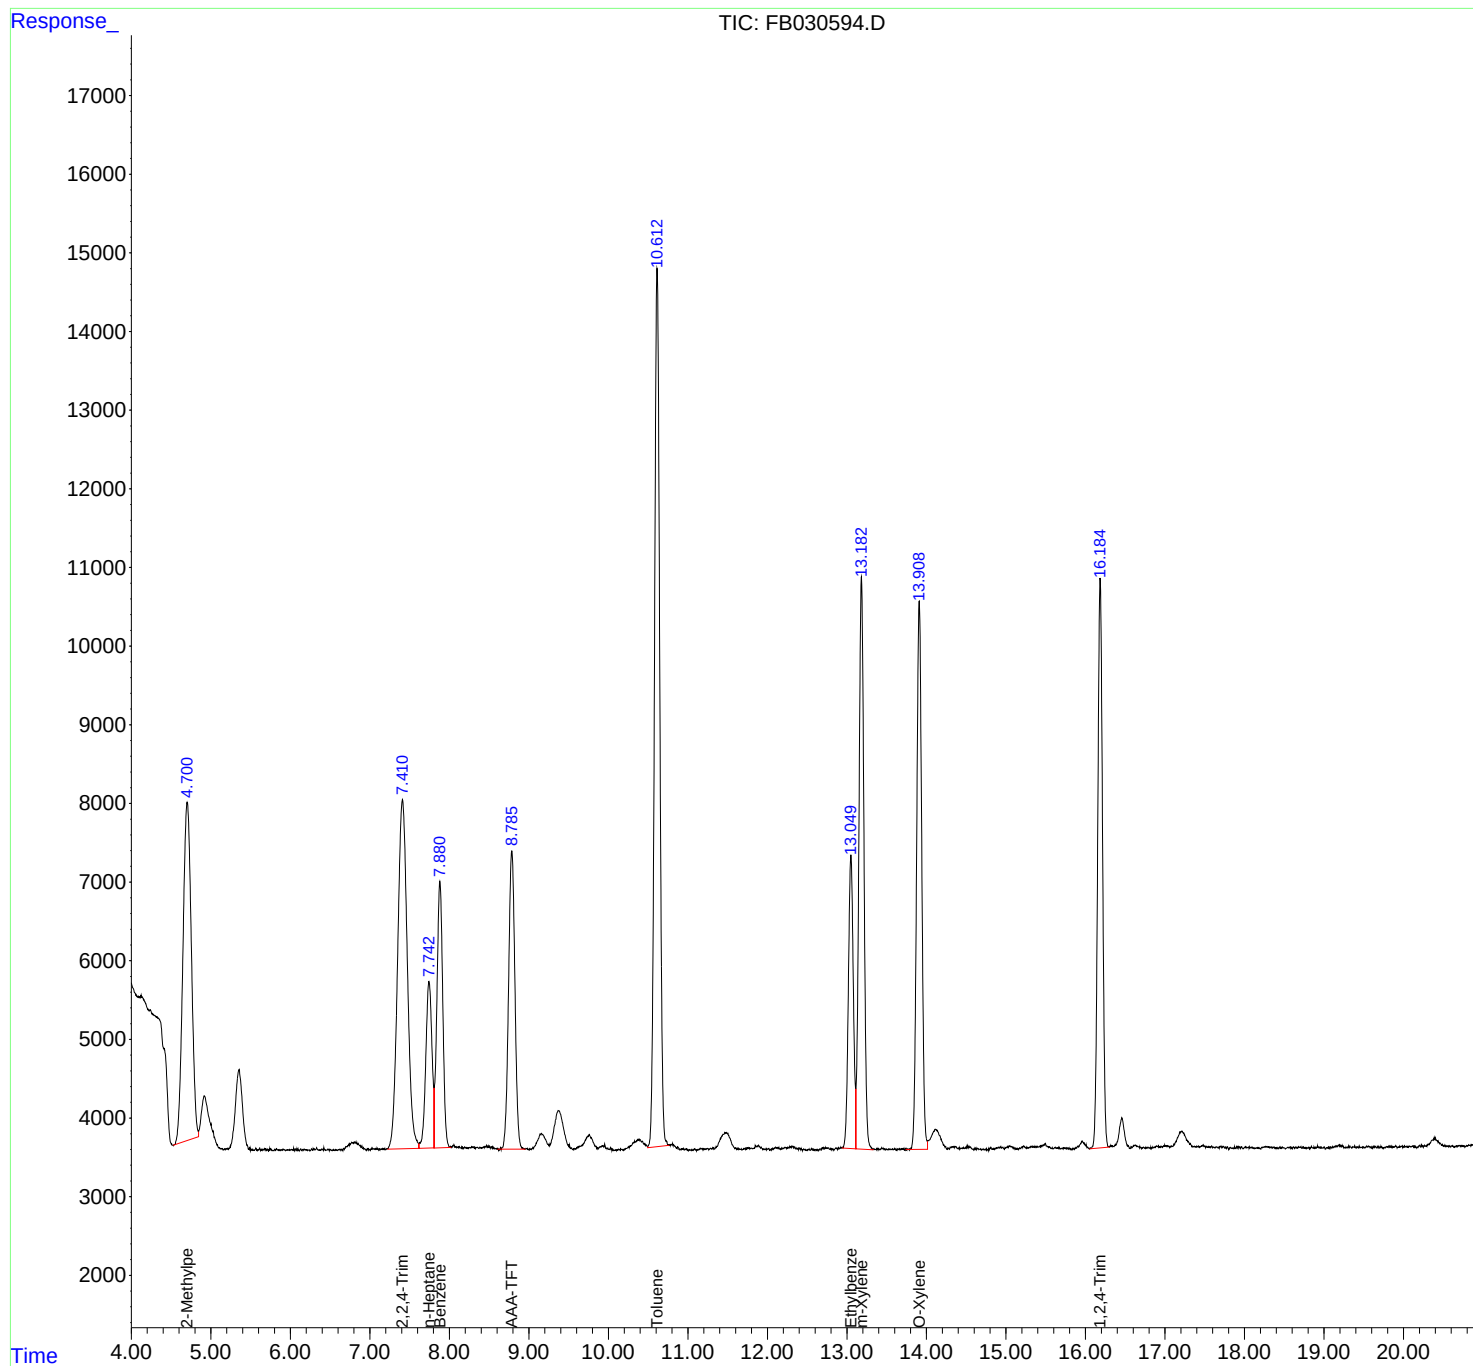

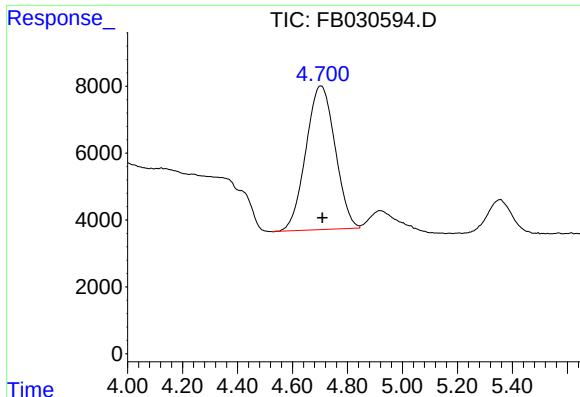


#1 2-Methylpentane

R.T.: 4.702 min
Delta R.T.: -0.007 min
Response: 317369
Conc: 23.20 ng/ml

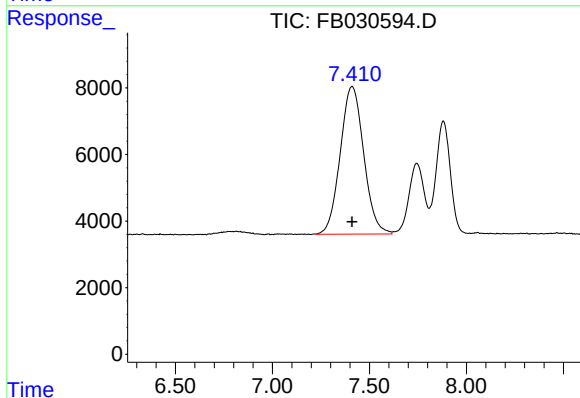


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: 0.001 min
Response: 373100
Conc: 23.83 ng/ml

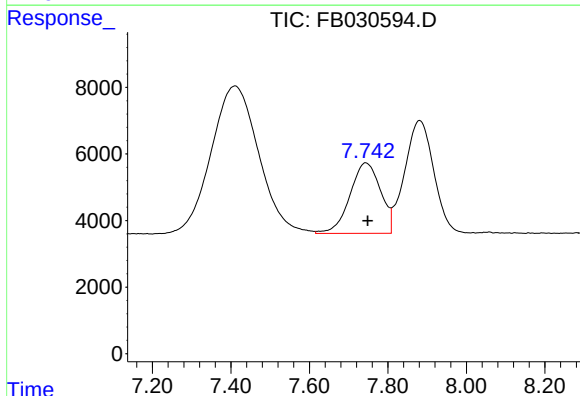


#3 n-Heptane

R.T.: 7.744 min
Delta R.T.: -0.005 min
Response: 114756
Conc: 8.12 ng/ml

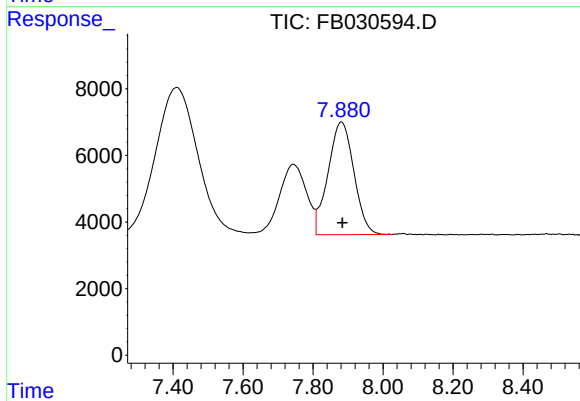


#4 Benzene

R.T.: 7.881 min
Delta R.T.: -0.002 min
Response: 173651
Conc: 8.64 ng/ml

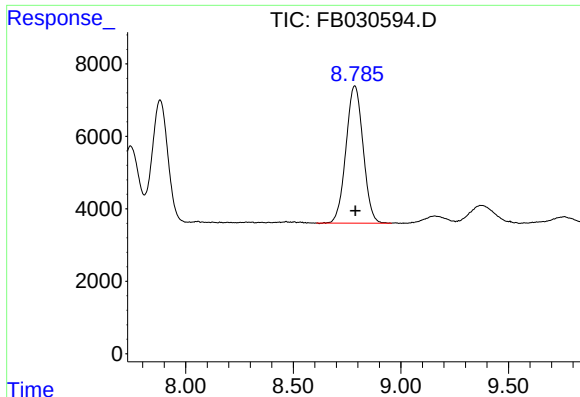


#5 AAA-TFT

R.T.: 8.786 min
Delta R.T.: -0.003 min
Response: 209112
Conc: 18.95 ng/ml

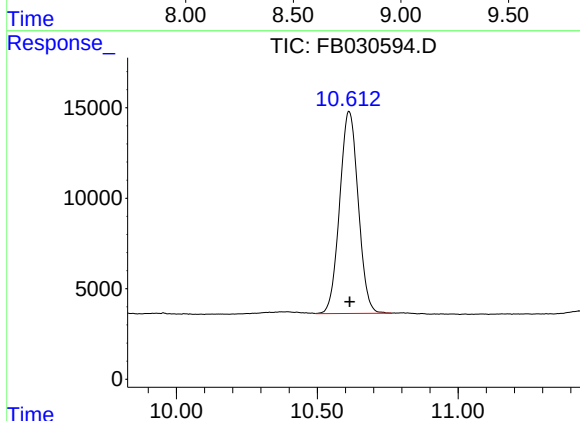


#6 Toluene

R.T.: 10.613 min
Delta R.T.: -0.002 min
Response: 510510
Conc: 25.75 ng/ml

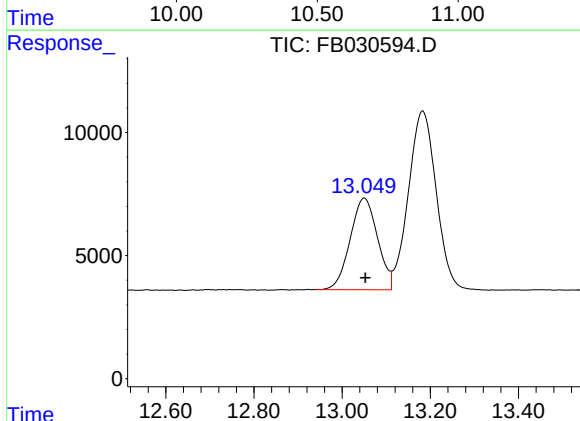


#7 Ethylbenzene

R.T.: 13.051 min
Delta R.T.: -0.002 min
Response: 160771
Conc: 8.48 ng/ml

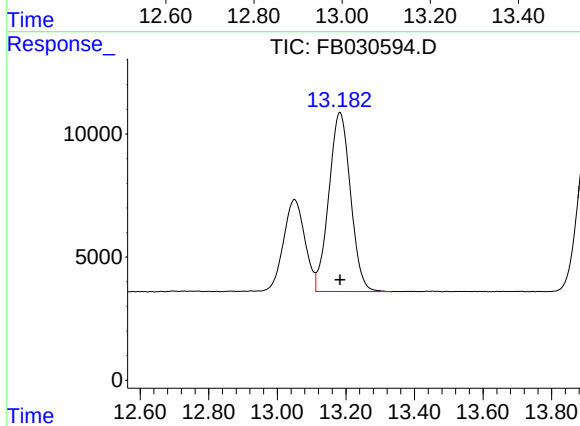


#8 m-Xylene

R.T.: 13.183 min
Delta R.T.: 0.000 min
Response: 319136
Conc: 16.78 ng/ml

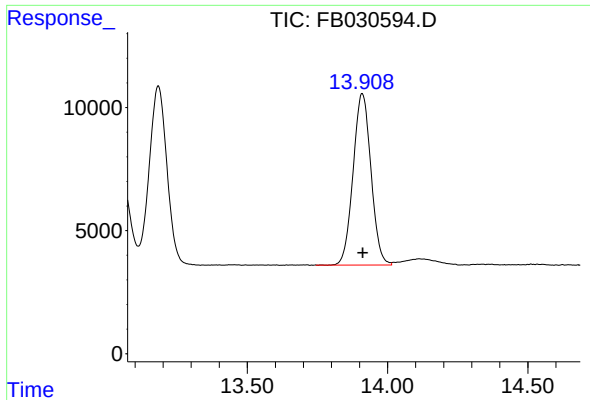

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: -0.002 min
Response: 308147
Conc: 16.25 ng/ml

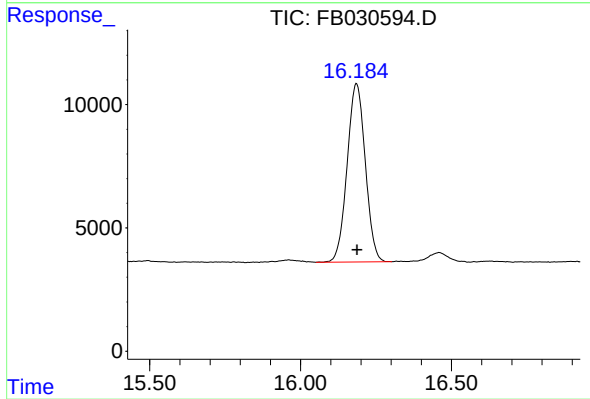

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: -0.001 min
Response: 302161
Conc: 15.94 ng/ml