

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021720\
 Data File : FB023675.D
 Signal(s) : FID2B.CH
 Acq On : 17 Feb 2020 10:46
 Operator : DD/AJ
 Sample : BSF0214S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 18 00:20:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	406279	19.955 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	875854	29.108 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	1004793	30.792 ng/ml
3) t n-Heptane	7.752	319547	9.932 ng/ml
4) t Benzene	7.887	399929	9.778 ng/ml
6) t Toluene	10.625	1176292	29.633 ng/ml
7) t Ethylbenzene	13.065	366815	9.867 ng/ml
8) t m-Xylene	13.198	706949	19.796 ng/ml
9) t O-Xylene	13.926	679461	19.701 ng/ml
10) t 1,2,4-Trimethylbenzene	16.204	589751	20.143 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021720\
Data File : FB023675.D
Signal(s) : FID2B.CH
Acq On : 17 Feb 2020 10:46
Operator : DD/AJ
Sample : BSF0214S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 18 00:20:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

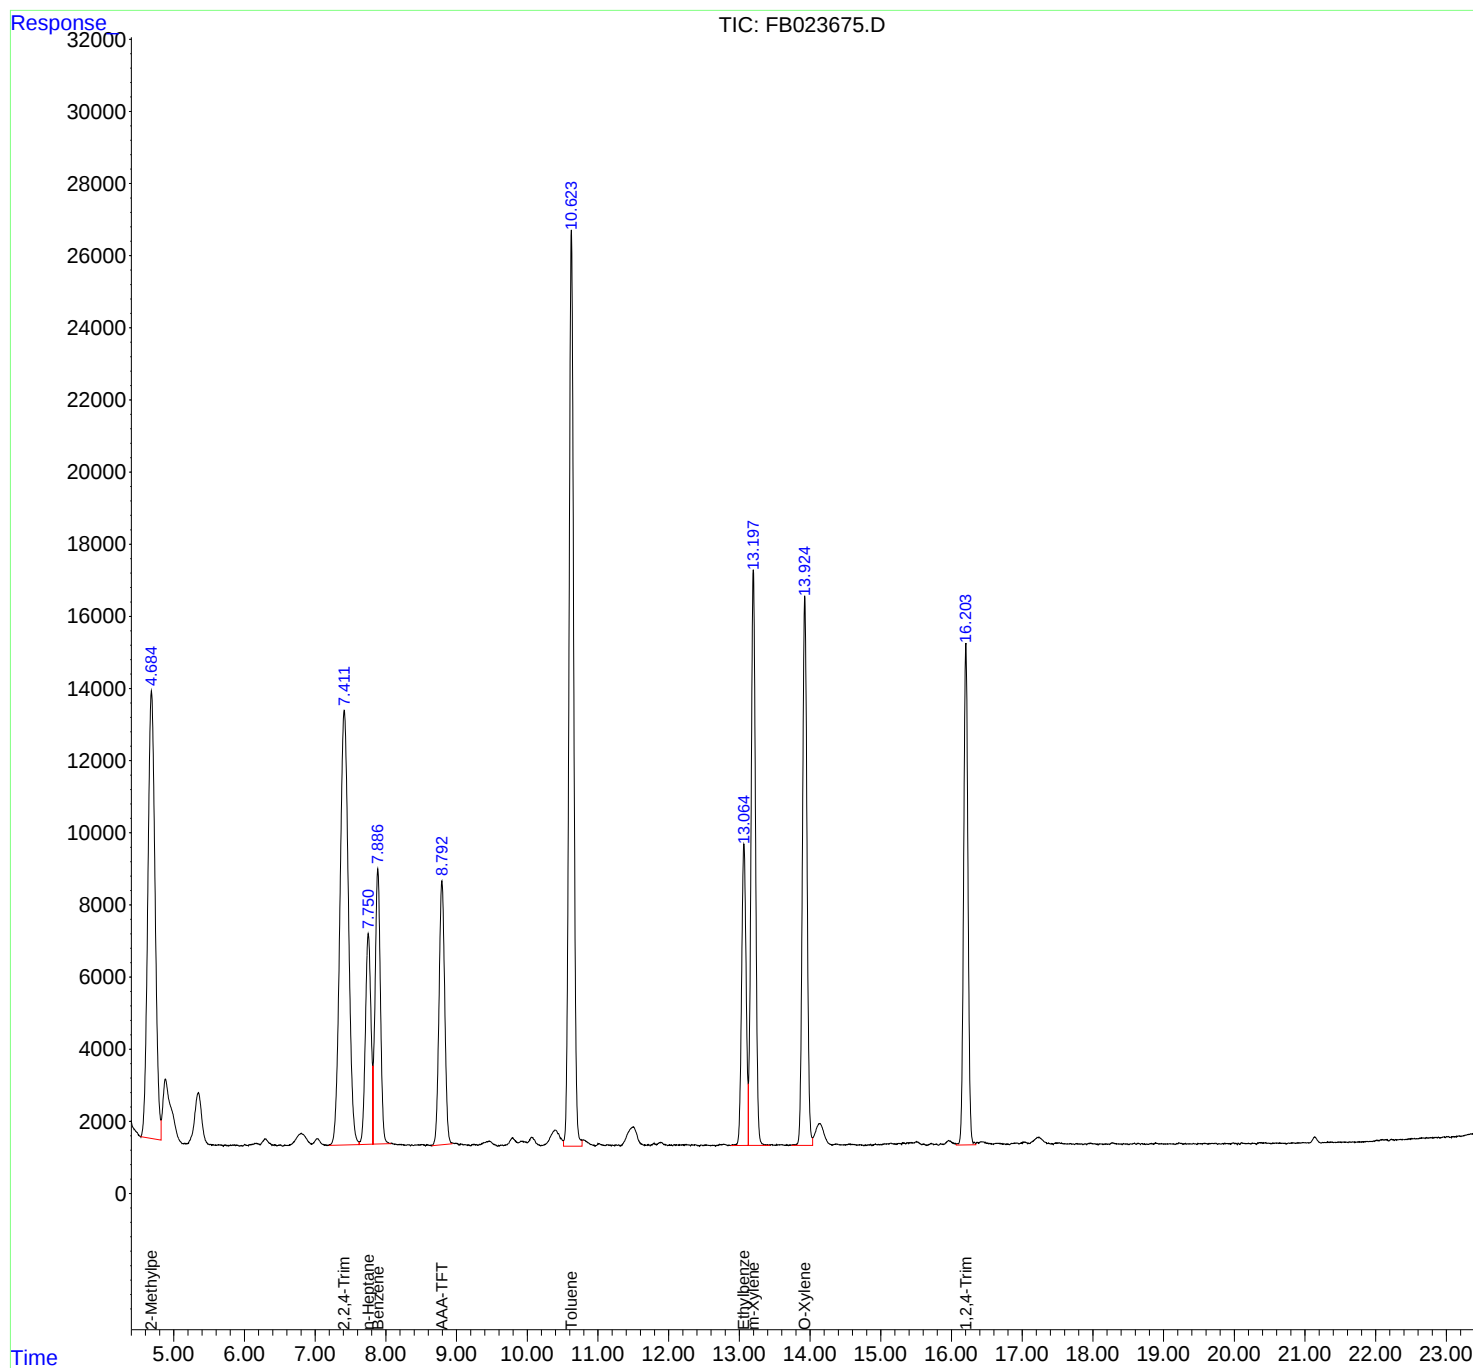

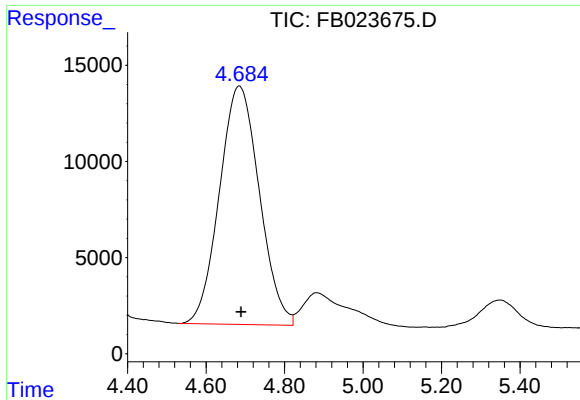


#1 2-Methylpentane

R.T.: 4.685 min
Delta R.T.: -0.004 min
Response: 875854
Conc: 29.11 ng/ml

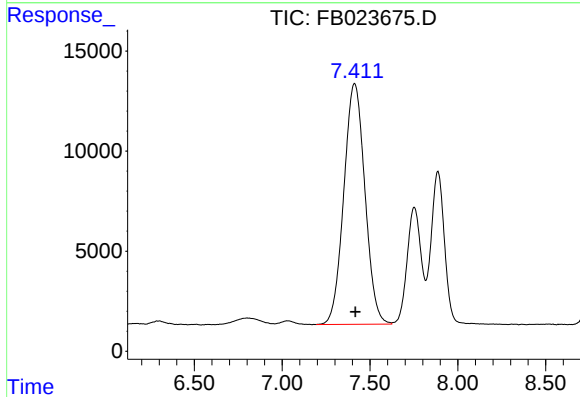


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.006 min
Response: 1004793
Conc: 30.79 ng/ml

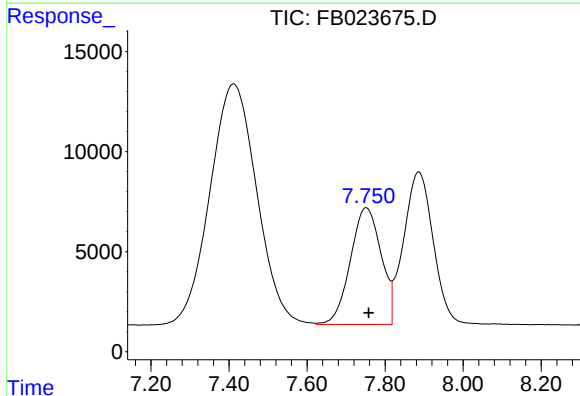


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.006 min
Response: 319547
Conc: 9.93 ng/ml

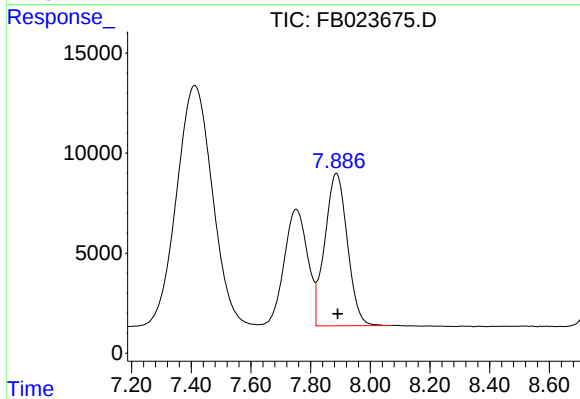


#4 Benzene

R.T.: 7.887 min
Delta R.T.: -0.005 min
Response: 399929
Conc: 9.78 ng/ml

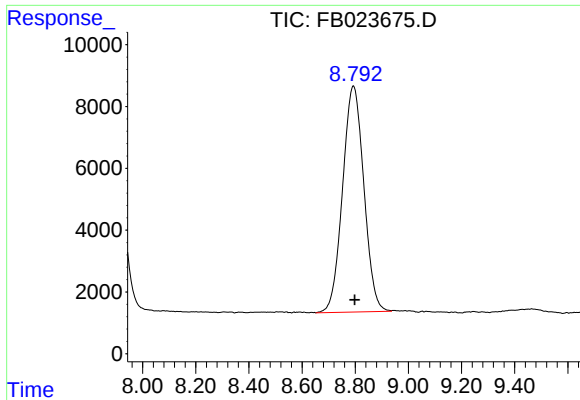


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: -0.005 min
Response: 406279
Conc: 19.96 ng/ml

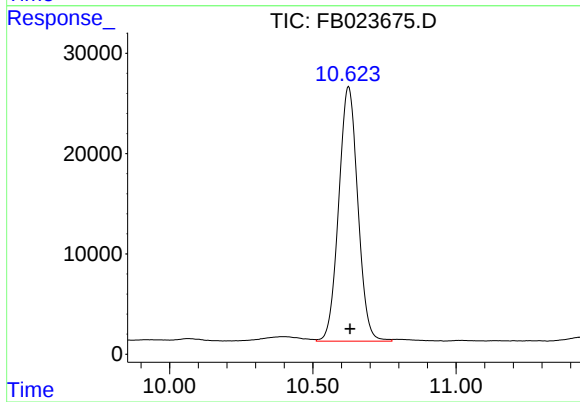


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.005 min
Response: 1176292
Conc: 29.63 ng/ml

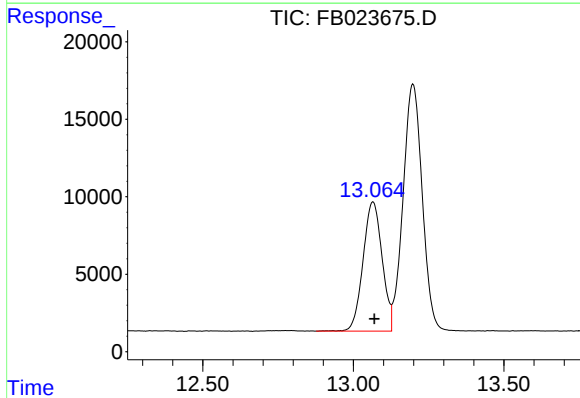


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.005 min
Response: 366815
Conc: 9.87 ng/ml

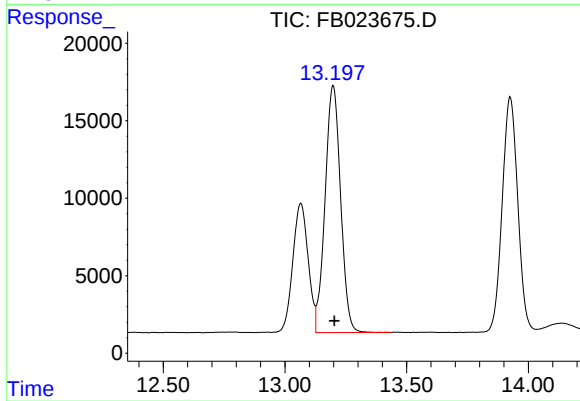


#8 m-Xylene

R.T.: 13.198 min
Delta R.T.: -0.005 min
Response: 706949
Conc: 19.80 ng/ml

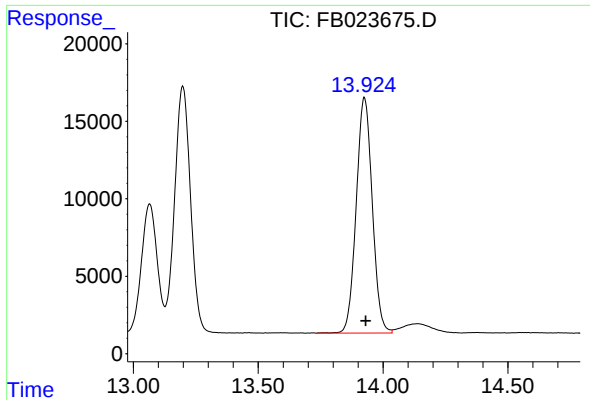

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: -0.005 min
Response: 679461
Conc: 19.70 ng/ml

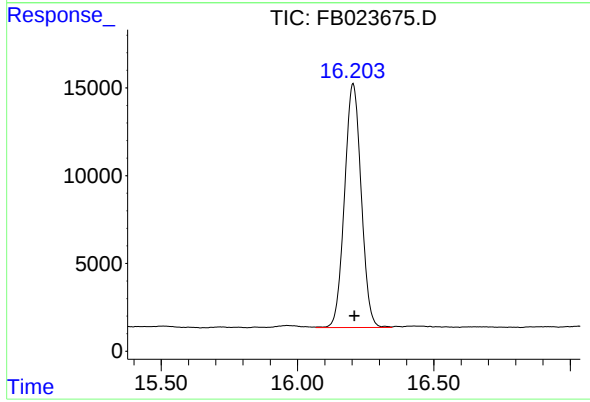

#10 1,2,4-Trimethylbenzene

R.T.: 16.204 min
Delta R.T.: -0.005 min
Response: 589751
Conc: 20.14 ng/ml