

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021722\
 Data File : FB026632.D
 Signal(s) : FID2B.CH
 Acq On : 17 Feb 2022 11:55
 Operator : AJ/MA
 Sample : BSF0217S1
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 17 12:48:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021122.M
 Quant Title :
 QLast Update : Fri Feb 11 12:15:14 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	257625	24.944 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	552114	35.452 ng/ml
2) t 2,2,4-Trimethylpentane	7.439	624514	34.301 ng/ml
3) t n-Heptane	7.750	203317	11.475 ng/ml
4) t Benzene	7.886	235975	11.557 ng/ml
6) t Toluene	10.619	681532	34.705 ng/ml
7) t Ethylbenzene	13.056	207273	11.223 ng/ml
8) t m-Xylene	13.189	411820	22.345 ng/ml
9) t O-Xylene	13.916	394114	21.916 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	389201	21.078 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021722\
Data File : FB026632.D
Signal(s) : FID2B.CH
Acq On : 17 Feb 2022 11:55
Operator : AJ/MA
Sample : BSF0217S1
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 17 12:48:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021122.M
Quant Title :
QLast Update : Fri Feb 11 12:15:14 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

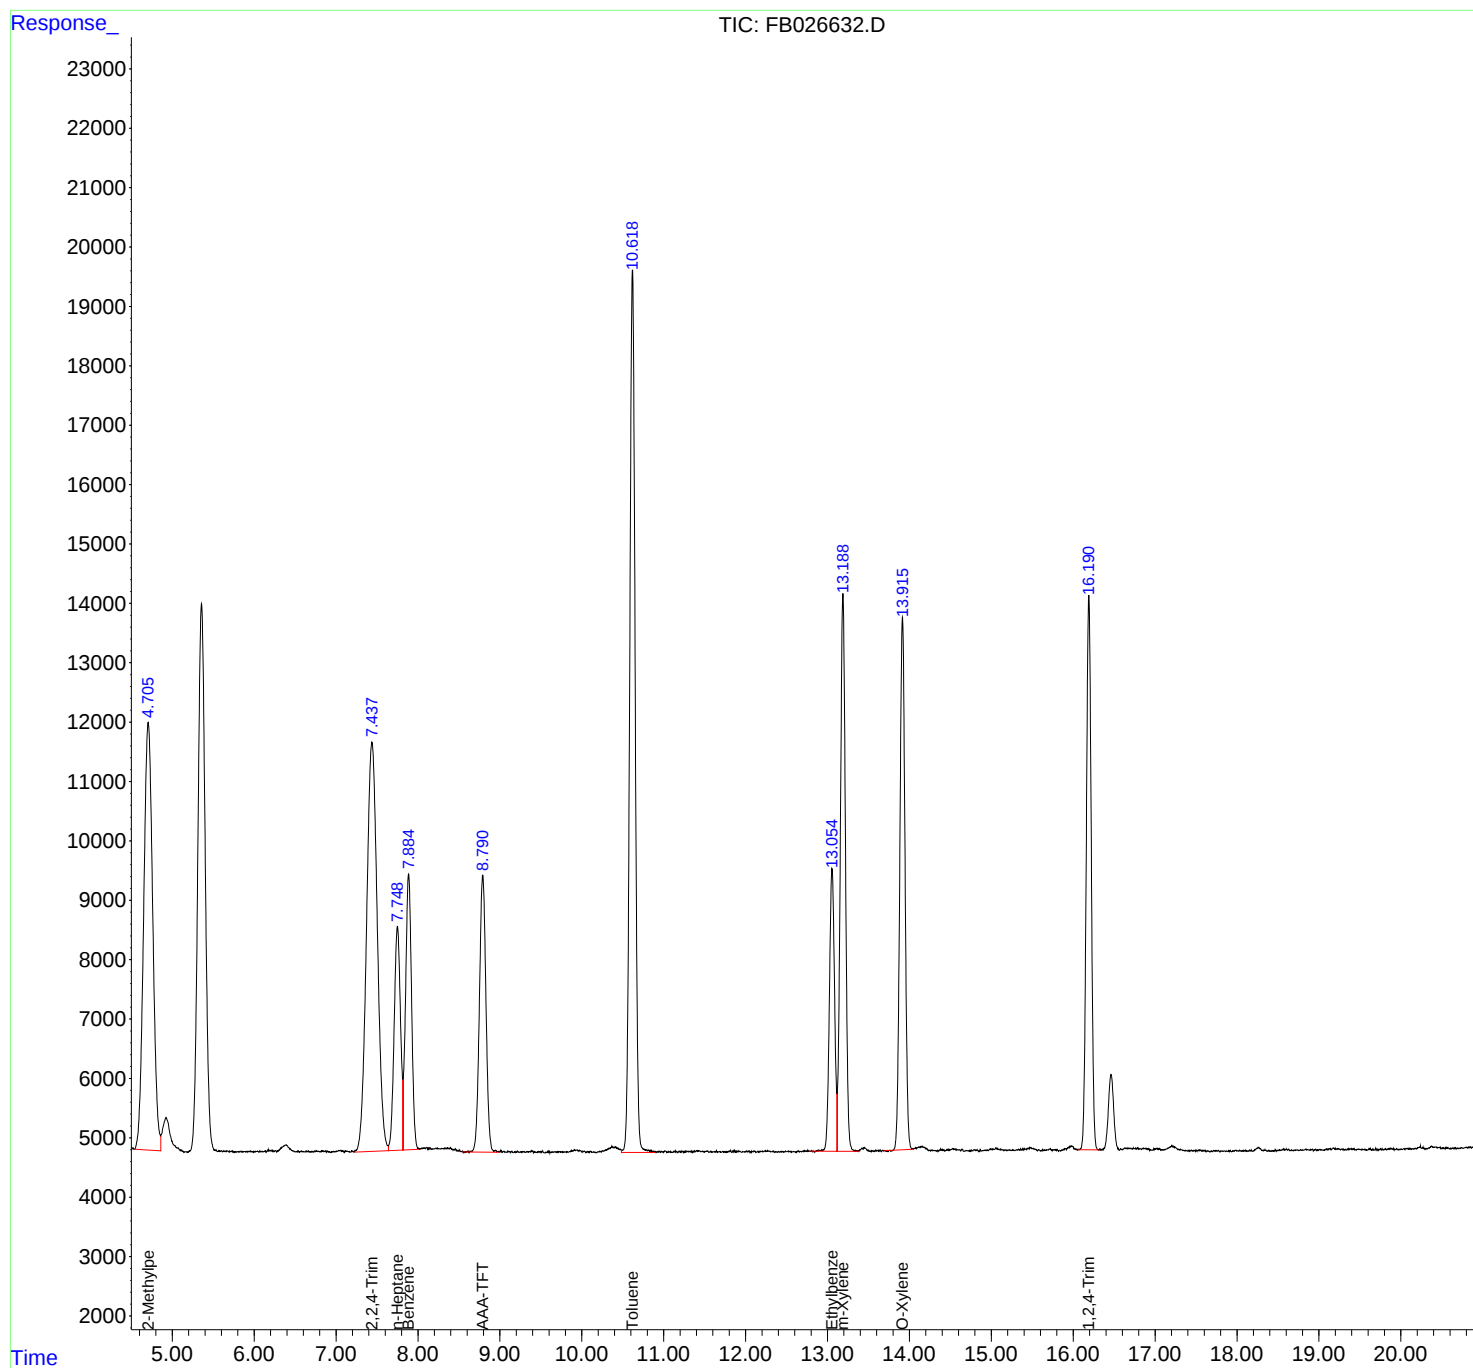

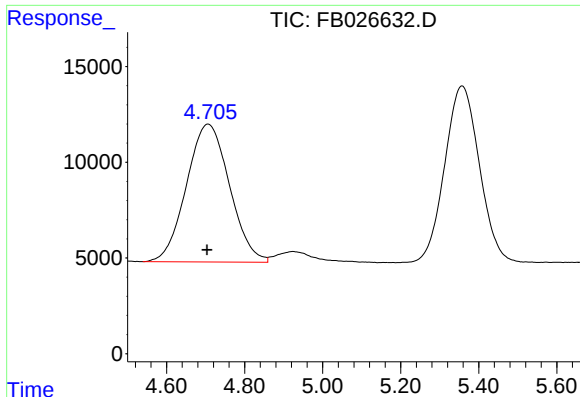


#1 2-Methylpentane

R.T.: 4.707 min
Delta R.T.: 0.003 min
Response: 552114
Conc: 35.45 ng/ml

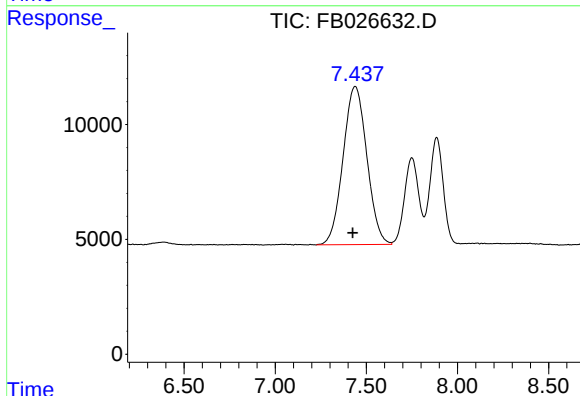


#2 2,2,4-Trimethylpentane

R.T.: 7.439 min
Delta R.T.: 0.013 min
Response: 624514
Conc: 34.30 ng/ml

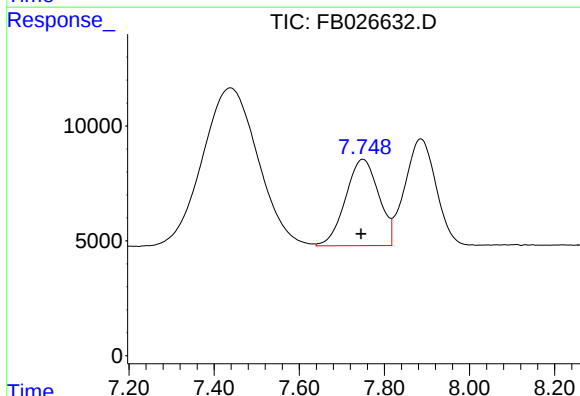


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.005 min
Response: 203317
Conc: 11.48 ng/ml

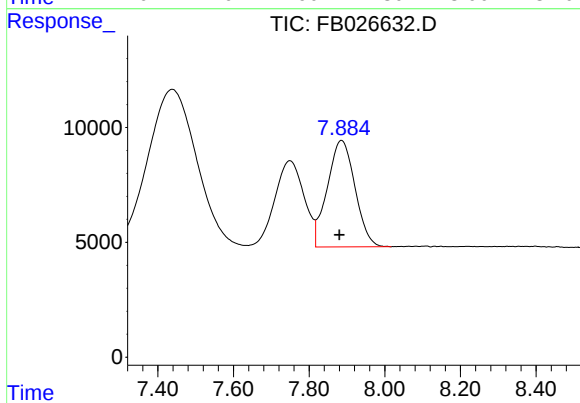


#4 Benzene

R.T.: 7.886 min
Delta R.T.: 0.006 min
Response: 235975
Conc: 11.56 ng/ml

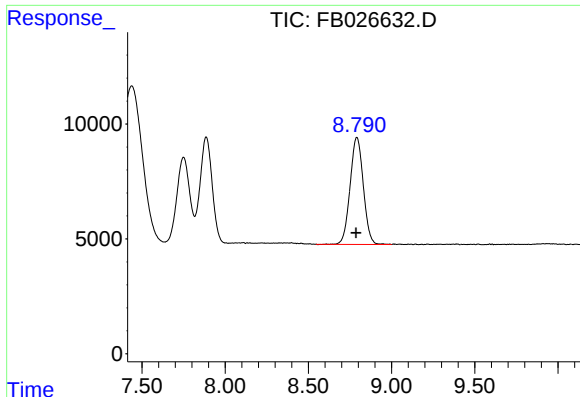


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.005 min
Response: 257625
Conc: 24.94 ng/ml

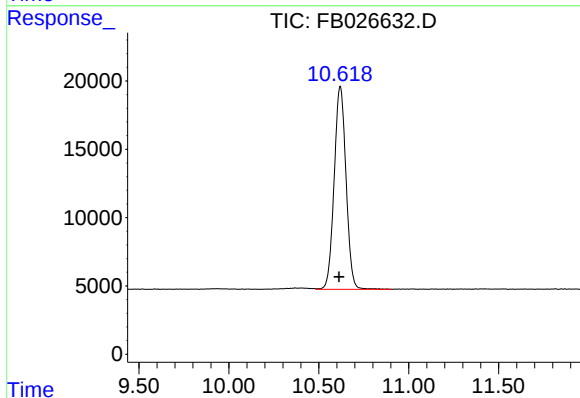


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.006 min
Response: 681532
Conc: 34.71 ng/ml

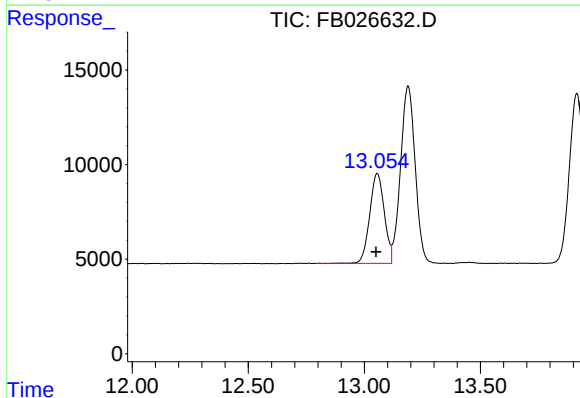


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.005 min
Response: 207273
Conc: 11.22 ng/ml

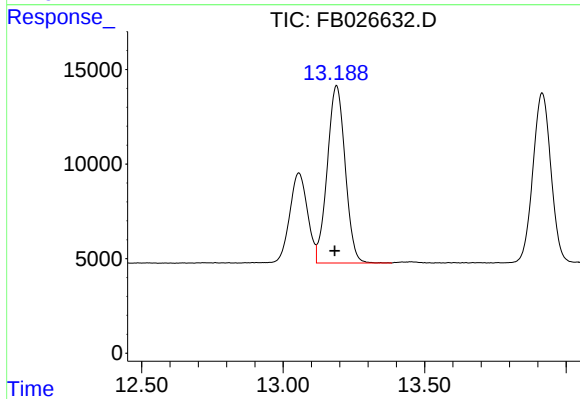


#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: 0.006 min
Response: 411820
Conc: 22.34 ng/ml

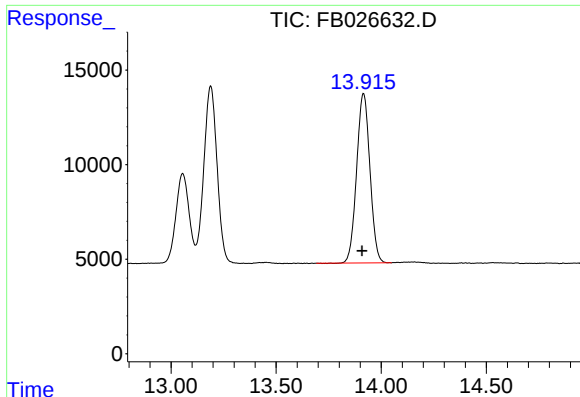

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.006 min
Response: 394114
Conc: 21.92 ng/ml

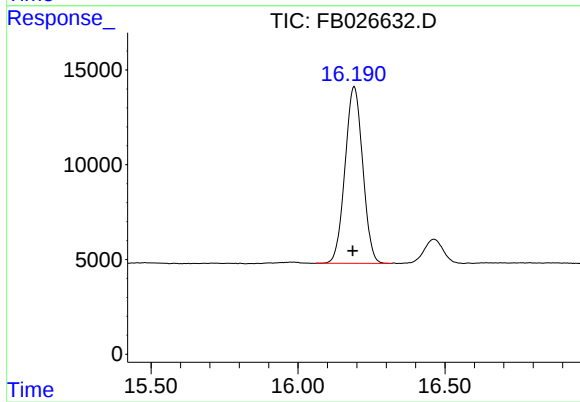

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.006 min
Response: 389201
Conc: 21.08 ng/ml