

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021723\
 Data File : FB029344.D
 Signal(s) : FID2B.CH
 Acq On : 17 Feb 2023 16:59
 Operator : YP/AJ
 Sample : 01586-09MS
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 17 22:08:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.798	54114	5.626 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.699	89443	5.637 ng/ml
2) t	2,2,4-Trimethylpentane	7.422	69510	4.036 ng/ml
3) t	n-Heptane	7.757	28922	1.598 ng/ml
4) t	Benzene	7.894	41236	1.980 ng/ml
6) t	Toluene	10.627	118845	5.865 ng/ml
7) t	Ethylbenzene	13.063	35591	1.865 ng/ml
8) t	m-Xylene	13.196	68160	3.595 ng/ml
9) t	O-Xylene	13.923	62501	3.426 ng/ml
10) t	1,2,4-Trimethylbenzene	16.198	54048	2.872 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021723\
Data File : FB029344.D
Signal(s) : FID2B.CH
Acq On : 17 Feb 2023 16:59
Operator : YP/AJ
Sample : 01586-09MS
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 17 22:08:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

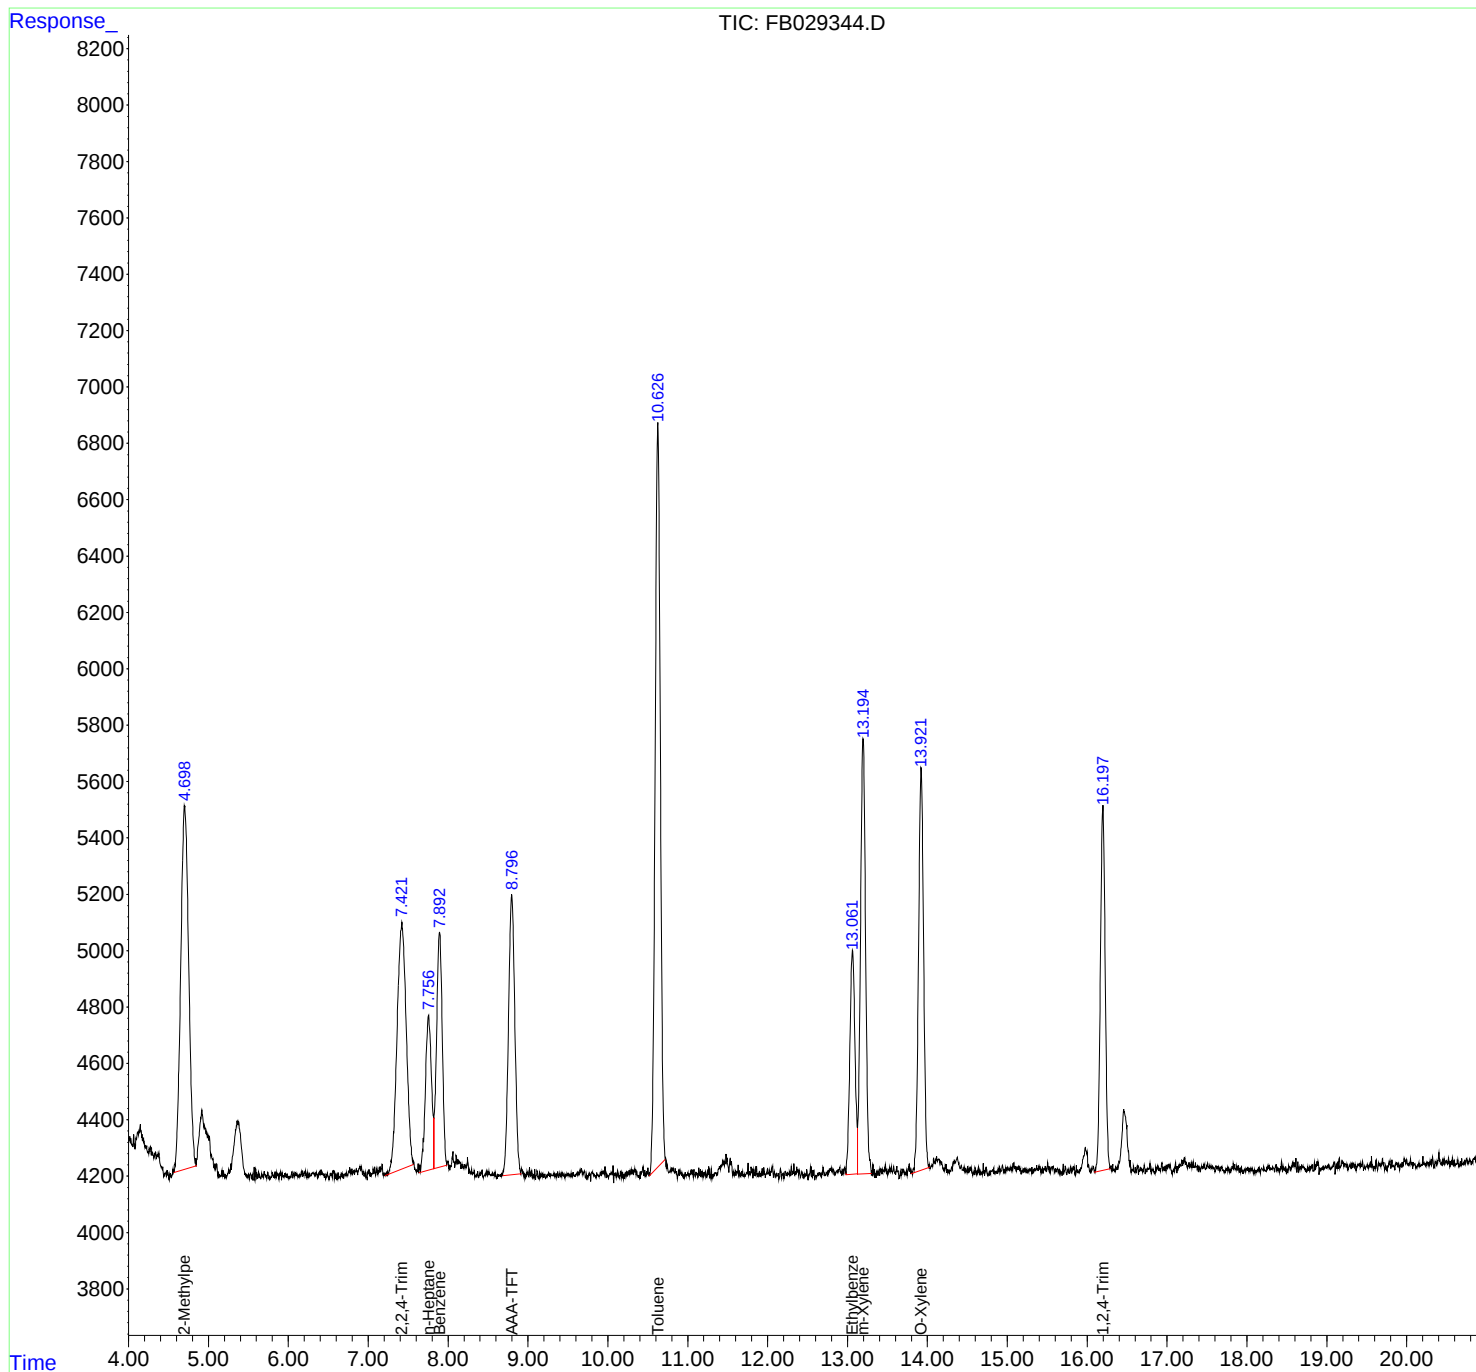

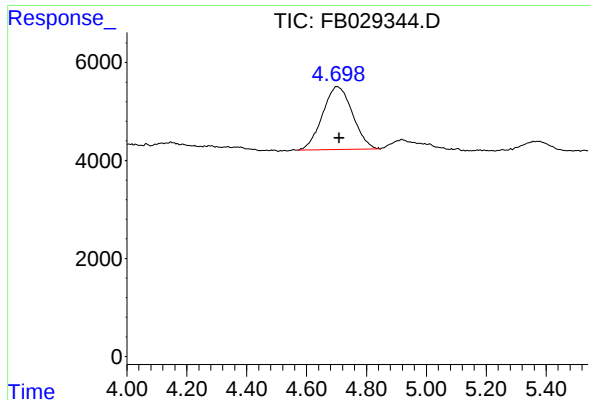


#1 2-Methylpentane

R.T.: 4.699 min
Delta R.T.: -0.010 min
Response: 89443
Conc: 5.64 ng/ml

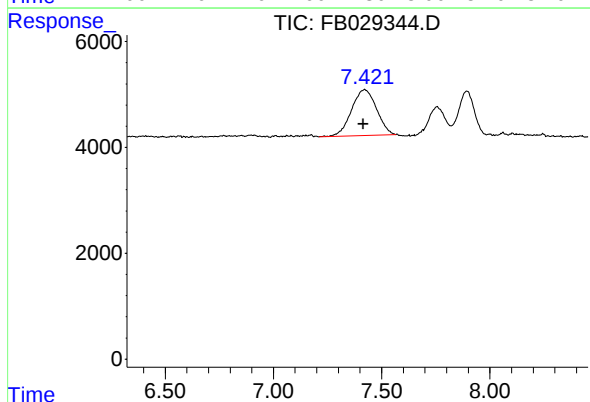


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.008 min
Response: 69510
Conc: 4.04 ng/ml

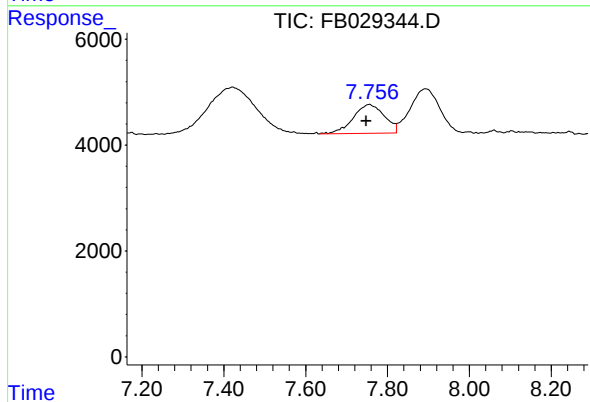


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.008 min
Response: 28922
Conc: 1.60 ng/ml

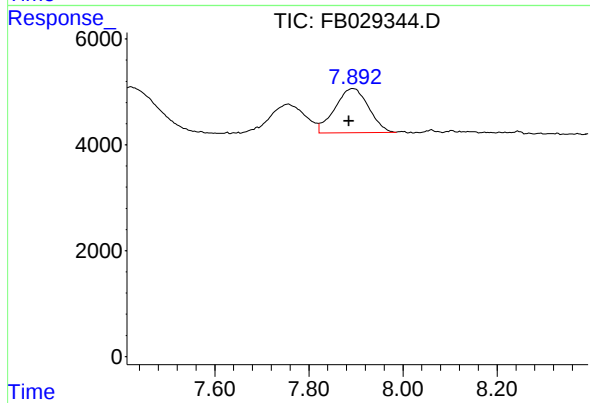


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.009 min
Response: 41236
Conc: 1.98 ng/ml

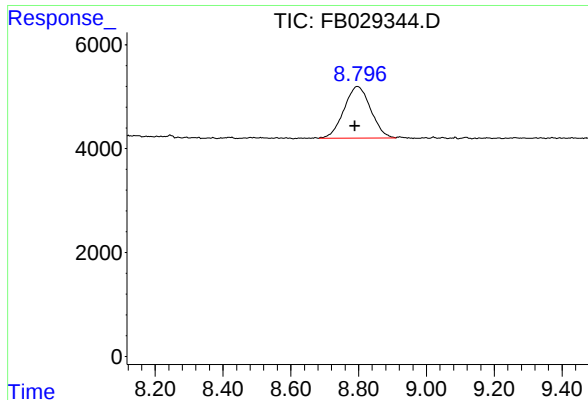


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.008 min
Response: 54114
Conc: 5.63 ng/ml

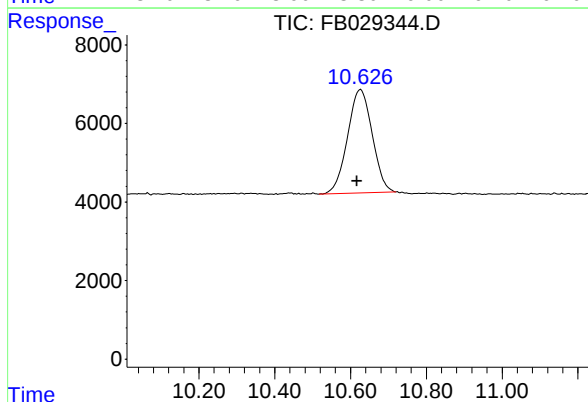


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.010 min
Response: 118845
Conc: 5.86 ng/ml

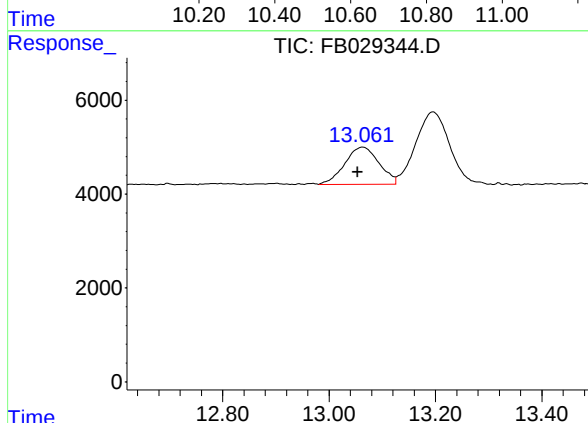


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.009 min
Response: 35591
Conc: 1.86 ng/ml

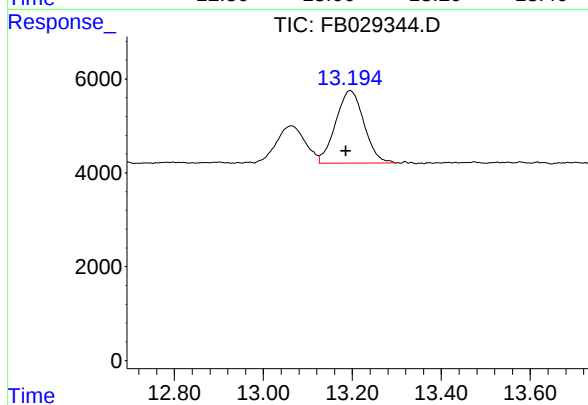


#8 m-Xylene

R.T.: 13.196 min
Delta R.T.: 0.010 min
Response: 68160
Conc: 3.60 ng/ml

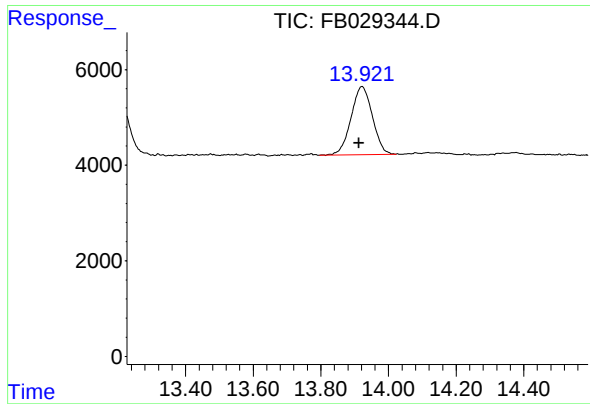

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: 0.010 min
Response: 62501
Conc: 3.43 ng/ml

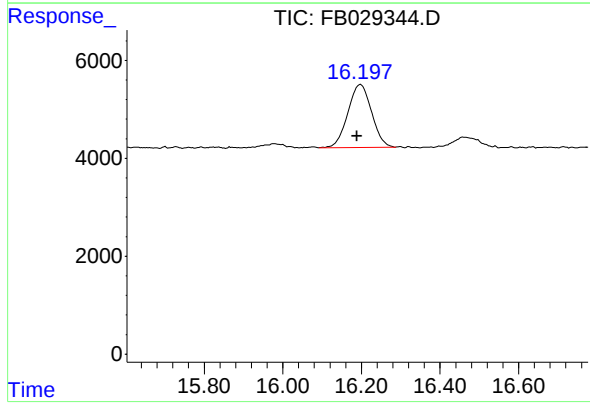

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.010 min
Response: 54048
Conc: 2.87 ng/ml