

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021725\
 Data File : FB031505.D
 Signal(s) : FID2B.CH
 Acq On : 17 Feb 2025 11:00
 Operator : YP/AJ
 Sample : BSF0217S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Feb 18 00:31:08 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021125.M
 Quant Title :
 QLast Update : Tue Feb 11 12:33:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	397209	16.896 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.719	976799	30.579 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	1235519	31.753 ng/ml
3) t n-Heptane	7.754	353925	10.276 ng/ml
4) t Benzene	7.892	466017	10.497 ng/ml
6) t Toluene	10.621	1321825	32.179 ng/ml
7) t Ethylbenzene	13.058	382247	10.528 ng/ml
8) t m-Xylene	13.192	838422	21.338 ng/ml
9) t O-Xylene	13.920	805307	21.530 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	602247	20.323 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021725\
Data File : FB031505.D
Signal(s) : FID2B.CH
Acq On : 17 Feb 2025 11:00
Operator : YP/AJ
Sample : BSF0217S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 18 00:31:08 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021125.M
Quant Title :
QLast Update : Tue Feb 11 12:33:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

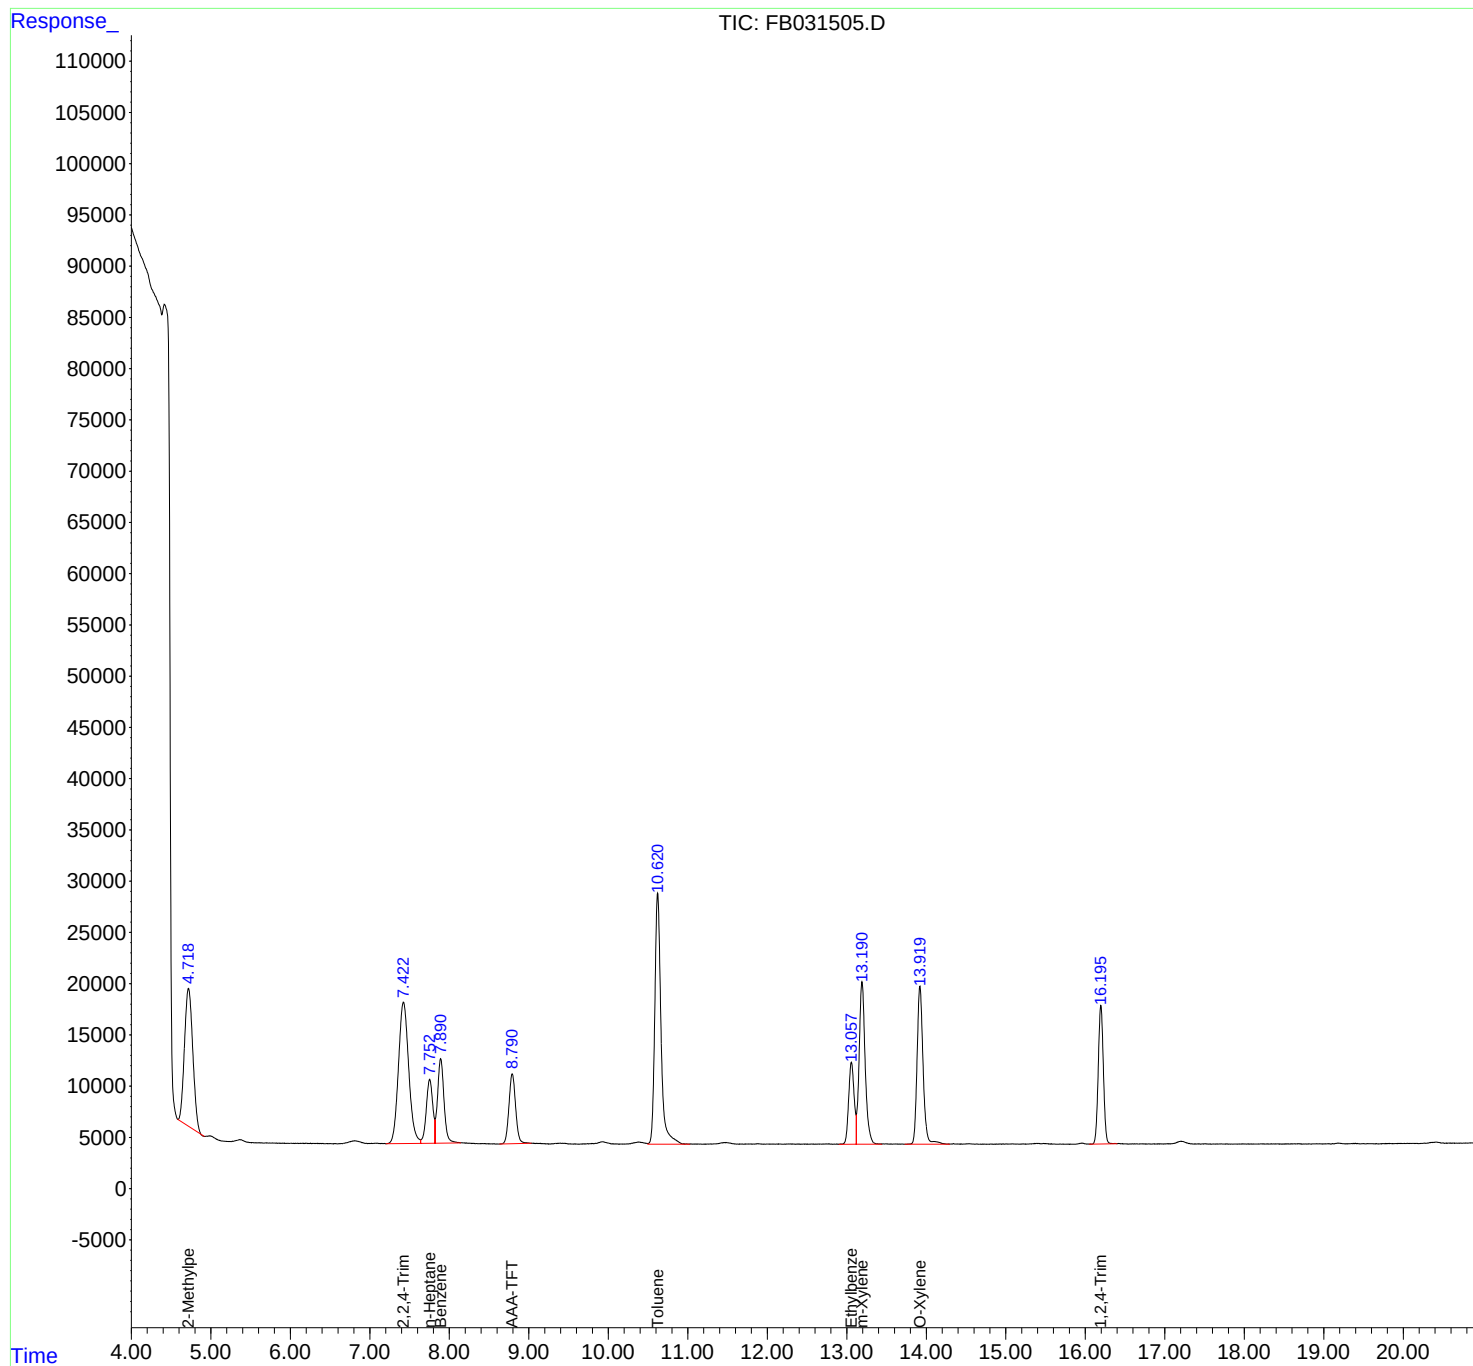


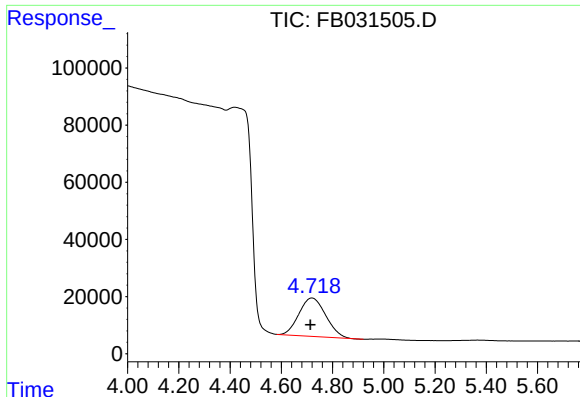

#1 2-Methylpentane


R.T.: 4.719 min
Delta R.T.: 0.005 min
Response: 976799
Conc: 30.58 ng/ml

Instrument :
FID_B
ClientSampleId :

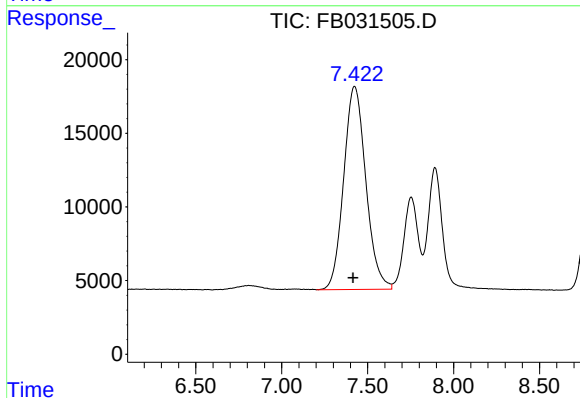


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: 0.007 min
Response: 1235519
Conc: 31.75 ng/ml

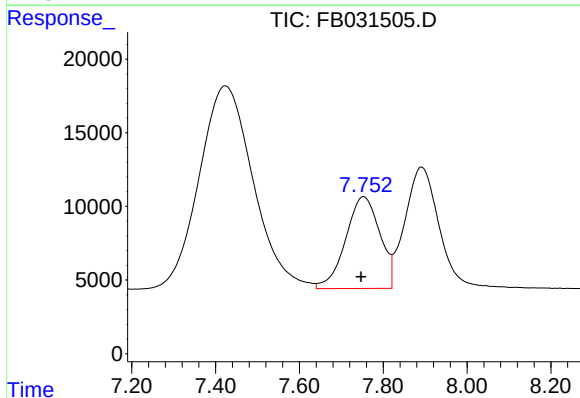


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.006 min
Response: 353925
Conc: 10.28 ng/ml

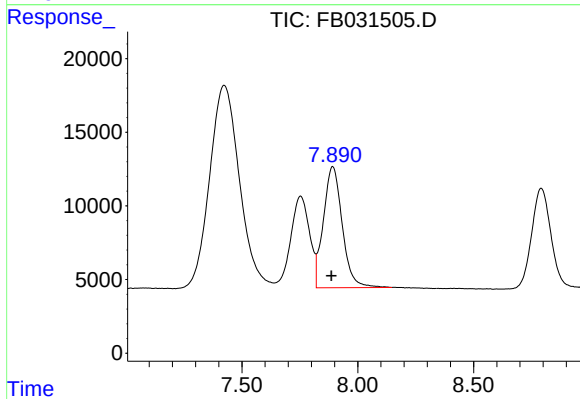

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.006 min
Response: 466017
Conc: 10.50 ng/ml

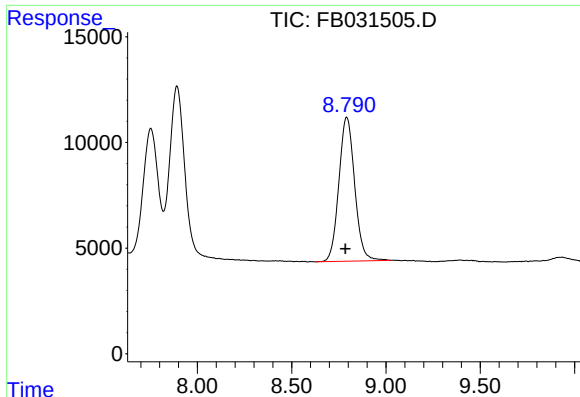

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.006 min
Response: 397209
Conc: 16.90 ng/ml

Instrument :
FID_B
ClientSampleId :

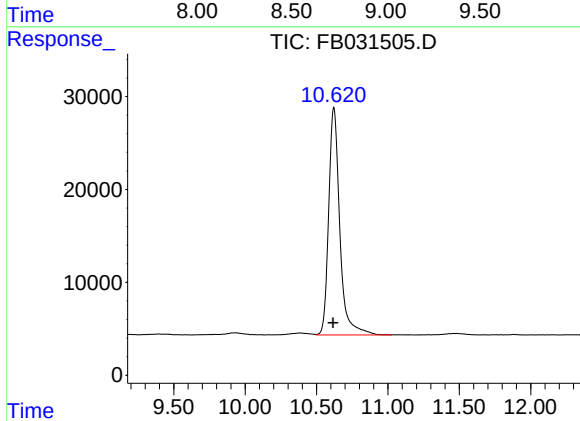


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.006 min
Response: 1321825
Conc: 32.18 ng/ml

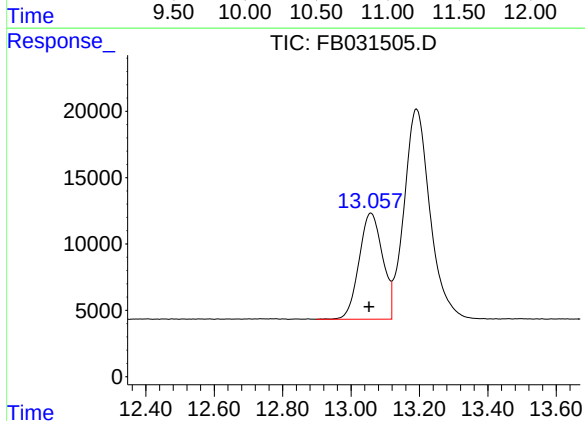


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.006 min
Response: 382247
Conc: 10.53 ng/ml

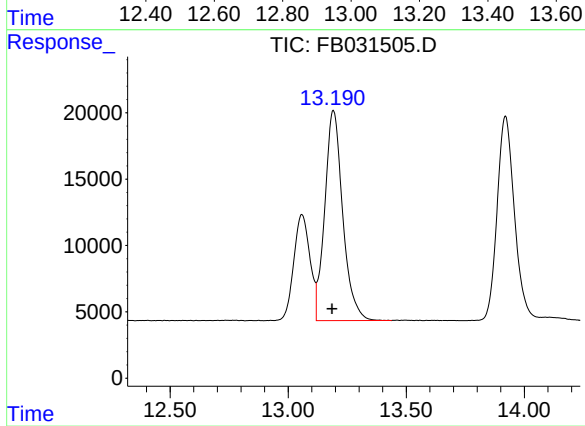

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.006 min
Response: 838422
Conc: 21.34 ng/ml

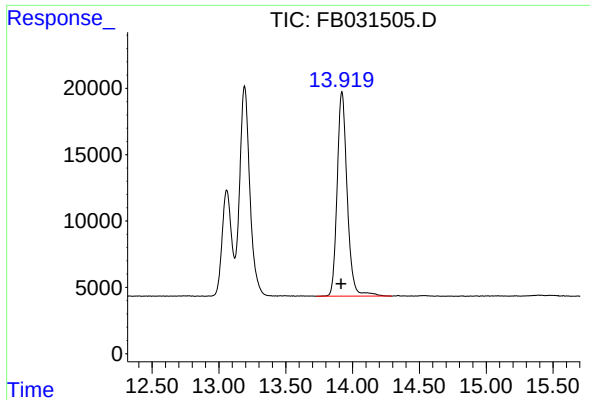

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.006 min
Response: 805307
Conc: 21.53 ng/ml

Instrument :
FID_B
ClientSampleId :

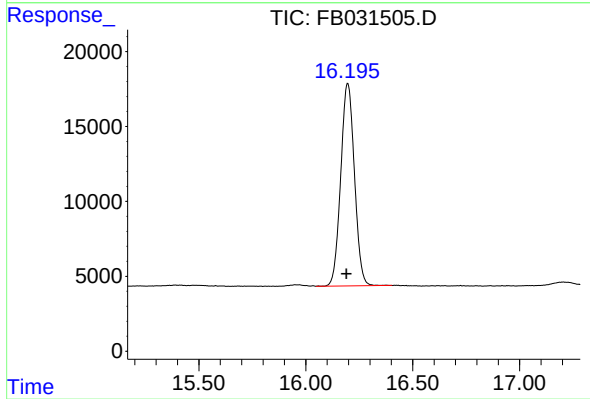

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.006 min
Response: 602247
Conc: 20.32 ng/ml