

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021819\
 Data File : FB019819.D
 Signal(s) : FID2B.CH
 Acq On : 18 Feb 2019 9:47
 Operator : MJ/SJ
 Sample : BSF0218S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 18 23:48:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.041	232144	19.859 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.896	643310	37.158 ng/ml
2) t	2,2,4-Trimethylpentane	7.656	623571	37.602 ng/ml
3) t	n-Heptane	7.996	191951	11.911 ng/ml
4) t	Benzene	8.133	217444	11.528 ng/ml
6) t	Toluene	10.888	559640	31.993 ng/ml
7) t	Ethylbenzene	13.340	221270	10.083 ng/ml
8) t	m-Xylene	13.473	464228	20.283 ng/ml
9) t	O-Xylene	14.205	454287	20.340 ng/ml
10) t	1,2,4-Trimethylbenzene	16.492	457944	19.764 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021819\
Data File : FB019819.D
Signal(s) : FID2B.CH
Acq On : 18 Feb 2019 9:47
Operator : MJ/SJ
Sample : BSF0218S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 18 23:48:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

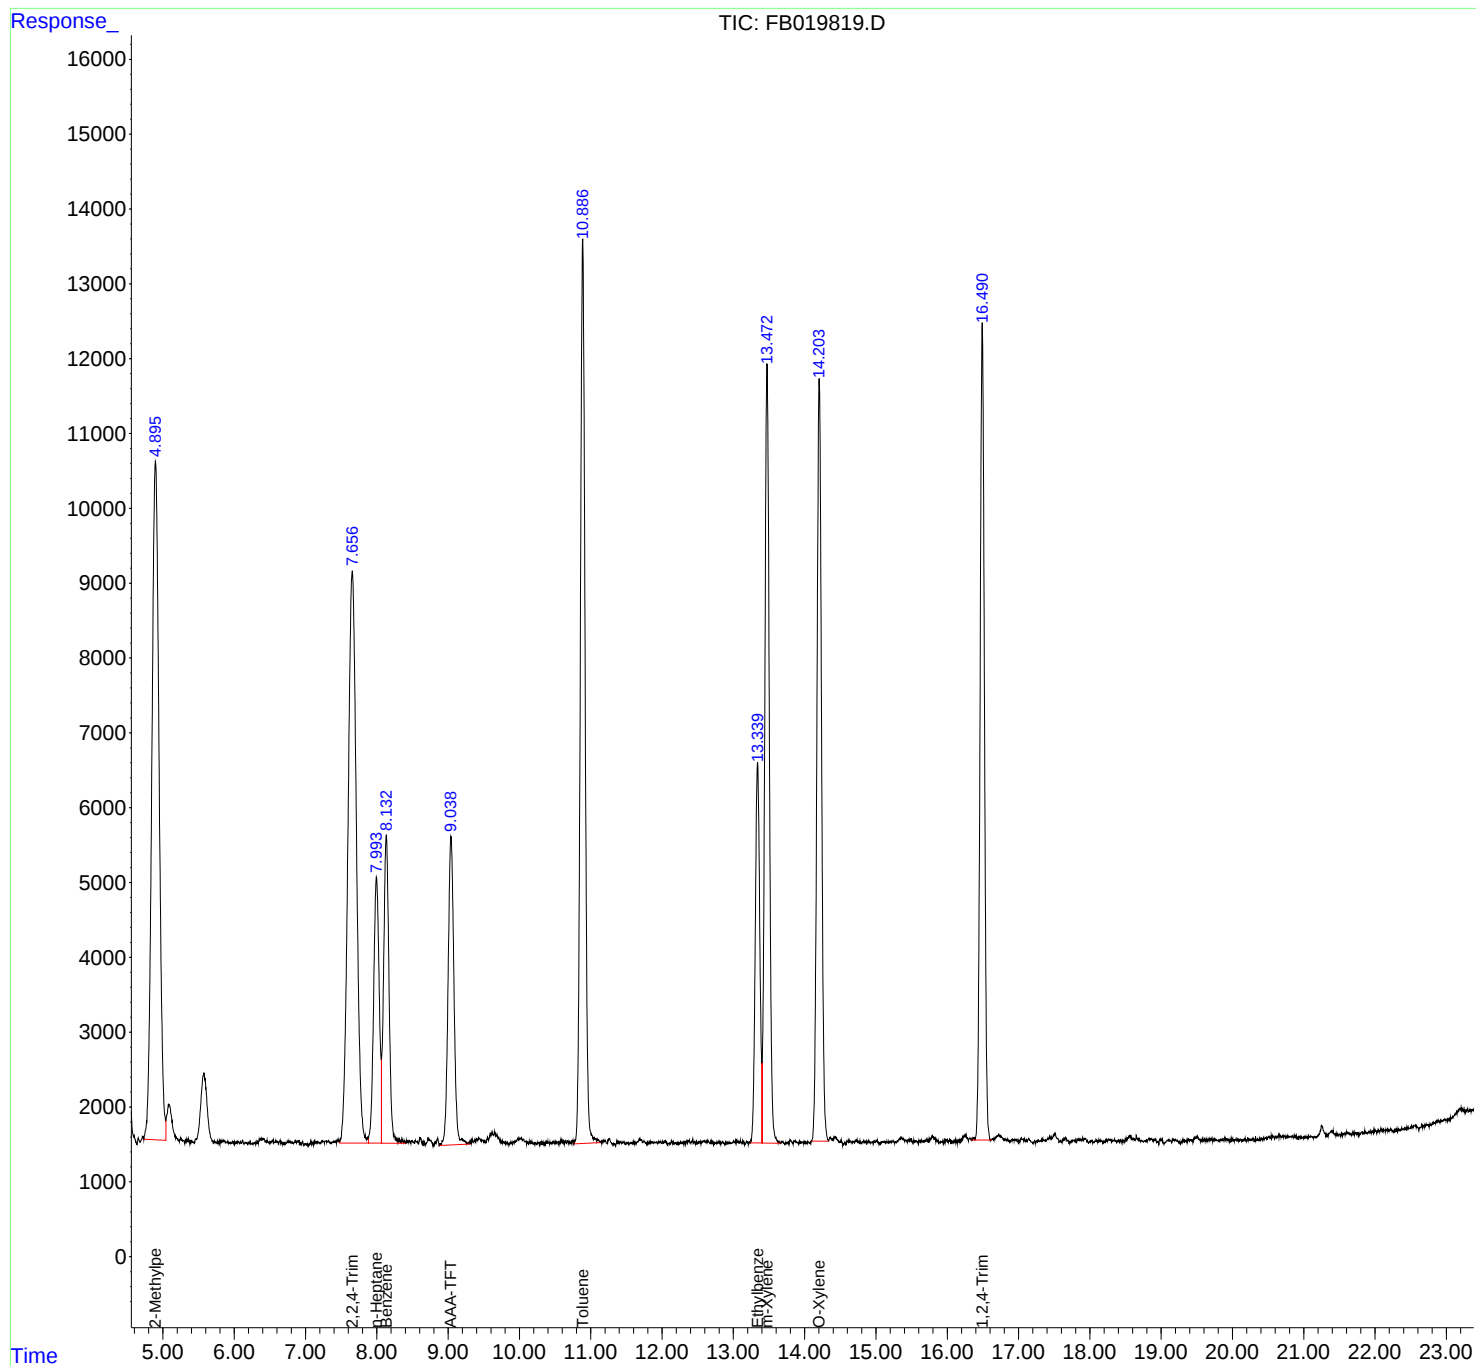

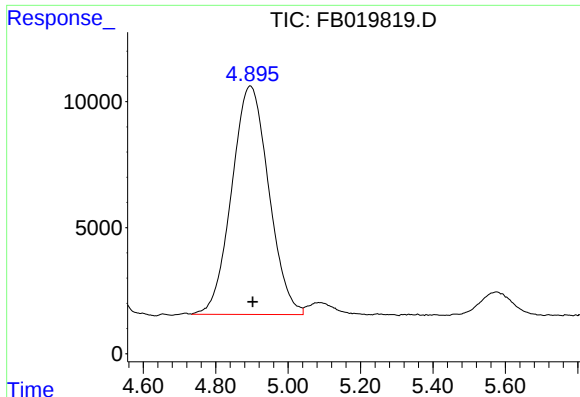


#1 2-Methylpentane

R.T.: 4.896 min
Delta R.T.: -0.006 min
Response: 643310
Conc: 37.16 ng/ml

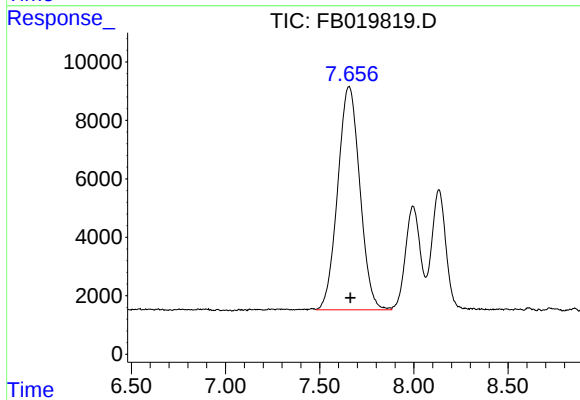


#2 2,2,4-Trimethylpentane

R.T.: 7.656 min
Delta R.T.: -0.008 min
Response: 623571
Conc: 37.60 ng/ml

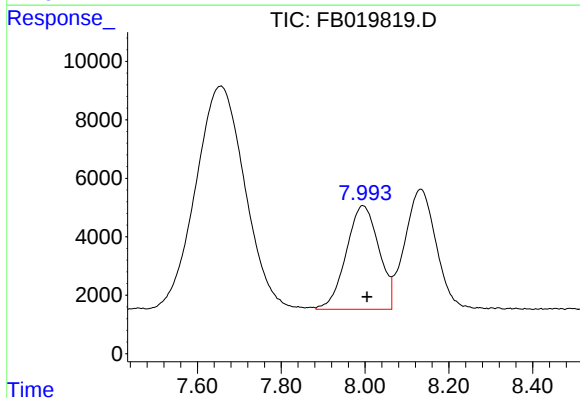


#3 n-Heptane

R.T.: 7.996 min
Delta R.T.: -0.009 min
Response: 191951
Conc: 11.91 ng/ml

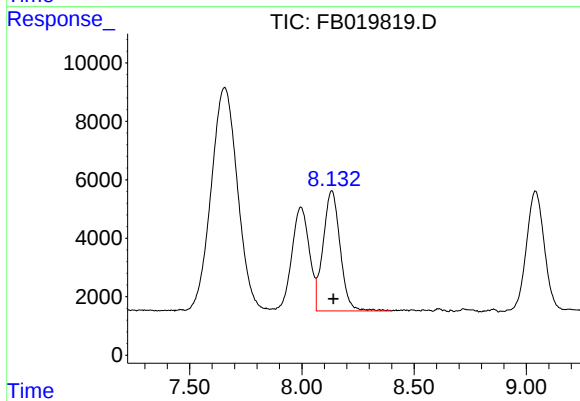


#4 Benzene

R.T.: 8.133 min
Delta R.T.: -0.008 min
Response: 217444
Conc: 11.53 ng/ml

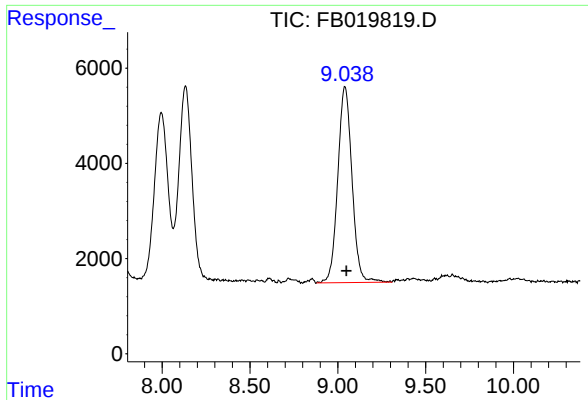


#5 AAA-TFT

R.T.: 9.041 min
Delta R.T.: -0.009 min
Response: 232144
Conc: 19.86 ng/ml

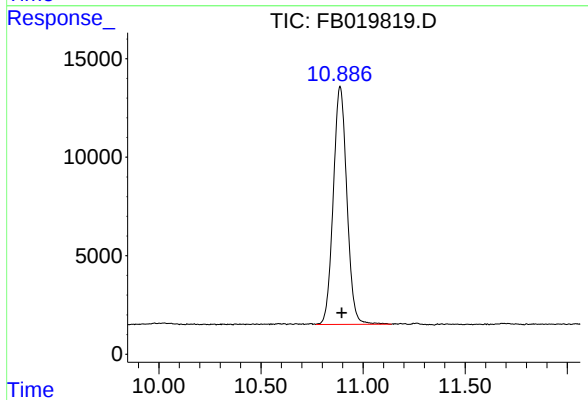


#6 Toluene

R.T.: 10.888 min
Delta R.T.: -0.009 min
Response: 559640
Conc: 31.99 ng/ml

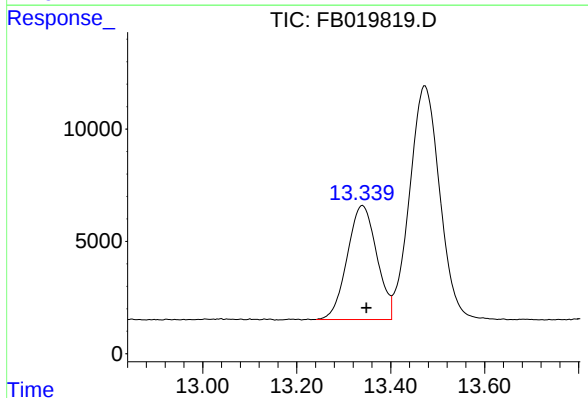


#7 Ethylbenzene

R.T.: 13.340 min
Delta R.T.: -0.008 min
Response: 221270
Conc: 10.08 ng/ml

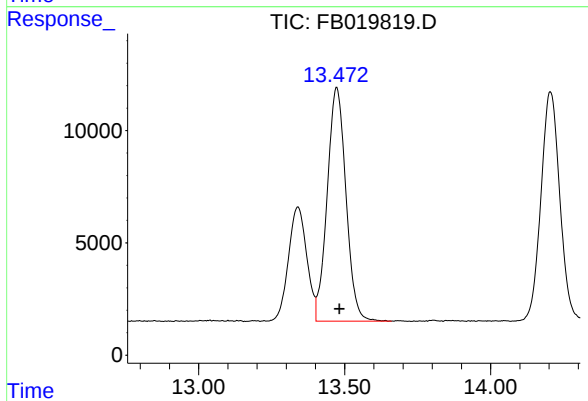

#8 m-Xylene

R.T.: 13.473 min
Delta R.T.: -0.009 min
Response: 464228
Conc: 20.28 ng/ml

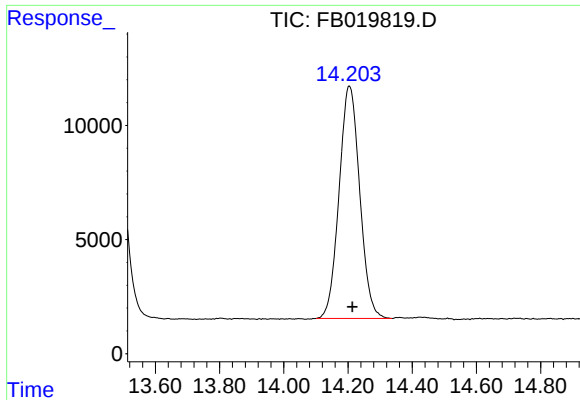


#9 O-Xylene

R.T.: 14.205 min

Delta R.T.: -0.009 min

Response: 454287

Conc: 20.34 ng/ml

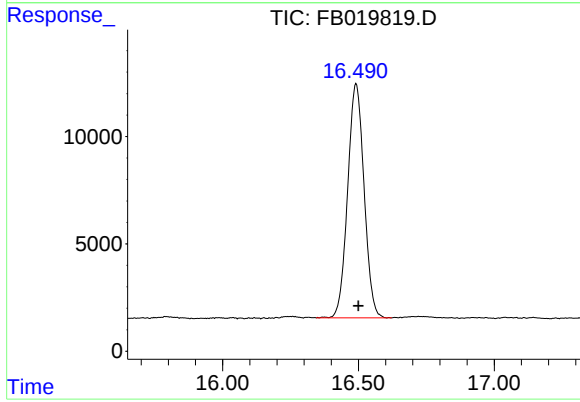

#10 1,2,4-Trimethylbenzene

R.T.: 16.492 min

Delta R.T.: -0.008 min

Response: 457944

Conc: 19.76 ng/ml