

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021819\
 Data File : FB019822.D
 Signal(s) : FID2B.CH
 Acq On : 18 Feb 2019 12:03
 Operator : MJ/SJ
 Sample : K1517-05MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 18 23:49:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.042	219443	18.773 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.895	557745	32.215 ng/ml
2) t 2,2,4-Trimethylpentane	7.658	507930	30.629 ng/ml
3) t n-Heptane	7.996	152143	9.441 ng/ml
4) t Benzene	8.133	189196	10.031 ng/ml
6) t Toluene	10.889	501028	28.643 ng/ml
7) t Ethylbenzene	13.342	205561	9.367 ng/ml
8) t m-Xylene	13.474	426647	18.641 ng/ml
9) t O-Xylene	14.206	427074	19.121 ng/ml
10) t 1,2,4-Trimethylbenzene	16.493	418316	18.054 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021819\
Data File : FB019822.D
Signal(s) : FID2B.CH
Acq On : 18 Feb 2019 12:03
Operator : MJ/SJ
Sample : K1517-05MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 18 23:49:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

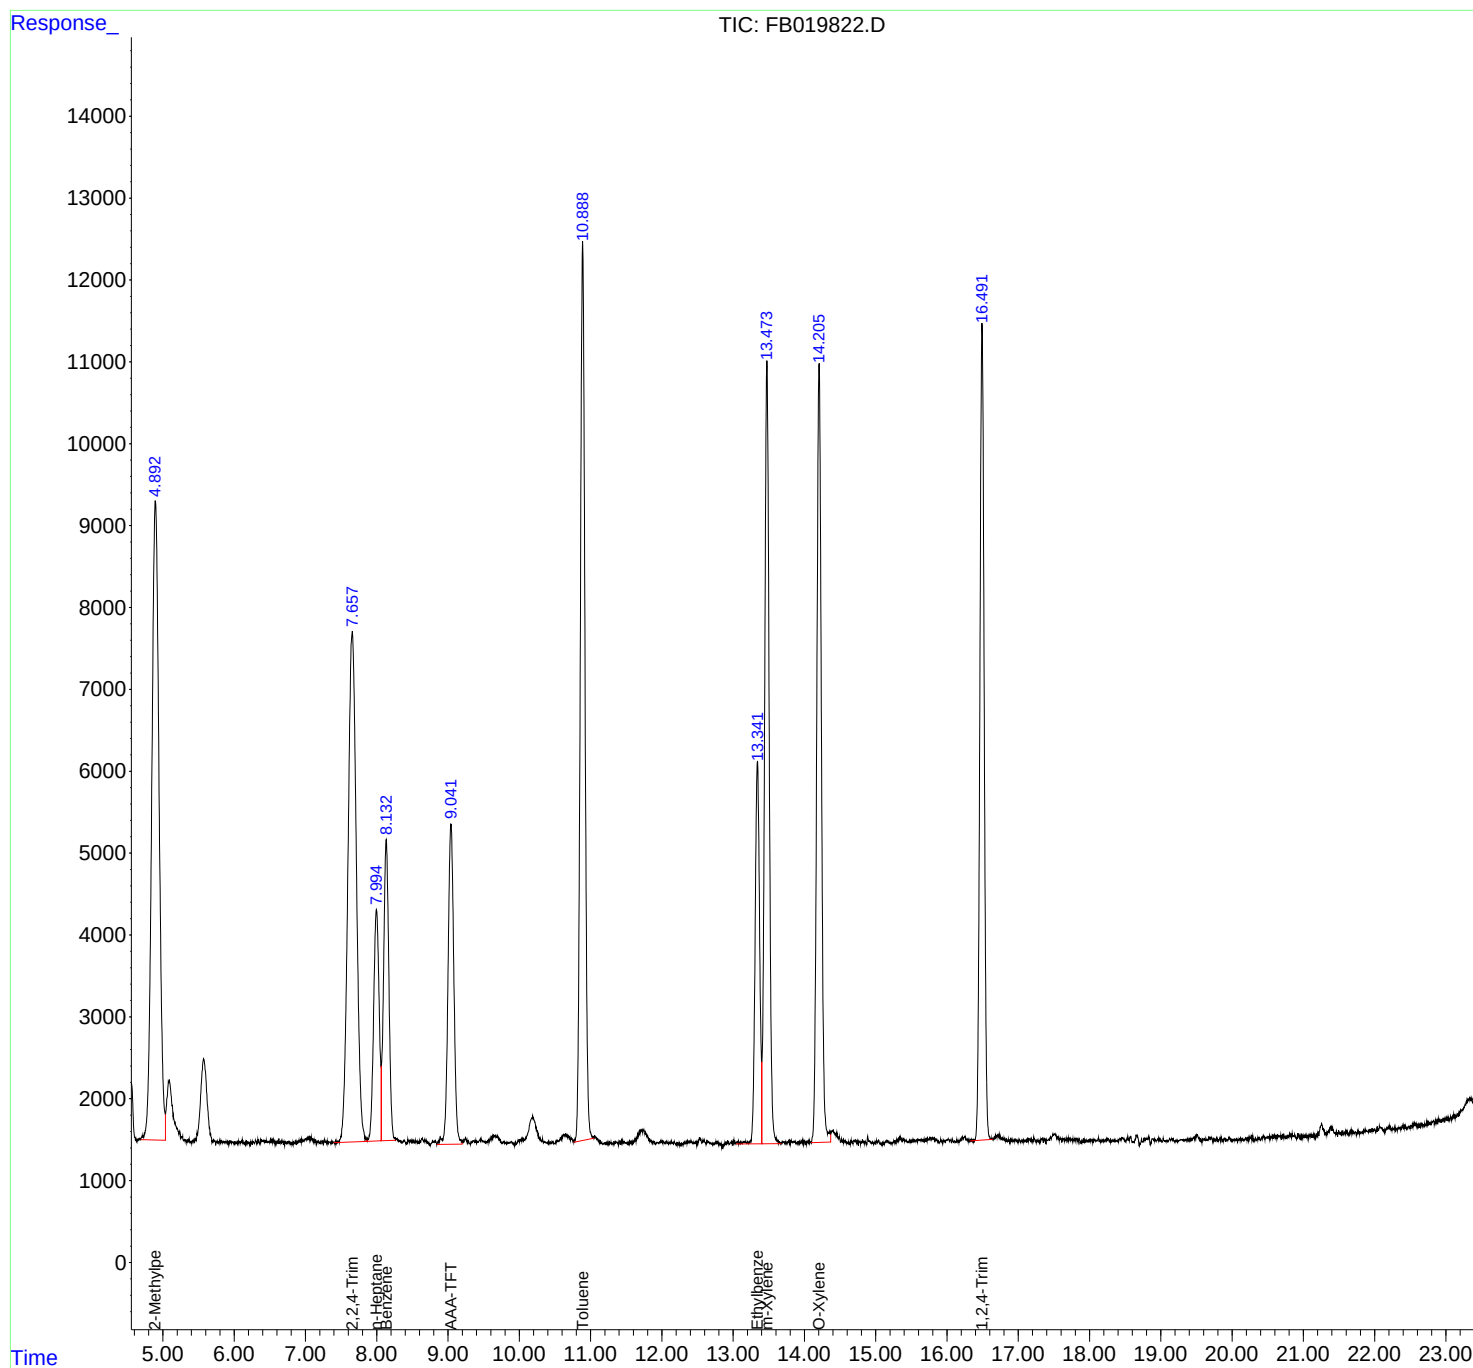

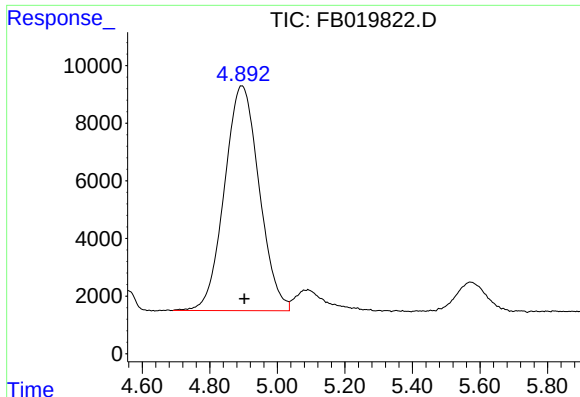


#1 2-Methylpentane

R.T.: 4.895 min
Delta R.T.: -0.007 min
Response: 557745
Conc: 32.22 ng/ml

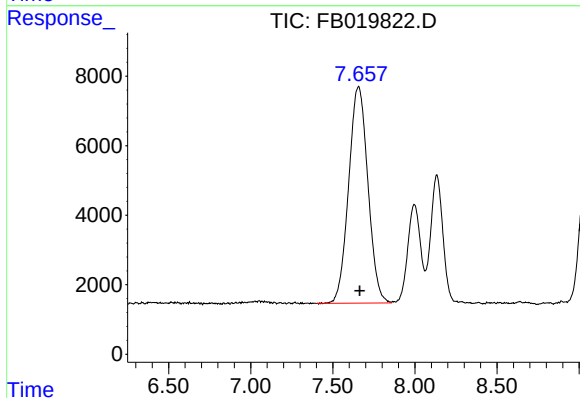


#2 2,2,4-Trimethylpentane

R.T.: 7.658 min
Delta R.T.: -0.007 min
Response: 507930
Conc: 30.63 ng/ml

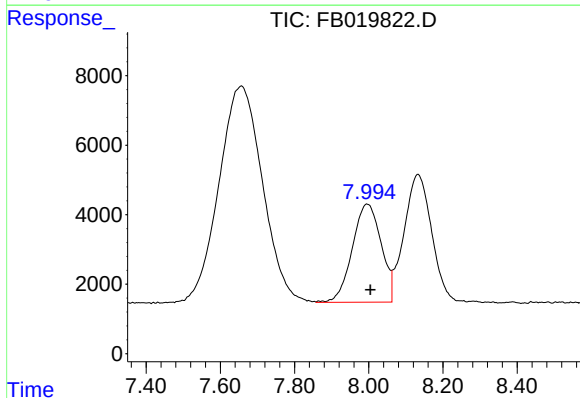


#3 n-Heptane

R.T.: 7.996 min
Delta R.T.: -0.008 min
Response: 152143
Conc: 9.44 ng/ml

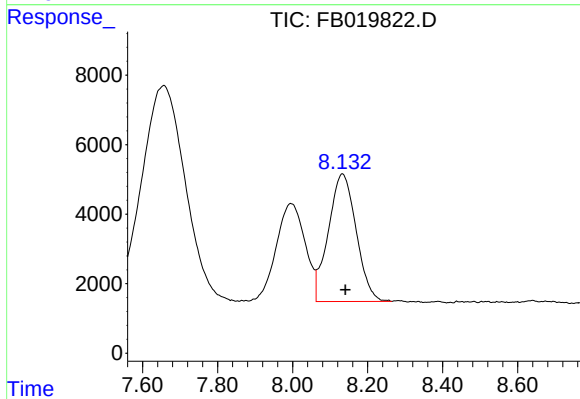


#4 Benzene

R.T.: 8.133 min
Delta R.T.: -0.008 min
Response: 189196
Conc: 10.03 ng/ml

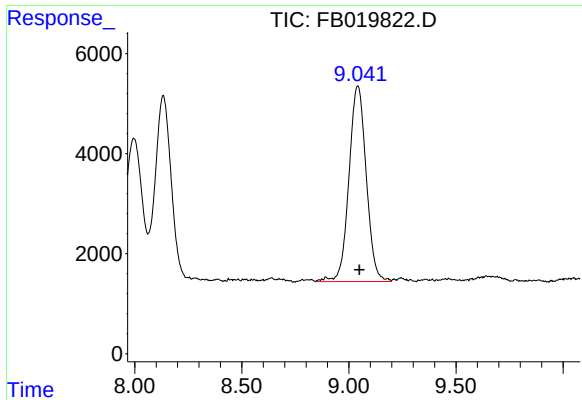


#5 AAA-TFT

R.T.: 9.042 min
Delta R.T.: -0.008 min
Response: 219443
Conc: 18.77 ng/ml

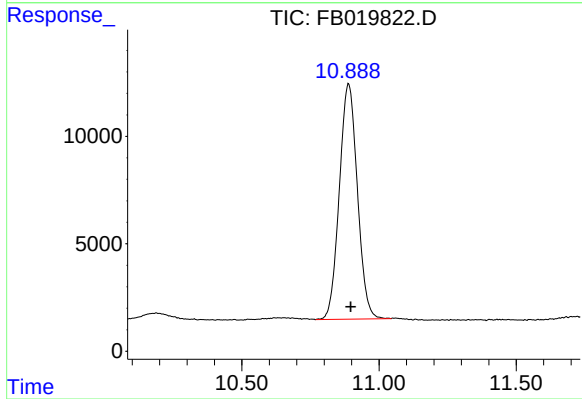


#6 Toluene

R.T.: 10.889 min
Delta R.T.: -0.007 min
Response: 501028
Conc: 28.64 ng/ml

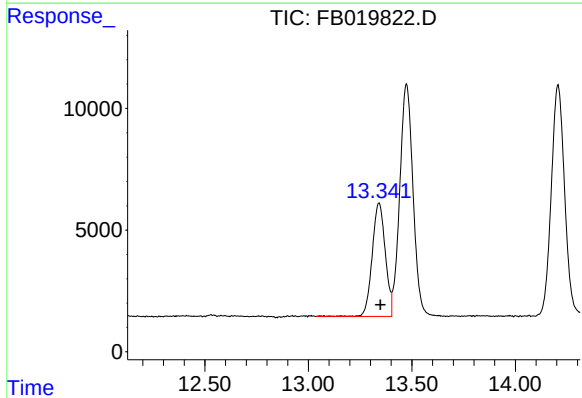


#7 Ethylbenzene

R.T.: 13.342 min
Delta R.T.: -0.007 min
Response: 205561
Conc: 9.37 ng/ml

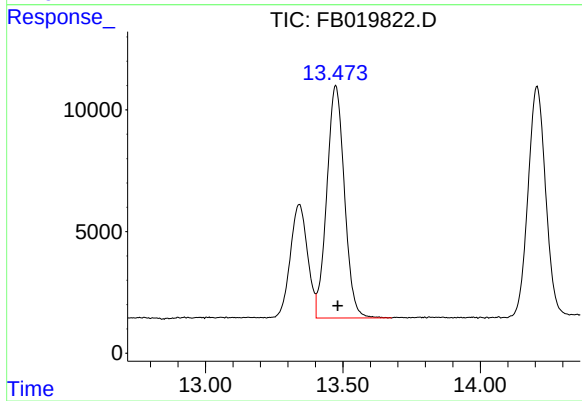


#8 m-Xylene

R.T.: 13.474 min
Delta R.T.: -0.008 min
Response: 426647
Conc: 18.64 ng/ml

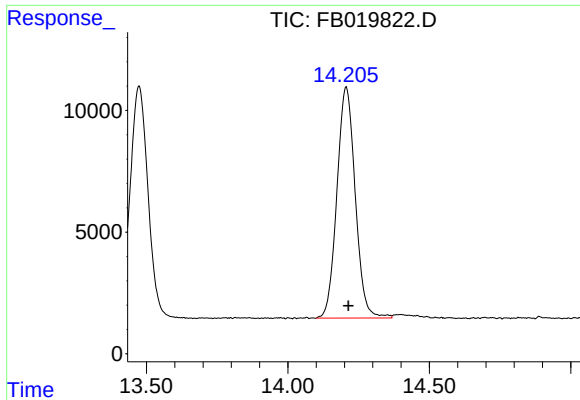

#9 O-Xylene

R.T.: 14.206 min
Delta R.T.: -0.007 min
Response: 427074
Conc: 19.12 ng/ml

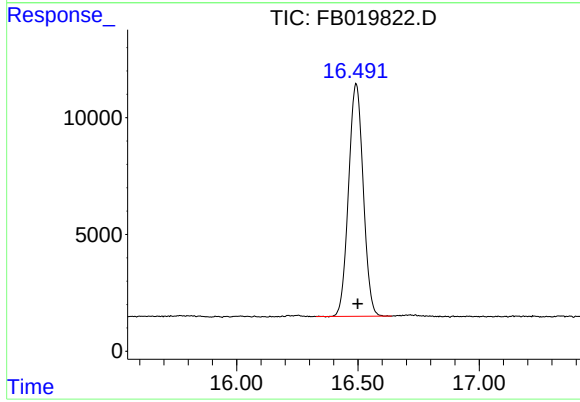

#10 1,2,4-Trimethylbenzene

R.T.: 16.493 min
Delta R.T.: -0.007 min
Response: 418316
Conc: 18.05 ng/ml