

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021919\
 Data File : FB019831.D
 Signal(s) : FID2B.CH
 Acq On : 19 Feb 2019 11:13
 Operator : MJ/SJ
 Sample : BSF0219S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 20 00:31:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.038	221606	18.958 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.893	627605	36.250 ng/ml
2) t 2,2,4-Trimethylpentane	7.655	607419	36.628 ng/ml
3) t n-Heptane	7.993	184938	11.476 ng/ml
4) t Benzene	8.131	207444	10.998 ng/ml
6) t Toluene	10.886	531079	30.361 ng/ml
7) t Ethylbenzene	13.337	211766	9.650 ng/ml
8) t m-Xylene	13.471	447952	19.572 ng/ml
9) t O-Xylene	14.202	442058	19.792 ng/ml
10) t 1,2,4-Trimethylbenzene	16.488	449554	19.402 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021919\
Data File : FB019831.D
Signal(s) : FID2B.CH
Acq On : 19 Feb 2019 11:13
Operator : MJ/SJ
Sample : BSF0219S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 20 00:31:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

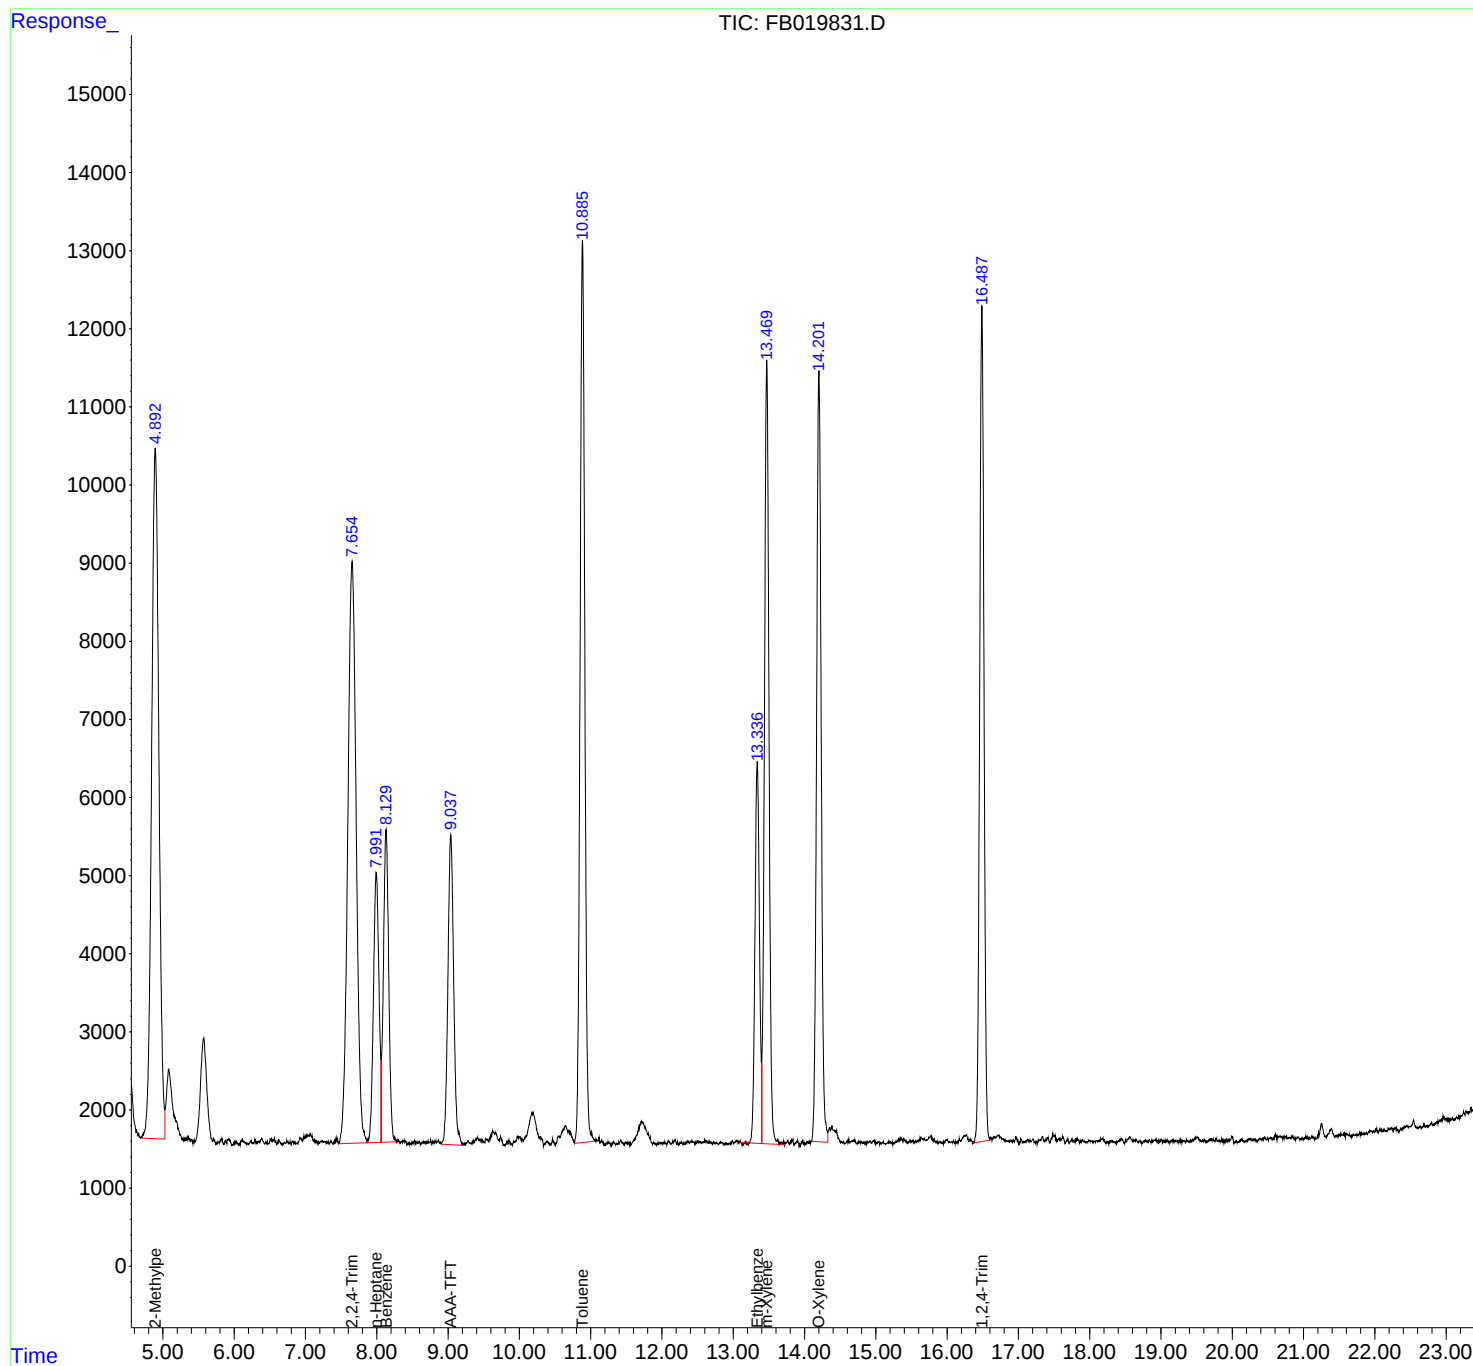

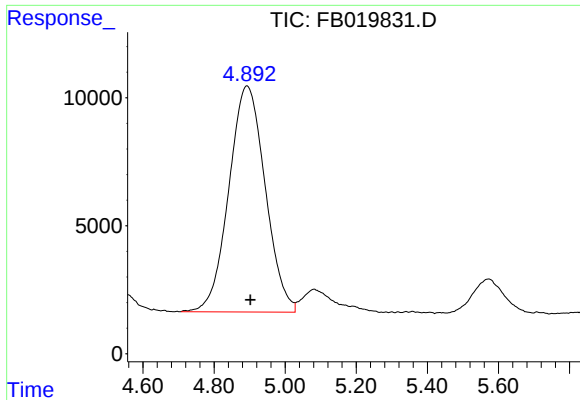


#1 2-Methylpentane

R.T.: 4.893 min
Delta R.T.: -0.009 min
Response: 627605
Conc: 36.25 ng/ml

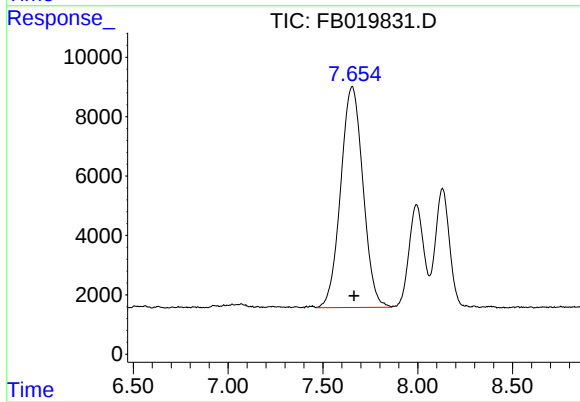


#2 2,2,4-Trimethylpentane

R.T.: 7.655 min
Delta R.T.: -0.009 min
Response: 607419
Conc: 36.63 ng/ml

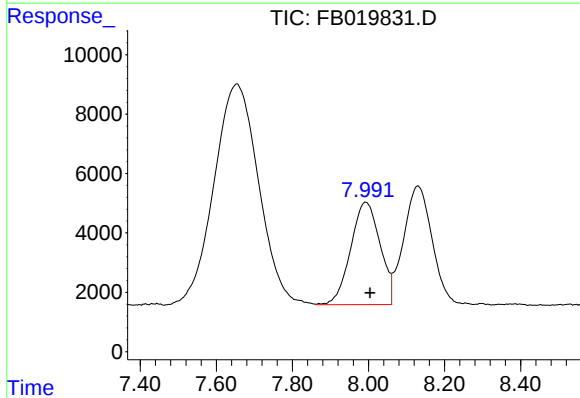


#3 n-Heptane

R.T.: 7.993 min
Delta R.T.: -0.011 min
Response: 184938
Conc: 11.48 ng/ml

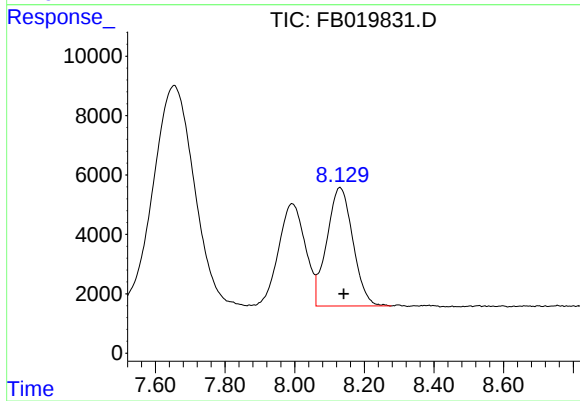


#4 Benzene

R.T.: 8.131 min
Delta R.T.: -0.011 min
Response: 207444
Conc: 11.00 ng/ml

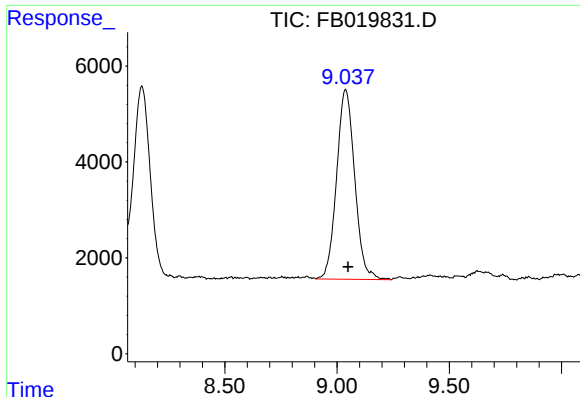


#5 AAA-TFT

R.T.: 9.038 min
Delta R.T.: -0.011 min
Response: 221606
Conc: 18.96 ng/ml

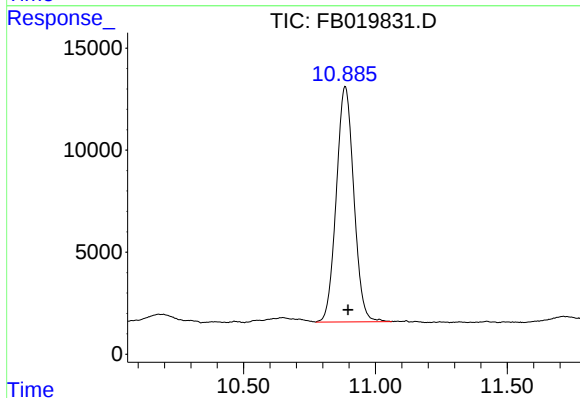


#6 Toluene

R.T.: 10.886 min
Delta R.T.: -0.011 min
Response: 531079
Conc: 30.36 ng/ml

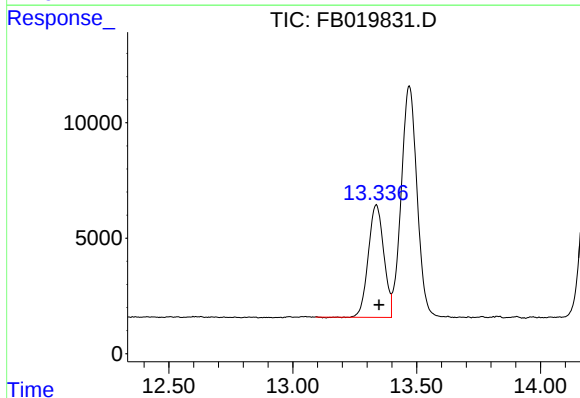


#7 Ethylbenzene

R.T.: 13.337 min
Delta R.T.: -0.011 min
Response: 211766
Conc: 9.65 ng/ml

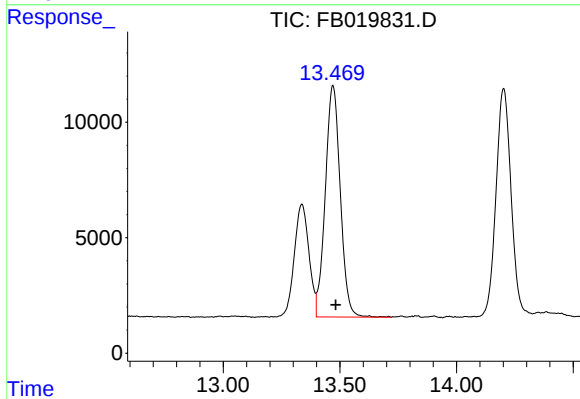


#8 m-Xylene

R.T.: 13.471 min
Delta R.T.: -0.011 min
Response: 447952
Conc: 19.57 ng/ml

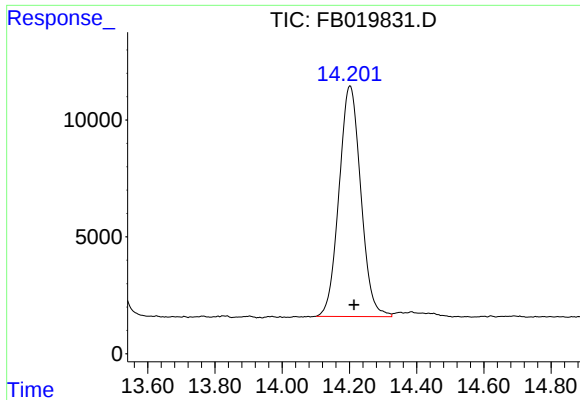

#9 O-Xylene

R.T.: 14.202 min
Delta R.T.: -0.012 min
Response: 442058
Conc: 19.79 ng/ml

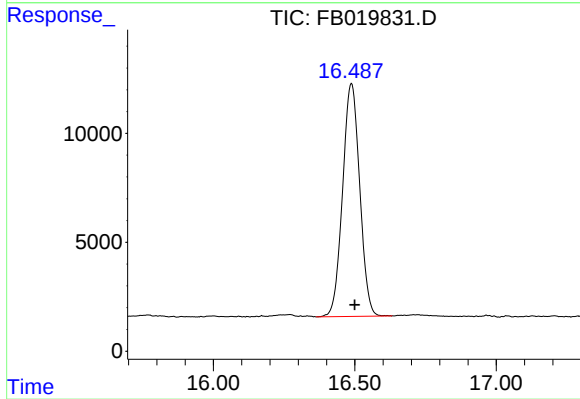

#10 1,2,4-Trimethylbenzene

R.T.: 16.488 min
Delta R.T.: -0.012 min
Response: 449554
Conc: 19.40 ng/ml