

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021920\
Data File : FB023681.D
Signal(s) : FID2B.CH
Acq On : 19 Feb 2020 9:08
Operator : DD/AJ
Sample : VBF0219S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 20 00:35:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	399202	19.607 ng/ml
Target Compounds			
6) t Toluene	10.628	3562	0.090 ng/ml
8) t m-Xylene	13.192	648	0.018 ng/ml
9) t O-Xylene	13.929	4530	0.131 ng/ml
10) t 1,2,4-Trimethylbenzene	16.201	4784	0.163 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021920\
Data File : FB023681.D
Signal(s) : FID2B.CH
Acq On : 19 Feb 2020 9:08
Operator : DD/AJ
Sample : VBF0219S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 20 00:35:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

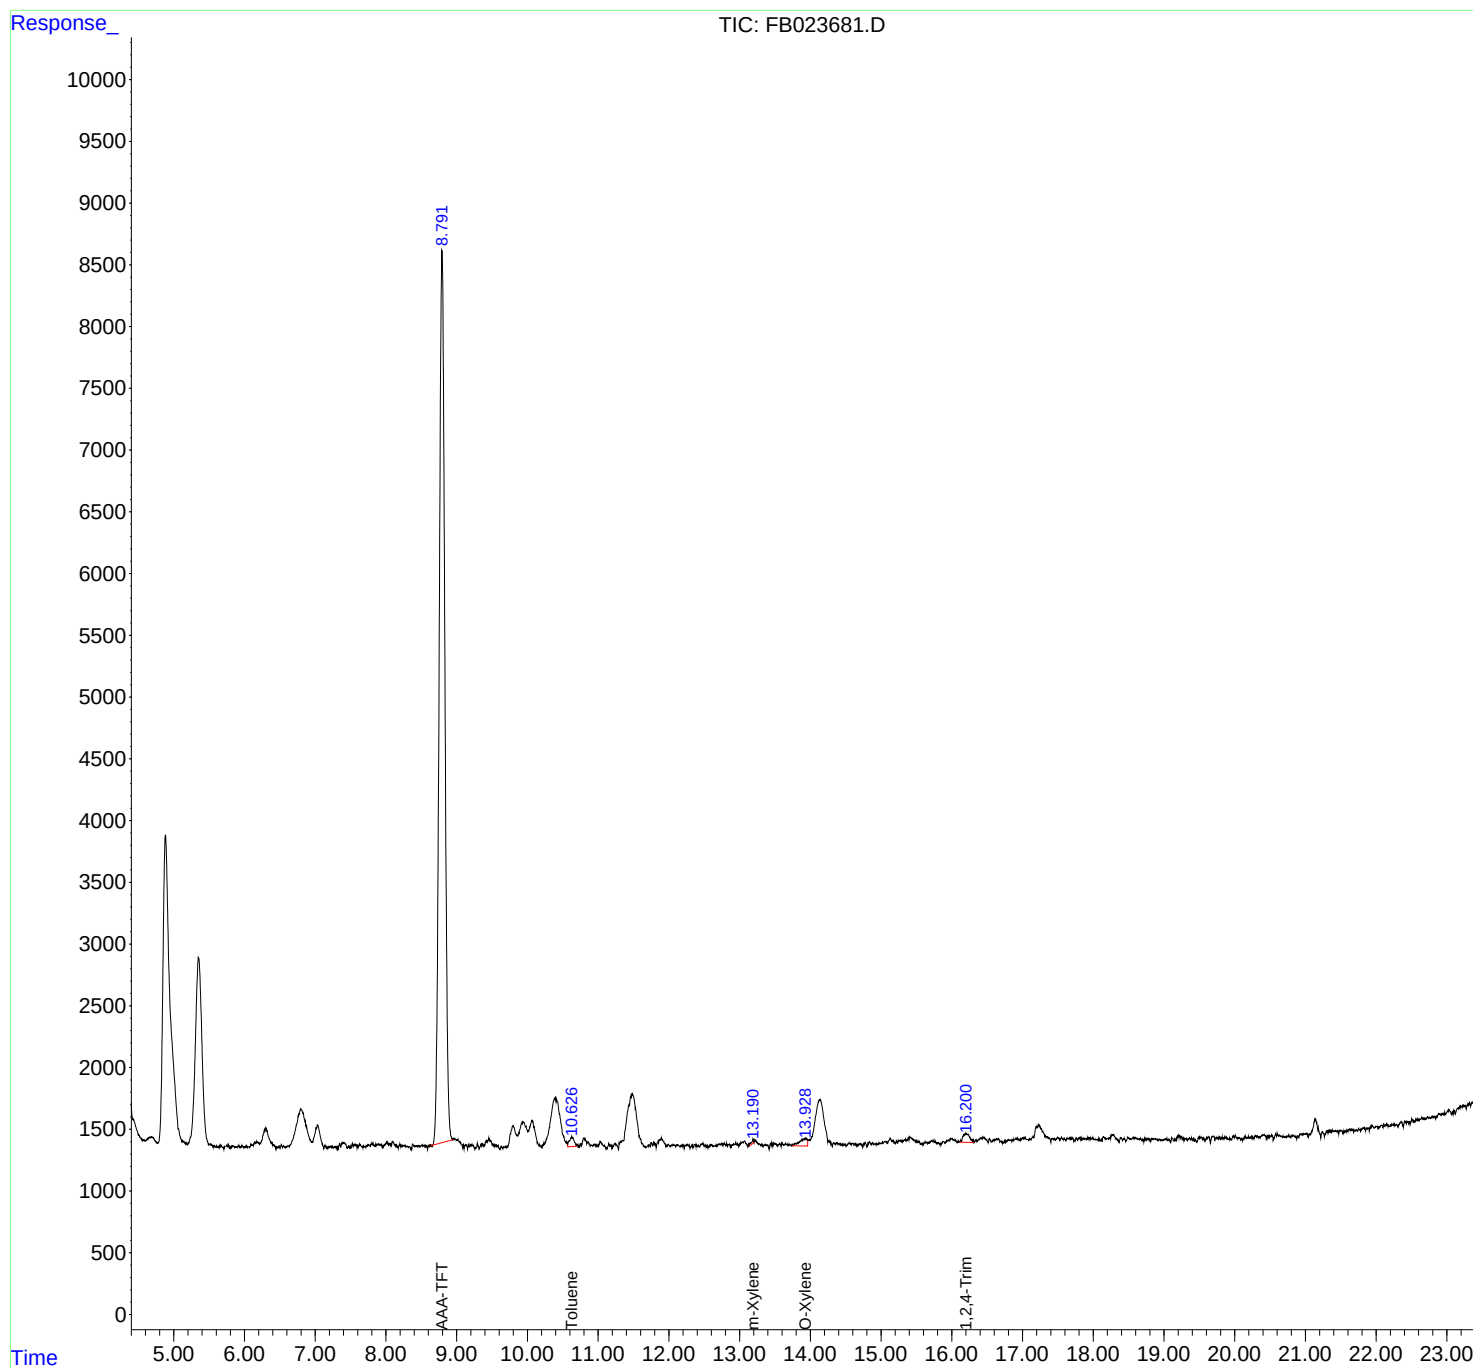

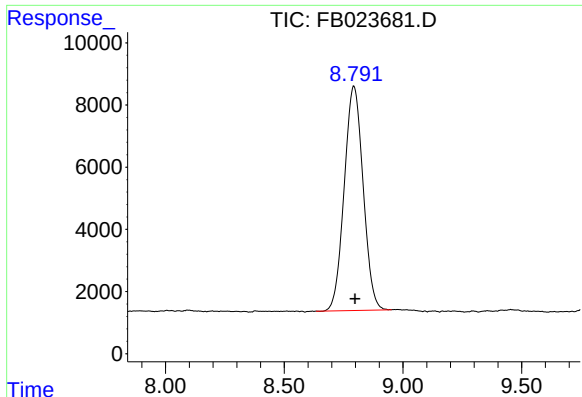


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.006 min
Response: 399202
Conc: 19.61 ng/ml

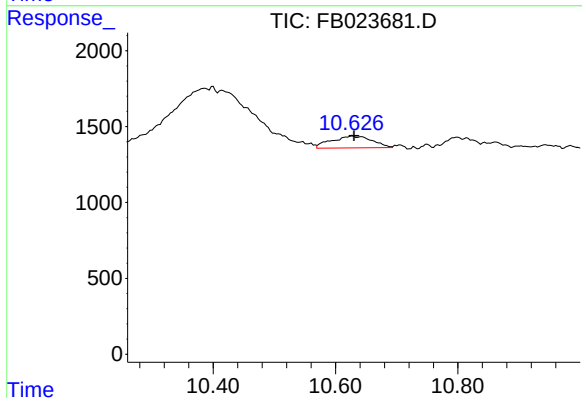


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.002 min
Response: 3562
Conc: 0.09 ng/ml

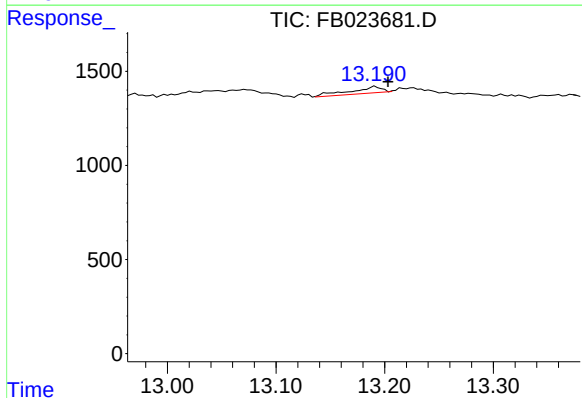


#8 m-Xylene

R.T.: 13.192 min
Delta R.T.: -0.011 min
Response: 648
Conc: 0.02 ng/ml

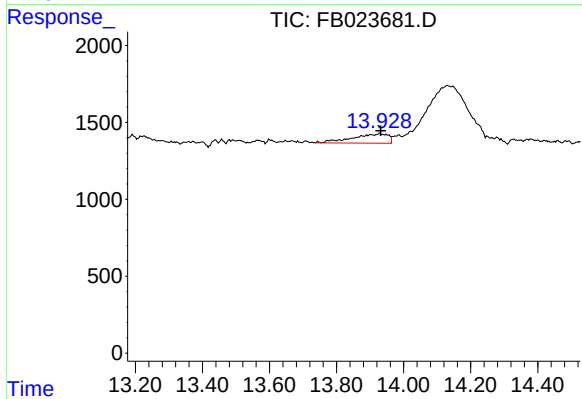

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.002 min
Response: 4530
Conc: 0.13 ng/ml

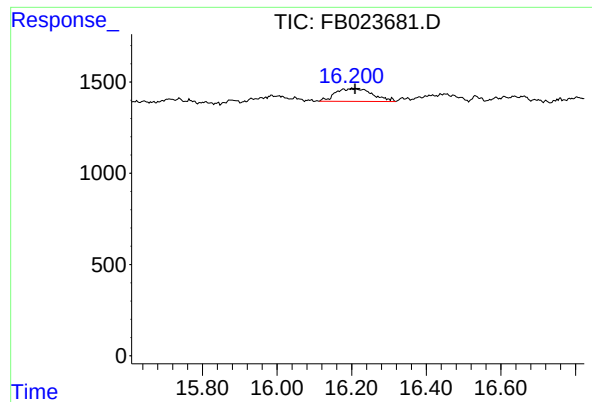

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: -0.008 min
Response: 4784
Conc: 0.16 ng/ml