

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021920\
Data File : FB023688.D
Signal(s) : FID2B.CH
Acq On : 19 Feb 2020 12:38
Operator : DD/AJ
Sample : L1573-06
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 20 00:35:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	242163	11.894 ng/ml
Target Compounds			
8) t m-Xylene	13.193	1109	0.031 ng/ml
9) t O-Xylene	13.908	826	0.024 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021920\
Data File : FB023688.D
Signal(s) : FID2B.CH
Acq On : 19 Feb 2020 12:38
Operator : DD/AJ
Sample : L1573-06
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 20 00:35:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

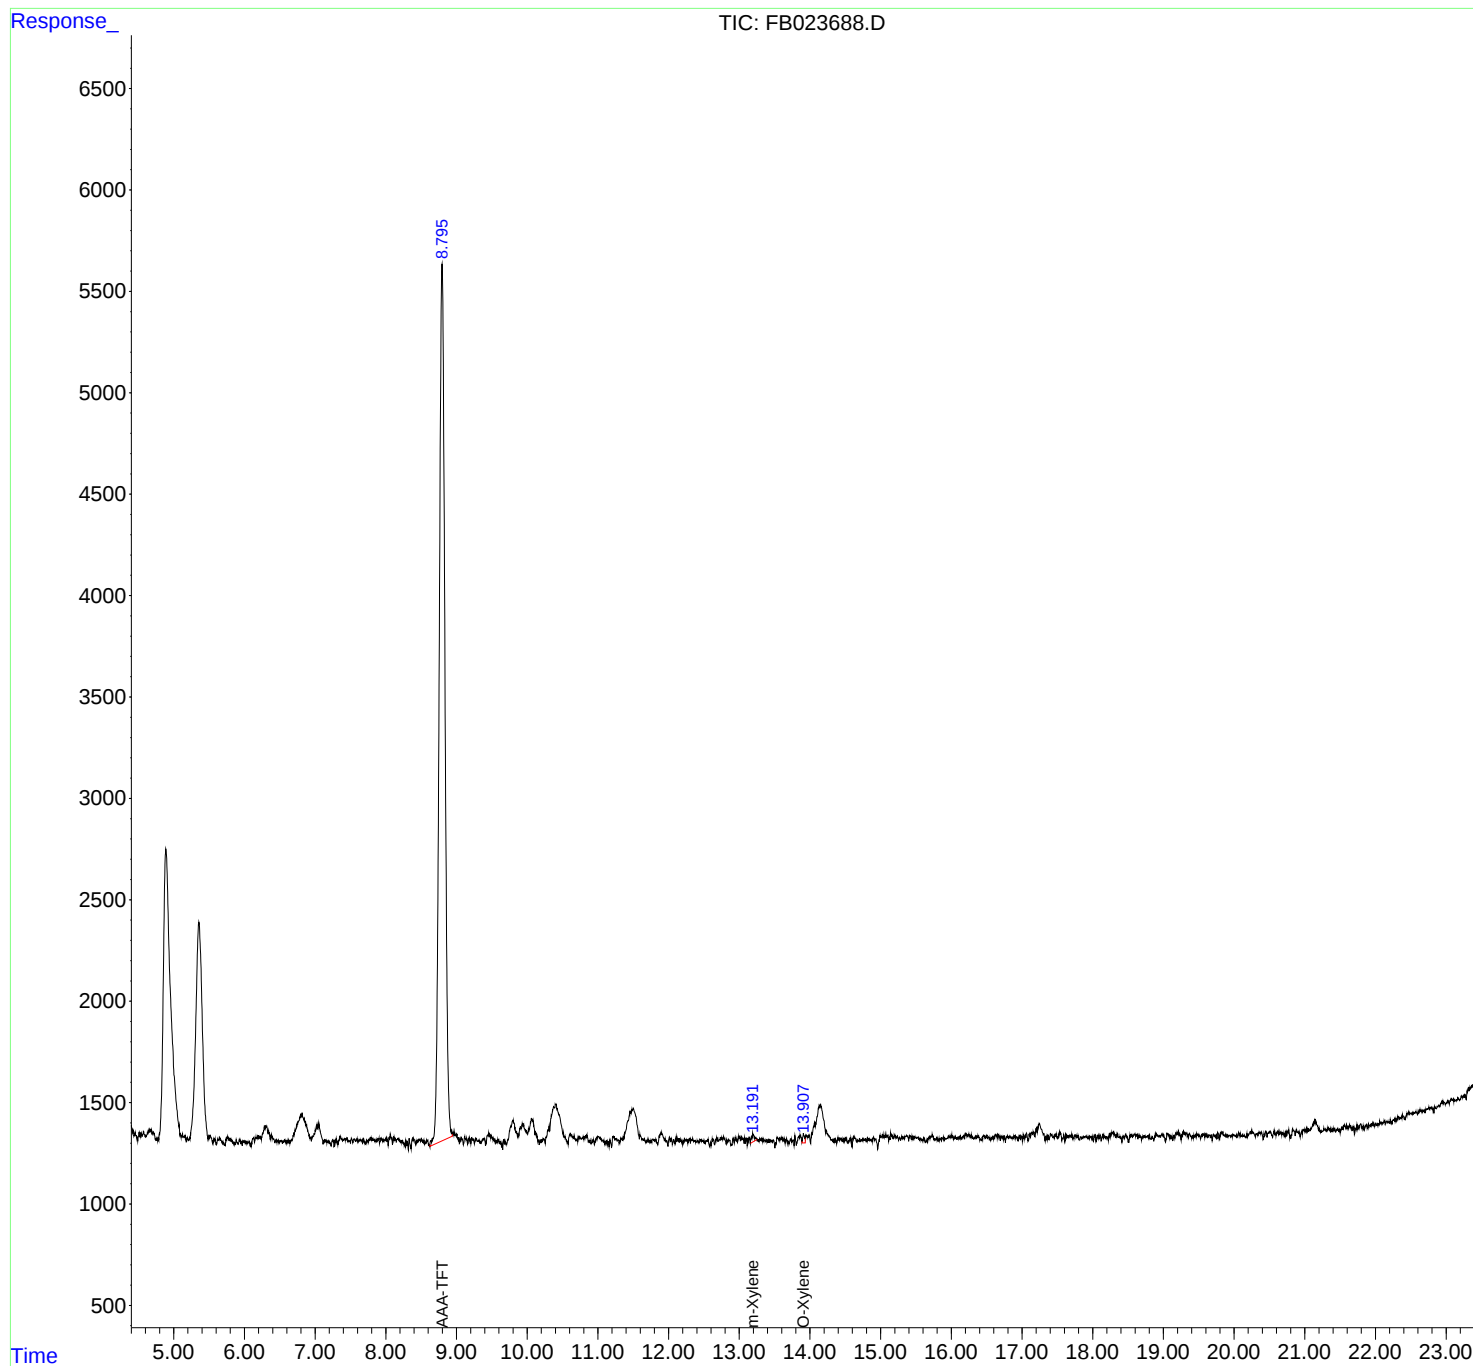

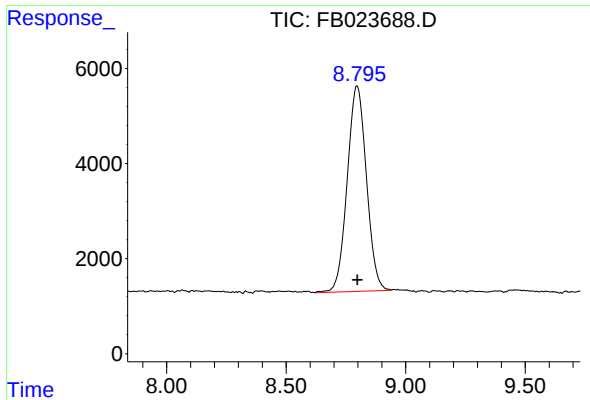


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 242163
Conc: 11.89 ng/ml

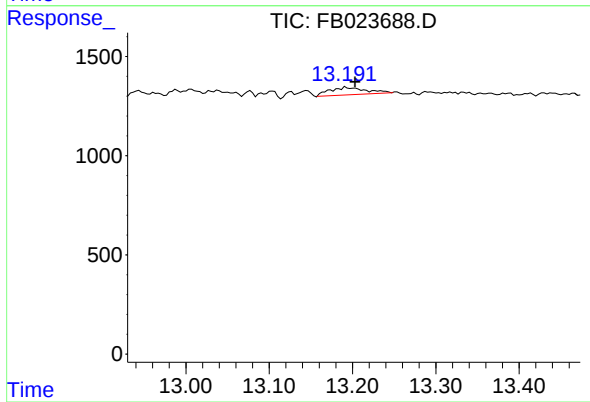

#8 m-Xylene

R.T.: 13.193 min
Delta R.T.: -0.011 min
Response: 1109
Conc: 0.03 ng/ml

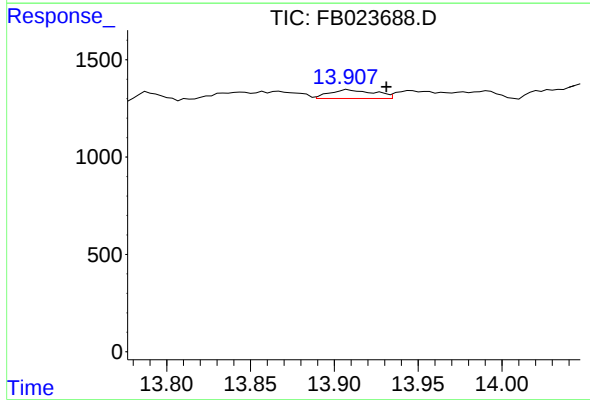

#9 O-Xylene

R.T.: 13.908 min
Delta R.T.: -0.023 min
Response: 826
Conc: 0.02 ng/ml