

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021920\
 Data File : FB023686.D
 Signal(s) : FID2B.CH
 Acq On : 19 Feb 2020 11:38
 Operator : DD/AJ
 Sample : L1573-02MSD
 Misc : 5.09g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 20 00:35:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	443470	21.782 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	774285	25.732 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	806379	24.712 ng/ml
3) t n-Heptane	7.754	257305	7.997 ng/ml
4) t Benzene	7.889	384042	9.390 ng/ml
6) t Toluene	10.627	1118036	28.166 ng/ml
7) t Ethylbenzene	13.067	351879	9.465 ng/ml
8) t m-Xylene	13.200	681131	19.073 ng/ml
9) t O-Xylene	13.927	659706	19.128 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	560336	19.138 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB021920\
Data File : FB023686.D
Signal(s) : FID2B.CH
Acq On : 19 Feb 2020 11:38
Operator : DD/AJ
Sample : L1573-02MSD
Misc : 5.09g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 20 00:35:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

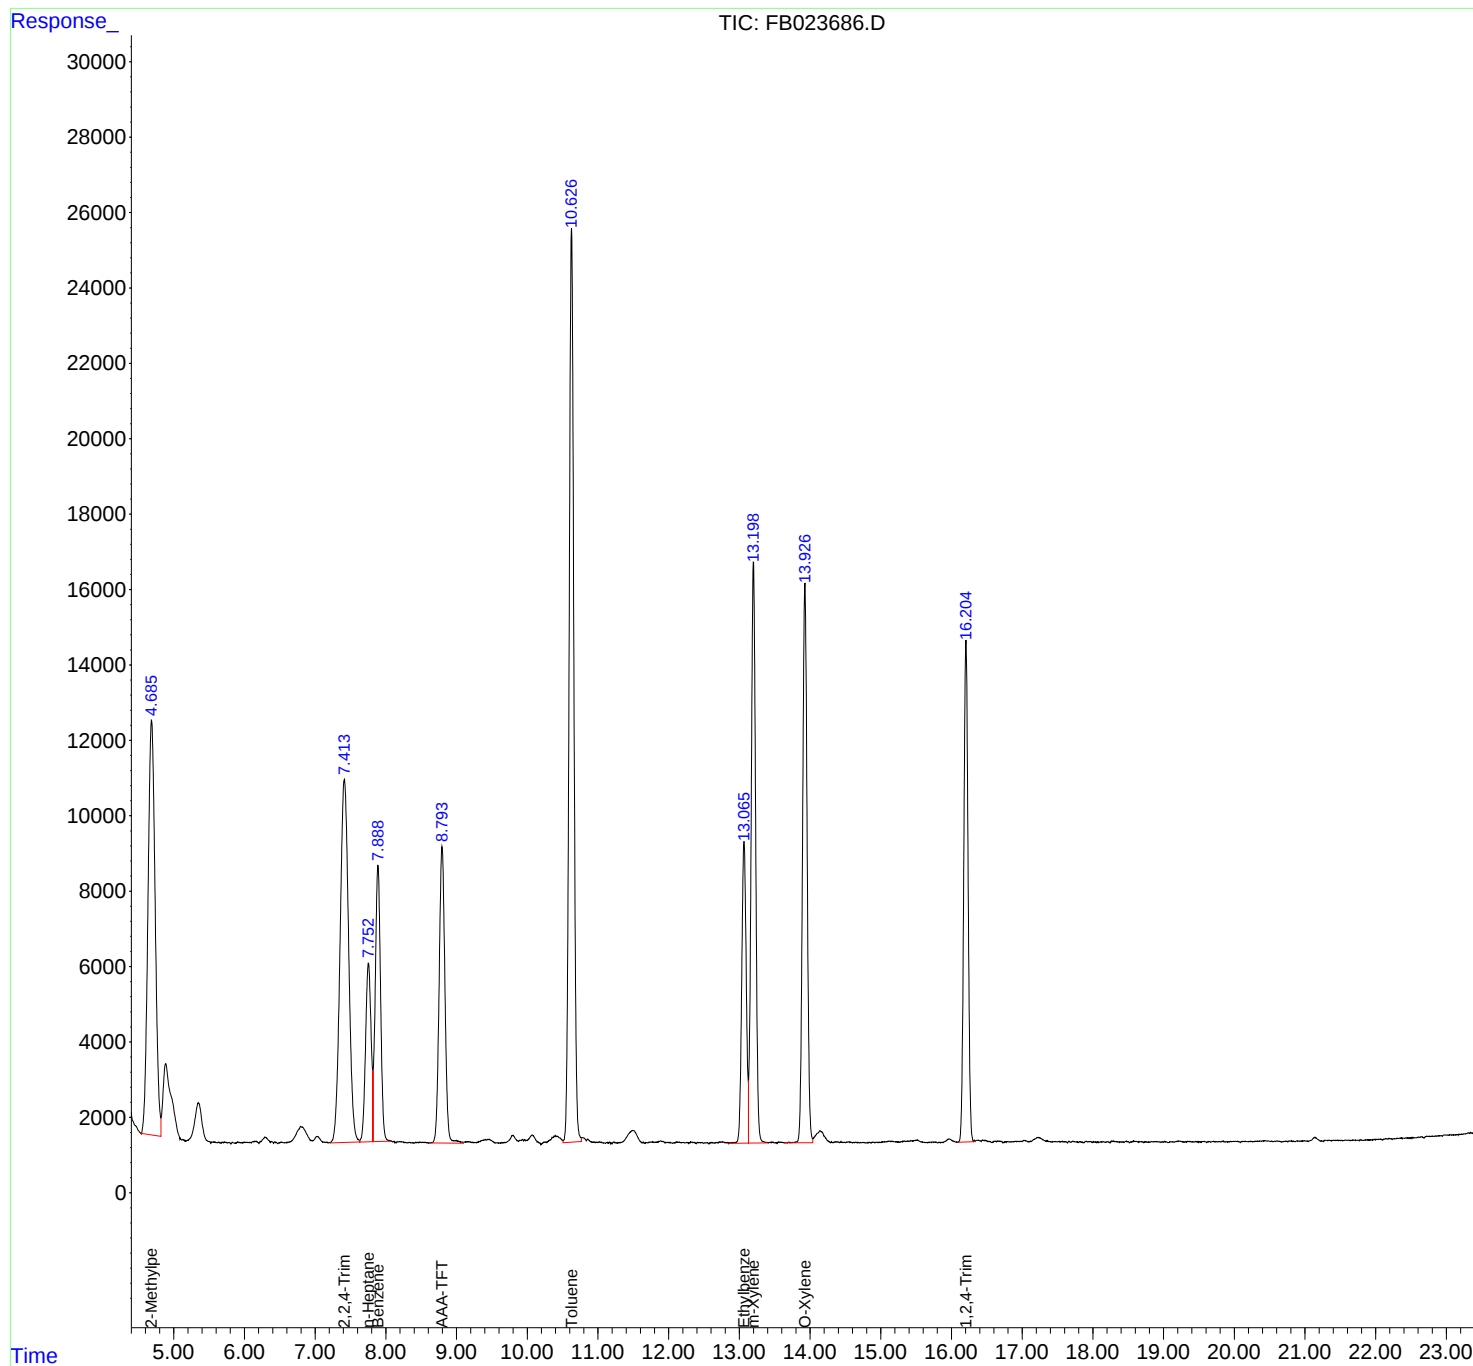

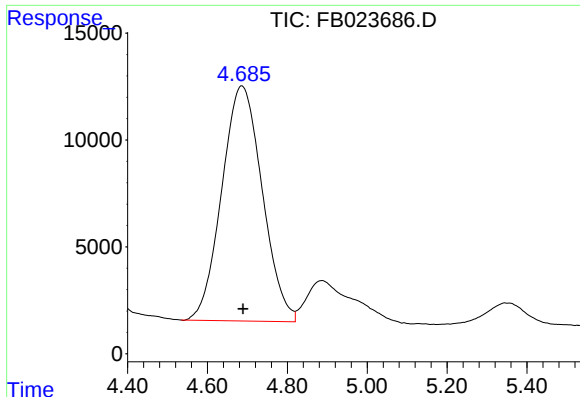


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: -0.003 min
Response: 774285
Conc: 25.73 ng/ml

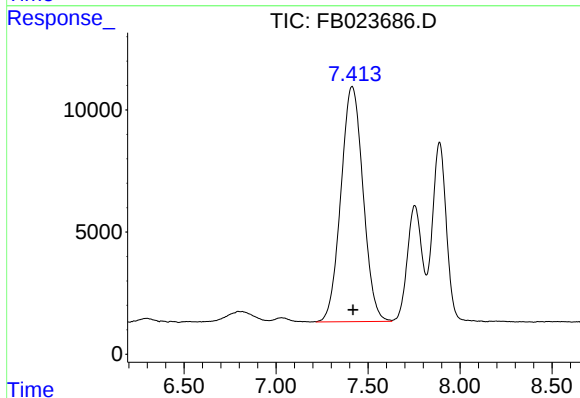


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 806379
Conc: 24.71 ng/ml

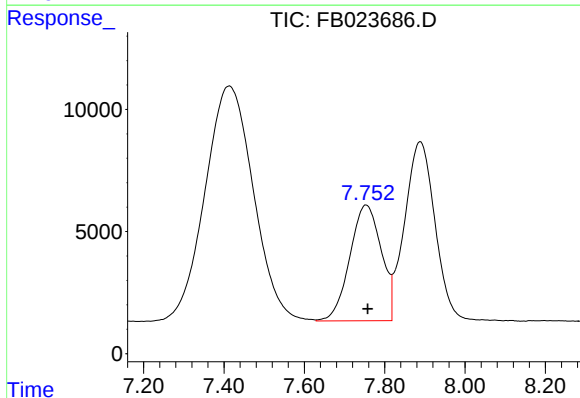


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.004 min
Response: 257305
Conc: 8.00 ng/ml

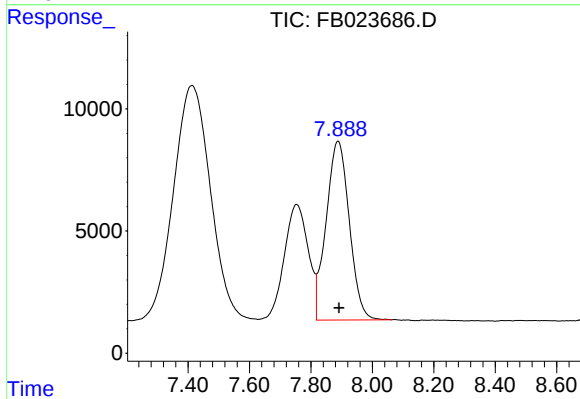


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.002 min
Response: 384042
Conc: 9.39 ng/ml

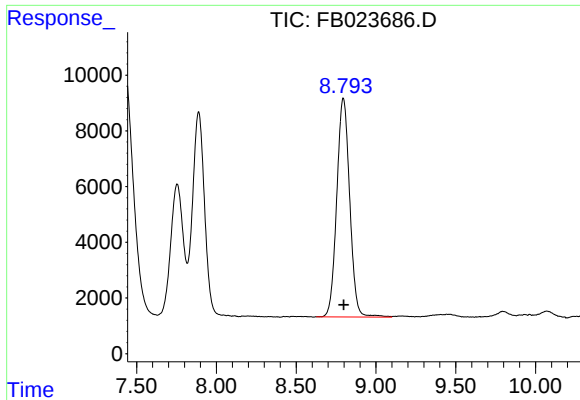


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.003 min
Response: 443470
Conc: 21.78 ng/ml

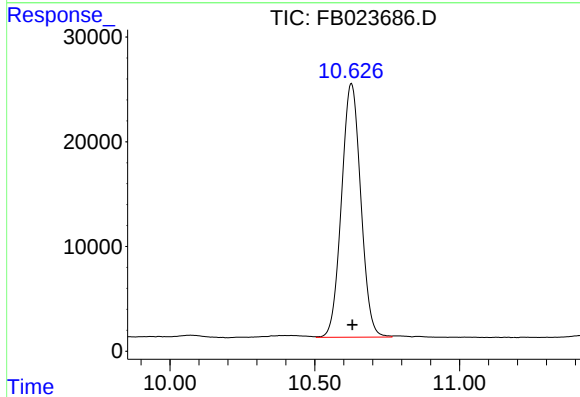


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.003 min
Response: 1118036
Conc: 28.17 ng/ml

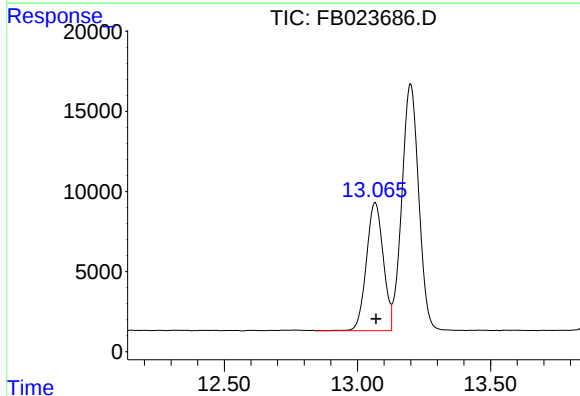


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.004 min
Response: 351879
Conc: 9.47 ng/ml

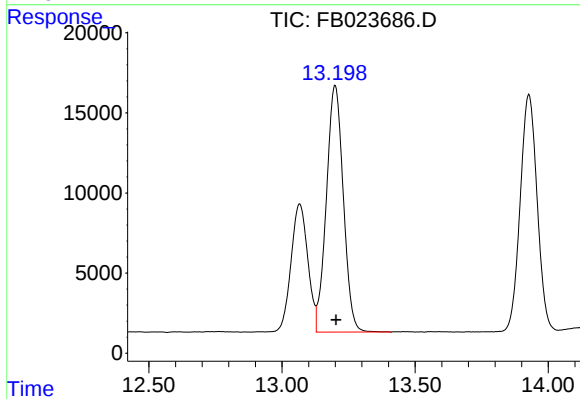


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.003 min
Response: 681131
Conc: 19.07 ng/ml

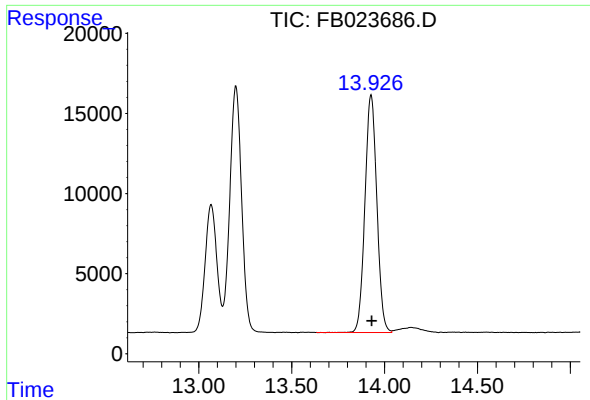

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.004 min
Response: 659706
Conc: 19.13 ng/ml

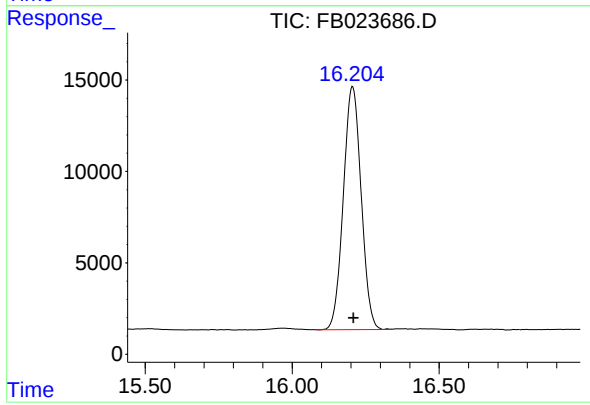

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.003 min
Response: 560336
Conc: 19.14 ng/ml