

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022019\
 Data File : FB019838.D
 Signal(s) : FID2B.CH
 Acq On : 20 Feb 2019 9:41
 Operator : MJ/SJ
 Sample : BSF0220S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 21 00:24:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.039	215522	18.437 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.896	577751	33.371 ng/ml
2) t 2,2,4-Trimethylpentane	7.654	565726	34.114 ng/ml
3) t n-Heptane	7.995	174566	10.833 ng/ml
4) t Benzene	8.132	192764	10.220 ng/ml
6) t Toluene	10.886	517625	29.591 ng/ml
7) t Ethylbenzene	13.338	214905	9.793 ng/ml
8) t m-Xylene	13.470	449219	19.627 ng/ml
9) t O-Xylene	14.202	434057	19.434 ng/ml
10) t 1,2,4-Trimethylbenzene	16.488	446890	19.287 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022019\
Data File : FB019838.D
Signal(s) : FID2B.CH
Acq On : 20 Feb 2019 9:41
Operator : MJ/SJ
Sample : BSF0220S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 21 00:24:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

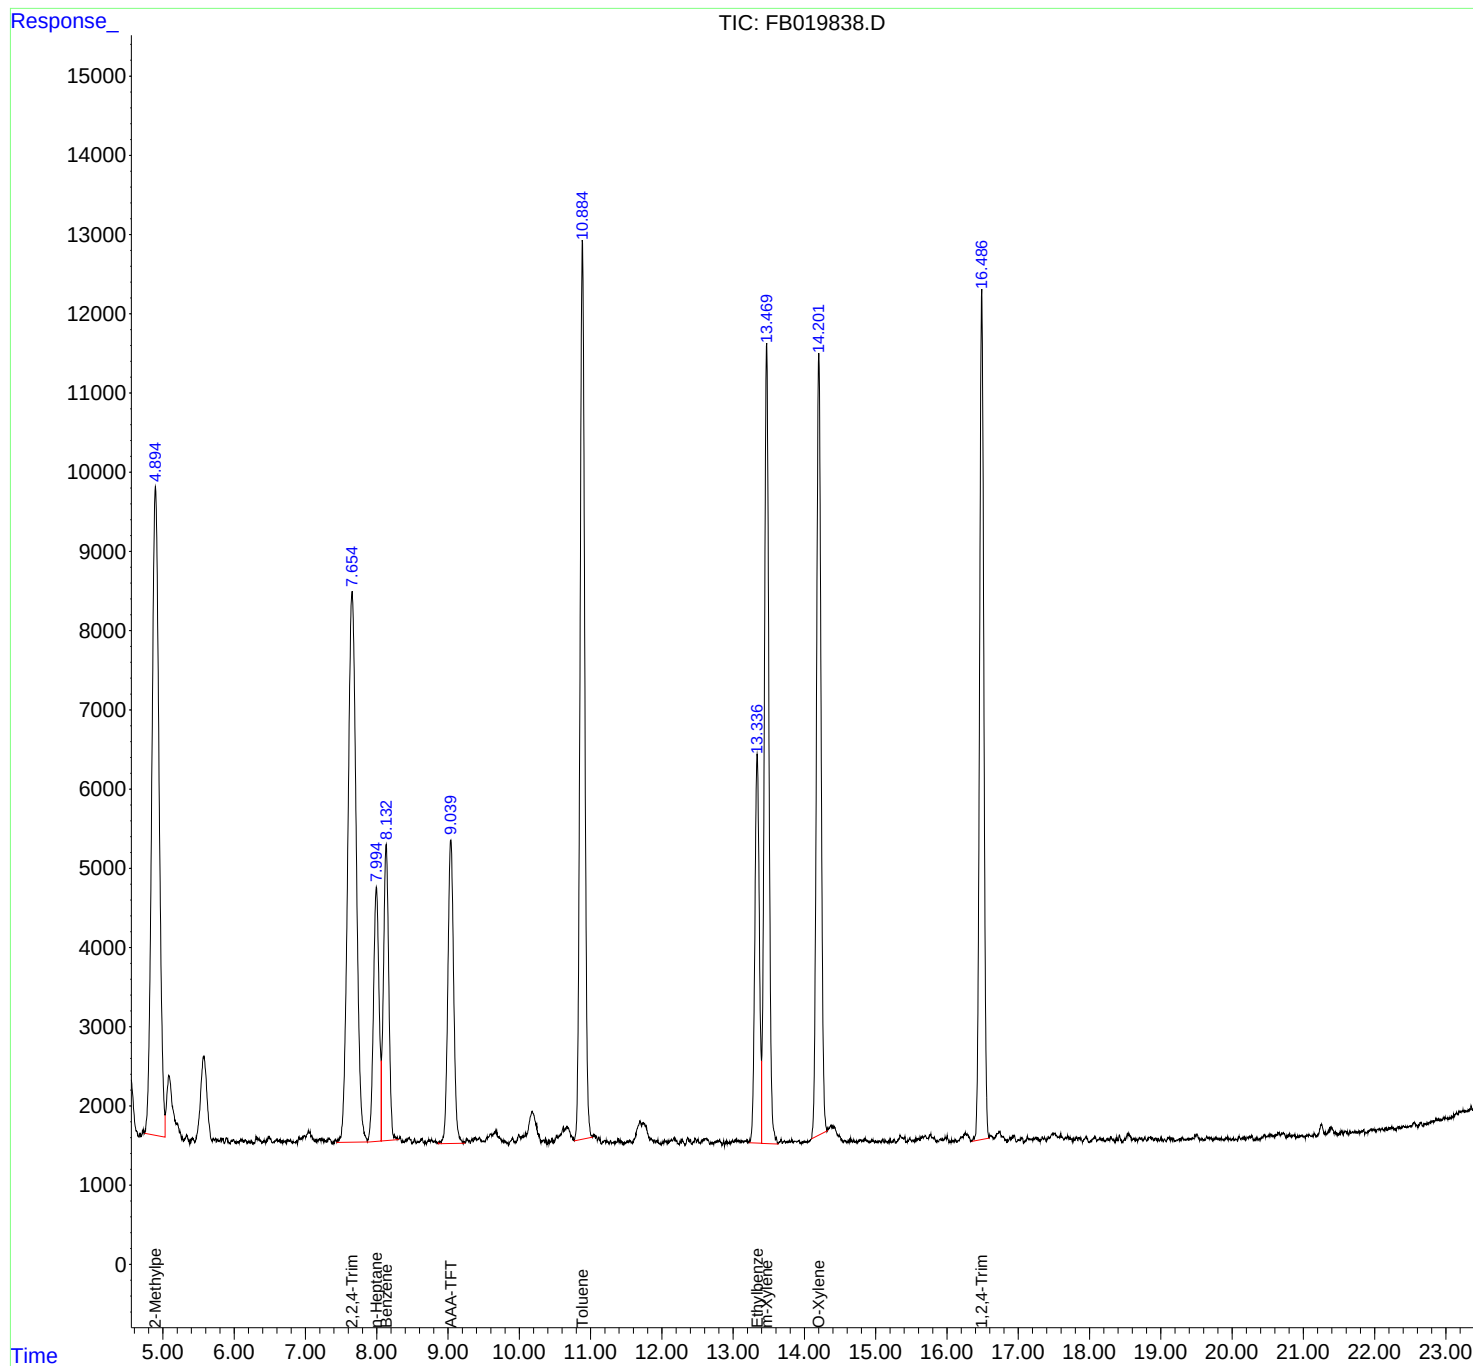

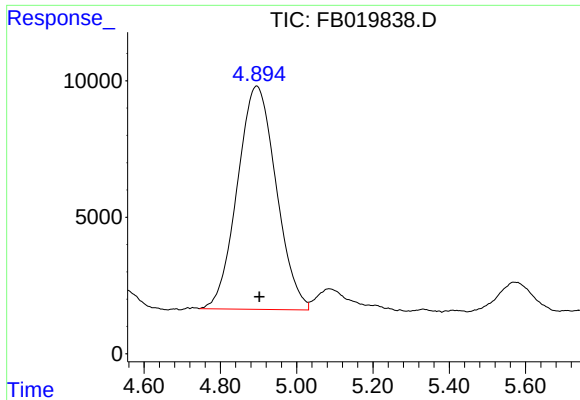


#1 2-Methylpentane

R.T.: 4.896 min
Delta R.T.: -0.006 min
Response: 577751
Conc: 33.37 ng/ml

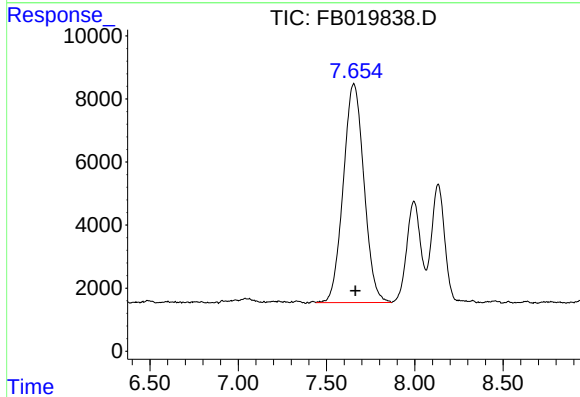


#2 2,2,4-Trimethylpentane

R.T.: 7.654 min
Delta R.T.: -0.010 min
Response: 565726
Conc: 34.11 ng/ml

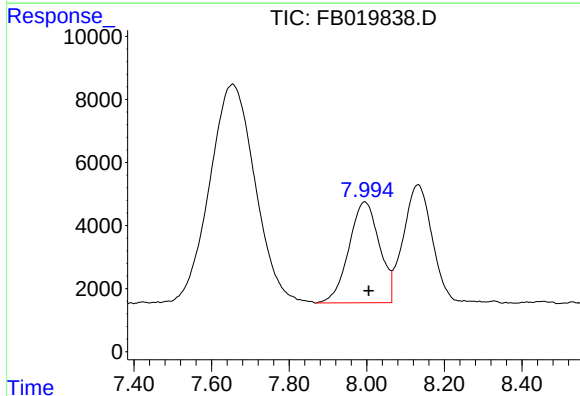


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: -0.009 min
Response: 174566
Conc: 10.83 ng/ml

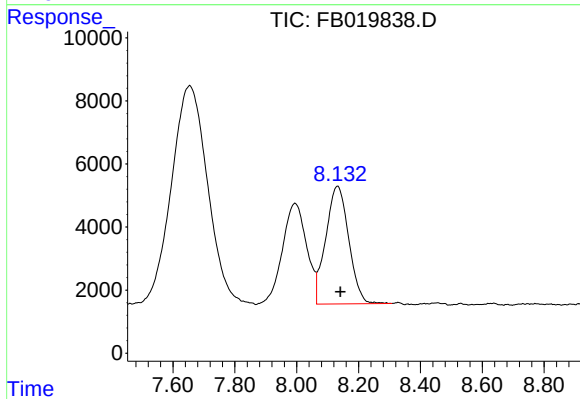


#4 Benzene

R.T.: 8.132 min
Delta R.T.: -0.009 min
Response: 192764
Conc: 10.22 ng/ml

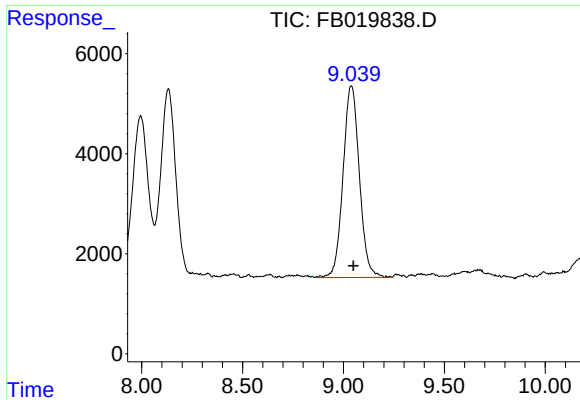


#5 AAA-TFT

R.T.: 9.039 min
Delta R.T.: -0.010 min
Response: 215522
Conc: 18.44 ng/ml

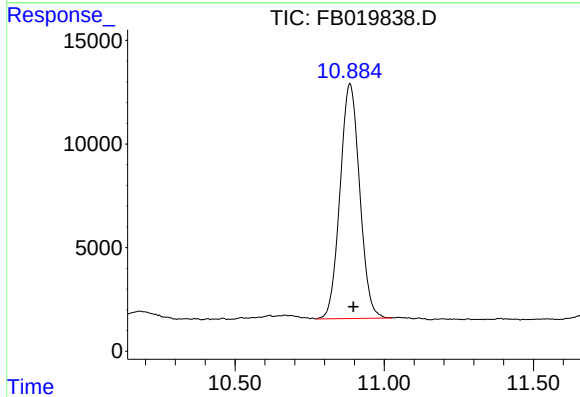


#6 Toluene

R.T.: 10.886 min
Delta R.T.: -0.011 min
Response: 517625
Conc: 29.59 ng/ml

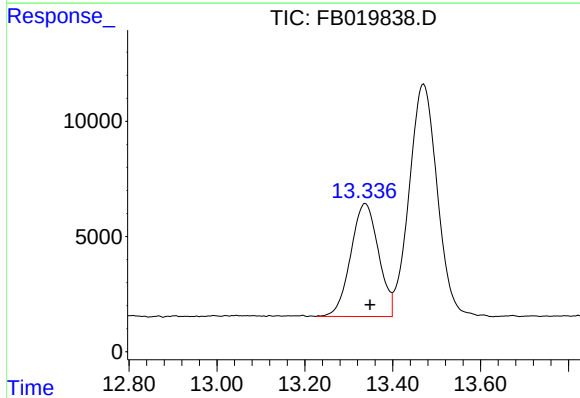


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: -0.011 min
Response: 214905
Conc: 9.79 ng/ml

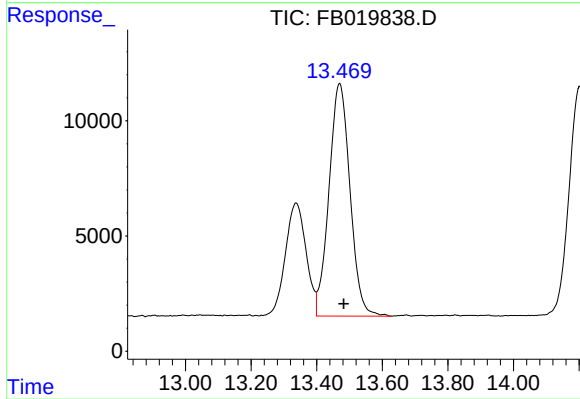


#8 m-Xylene

R.T.: 13.470 min
Delta R.T.: -0.012 min
Response: 449219
Conc: 19.63 ng/ml

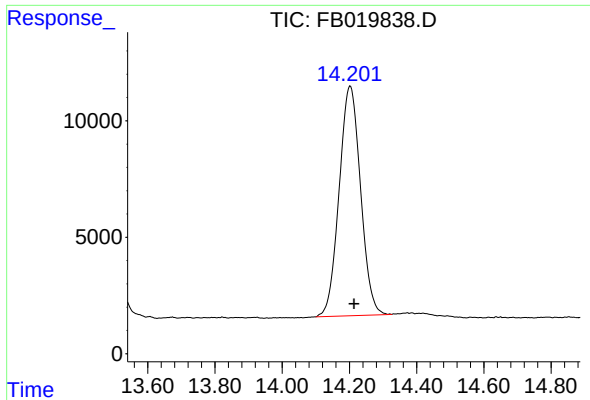

#9 O-Xylene

R.T.: 14.202 min
Delta R.T.: -0.012 min
Response: 434057
Conc: 19.43 ng/ml

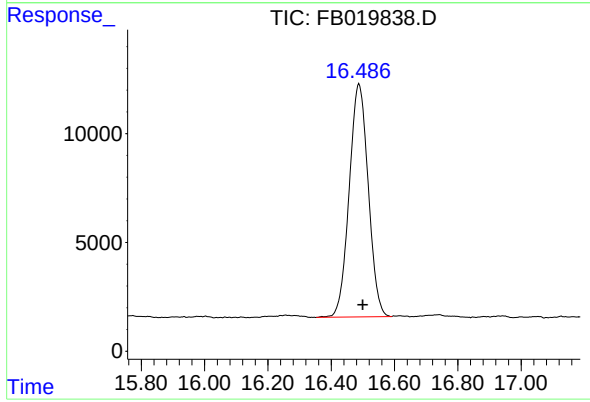

#10 1,2,4-Trimethylbenzene

R.T.: 16.488 min
Delta R.T.: -0.012 min
Response: 446890
Conc: 19.29 ng/ml