

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022019\
 Data File : FB019842.D
 Signal(s) : FID2B.CH
 Acq On : 20 Feb 2019 11:57
 Operator : MJ/SJ
 Sample : K1349-09MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 21 00:25:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	222673	19.049 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.895	515086	29.751 ng/ml
2) t 2,2,4-Trimethylpentane	7.656	444216	26.787 ng/ml
3) t n-Heptane	7.995	137158	8.511 ng/ml
4) t Benzene	8.133	183504	9.729 ng/ml
6) t Toluene	10.887	460460	26.323 ng/ml
7) t Ethylbenzene	13.339	188326	8.581 ng/ml
8) t m-Xylene	13.472	386177	16.873 ng/ml
9) t O-Xylene	14.203	383622	17.176 ng/ml
10) t 1,2,4-Trimethylbenzene	16.489	371702	16.042 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022019\
Data File : FB019842.D
Signal(s) : FID2B.CH
Acq On : 20 Feb 2019 11:57
Operator : MJ/SJ
Sample : K1349-09MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 21 00:25:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

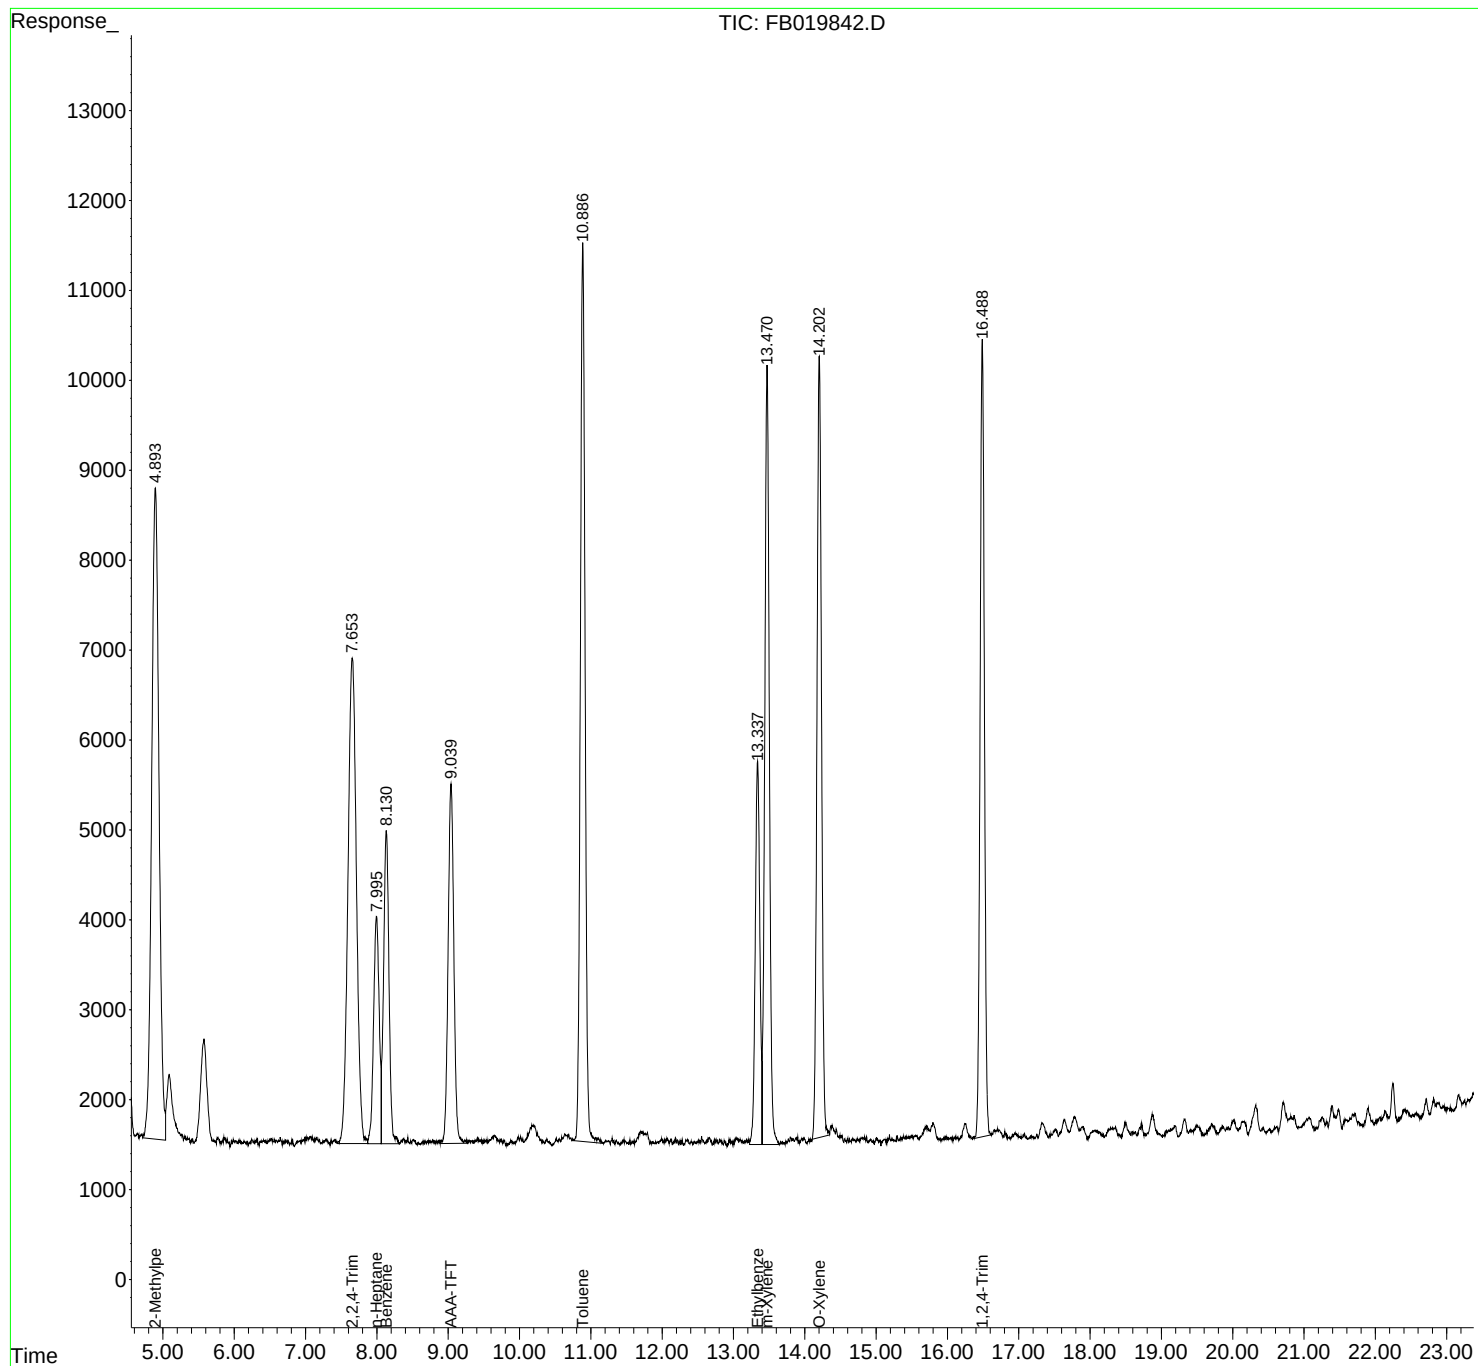

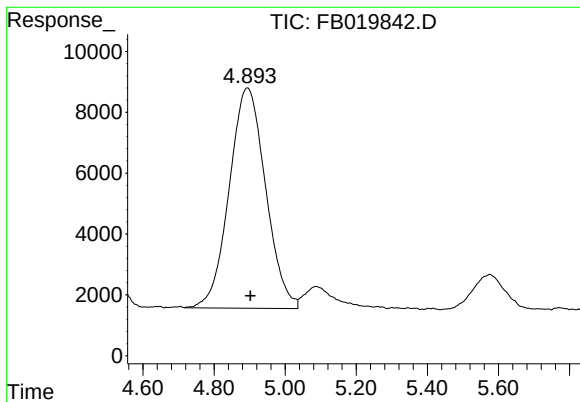


#1 2-Methylpentane

R.T.: 4.895 min
 Delta R.T.: -0.007 min
 Response: 515086
 Conc: 29.75 ng/ml

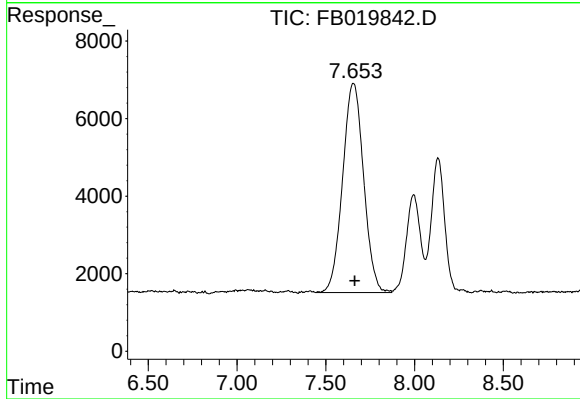


#2 2,2,4-Trimethylpentane

R.T.: 7.656 min
 Delta R.T.: -0.009 min
 Response: 444216
 Conc: 26.79 ng/ml

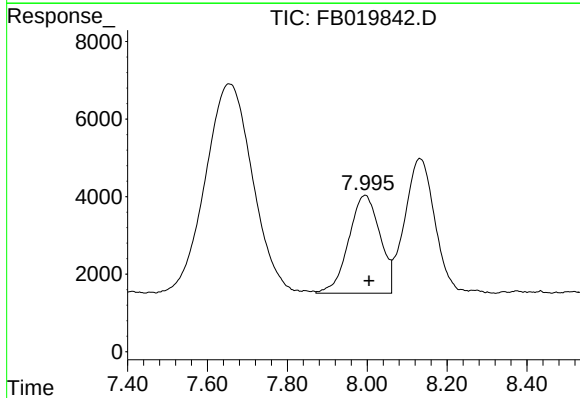


#3 n-Heptane

R.T.: 7.995 min
 Delta R.T.: -0.010 min
 Response: 137158
 Conc: 8.51 ng/ml

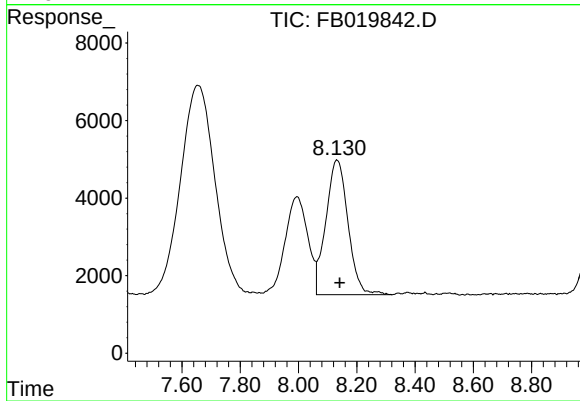


#4 Benzene

R.T.: 8.133 min
 Delta R.T.: -0.008 min
 Response: 183504
 Conc: 9.73 ng/ml

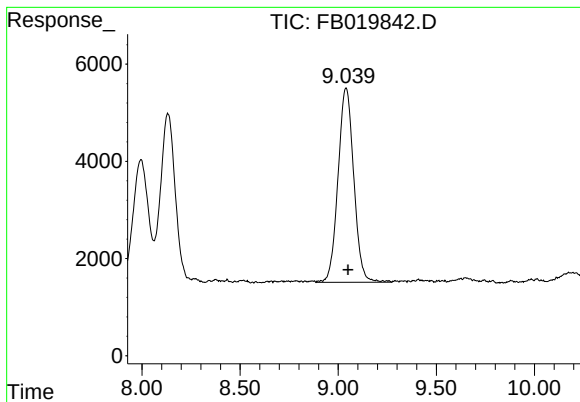


#5 AAA-TFT

R.T.: 9.040 min
Delta R.T.: -0.009 min
Response: 222673
Conc: 19.05 ng/ml

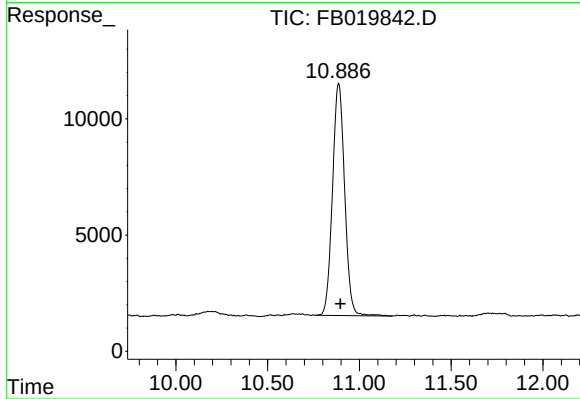


#6 Toluene

R.T.: 10.887 min
Delta R.T.: -0.009 min
Response: 460460
Conc: 26.32 ng/ml

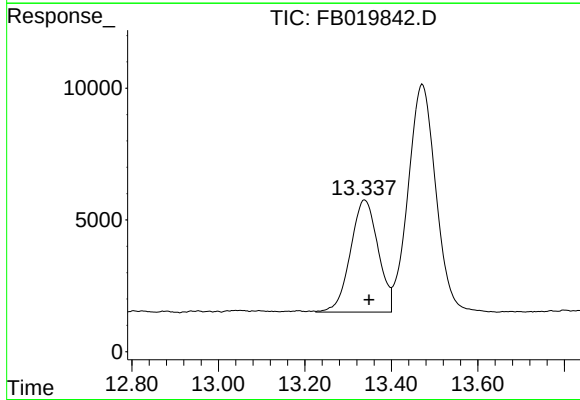


#7 Ethylbenzene

R.T.: 13.339 min
Delta R.T.: -0.010 min
Response: 188326
Conc: 8.58 ng/ml

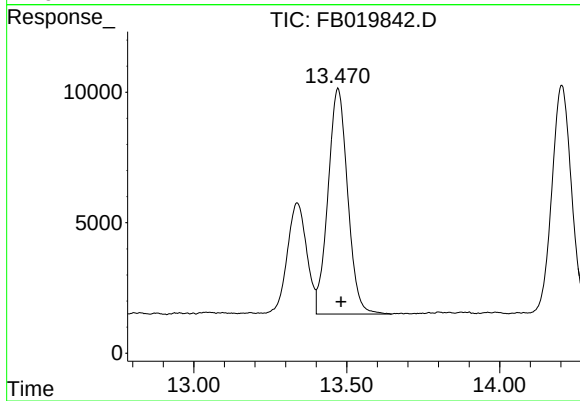


#8 m-Xylene

R.T.: 13.472 min
Delta R.T.: -0.010 min
Response: 386177
Conc: 16.87 ng/ml

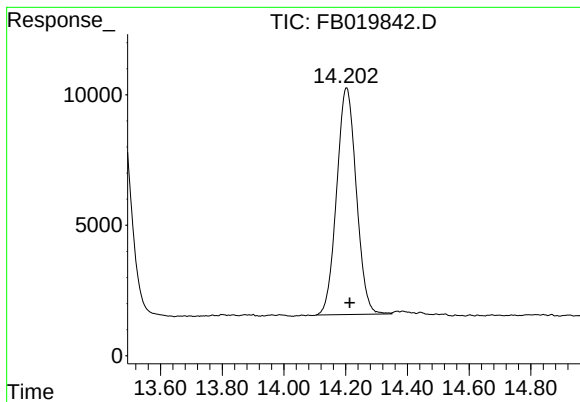

#9 O-Xylene

R.T.: 14.203 min
Delta R.T.: -0.010 min
Response: 383622
Conc: 17.18 ng/ml

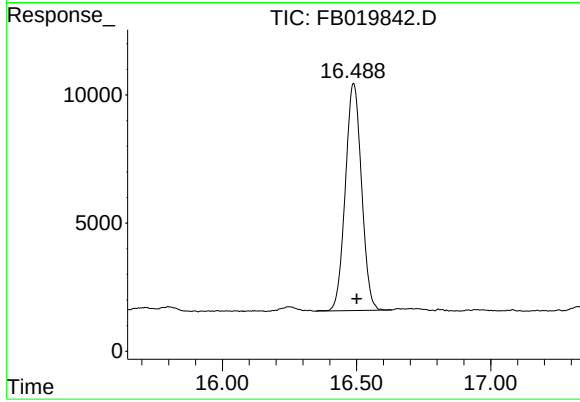

#10 1,2,4-Trimethylbenzene

R.T.: 16.489 min
Delta R.T.: -0.011 min
Response: 371702
Conc: 16.04 ng/ml