

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022120\
Data File : FB023703.D
Signal(s) : FID2B.CH
Acq On : 21 Feb 2020 13:09
Operator : DD/AJ
Sample : L1636-01MS
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 21 22:08:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.793	447682	21.989 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.687	818396	27.198 ng/ml
2) t	2,2,4-Trimethylpentane	7.412	884860	27.117 ng/ml
3) t	n-Heptane	7.753	272732	8.477 ng/ml
4) t	Benzene	7.887	401430	9.815 ng/ml
6) t	Toluene	10.624	1173901	29.573 ng/ml
7) t	Ethylbenzene	13.064	353572	9.511 ng/ml
8) t	m-Xylene	13.197	682770	19.119 ng/ml
9) t	O-Xylene	13.925	661376	19.176 ng/ml
10) t	1,2,4-Trimethylbenzene	16.203	551804	18.847 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022120\
Data File : FB023703.D
Signal(s) : FID2B.CH
Acq On : 21 Feb 2020 13:09
Operator : DD/AJ
Sample : L1636-01MS
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 21 22:08:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

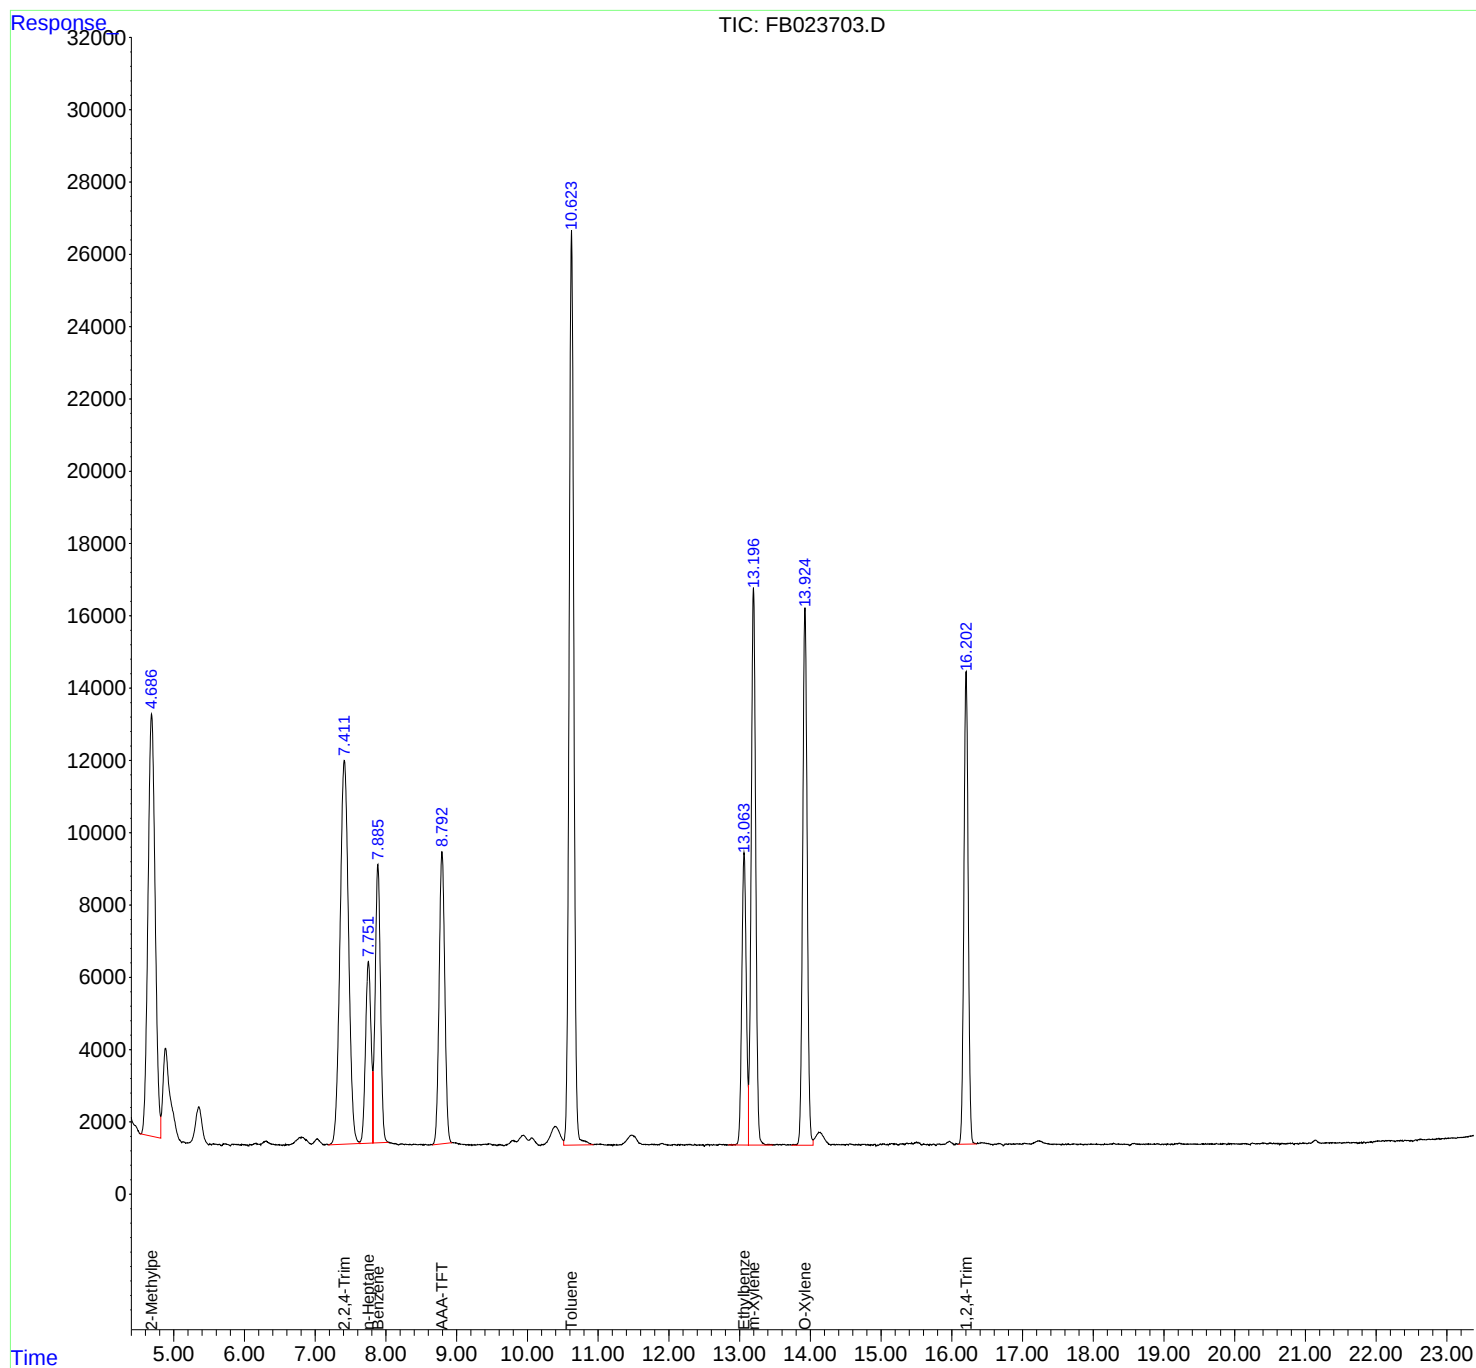

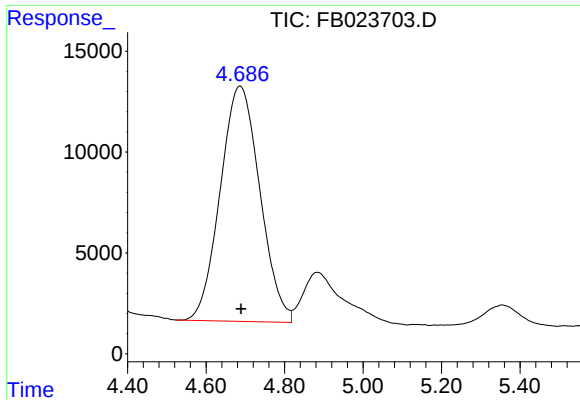


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: -0.002 min
Response: 818396
Conc: 27.20 ng/ml

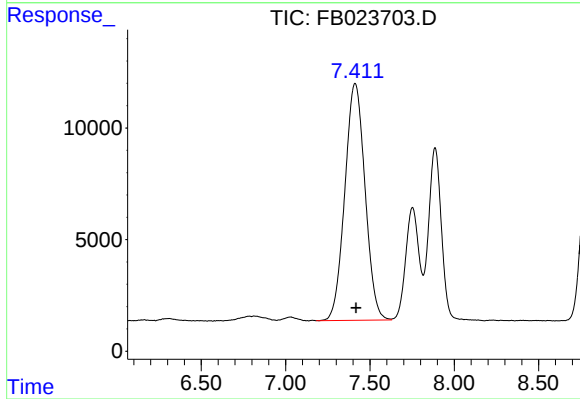


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.006 min
Response: 884860
Conc: 27.12 ng/ml

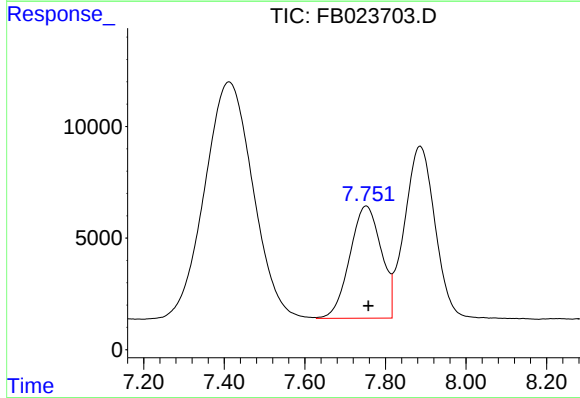


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.005 min
Response: 272732
Conc: 8.48 ng/ml

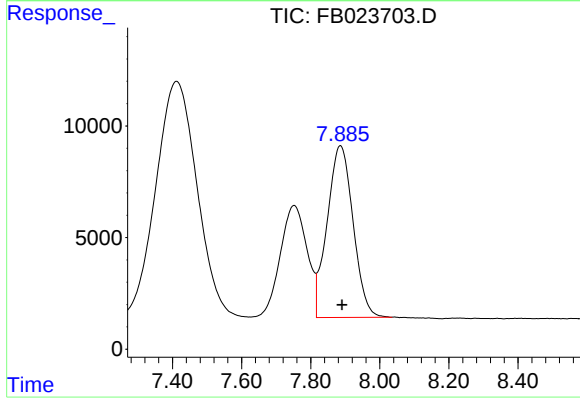


#4 Benzene

R.T.: 7.887 min
Delta R.T.: -0.005 min
Response: 401430
Conc: 9.81 ng/ml

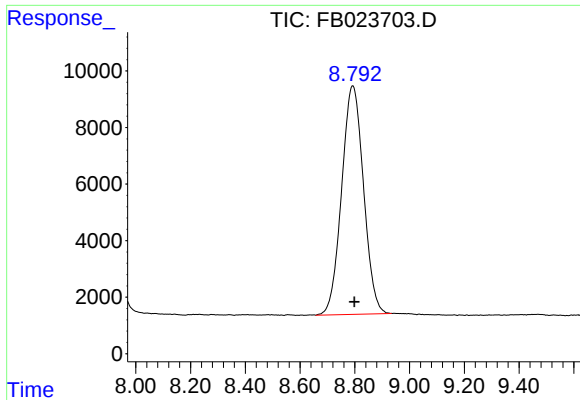


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.006 min
Response: 447682
Conc: 21.99 ng/ml

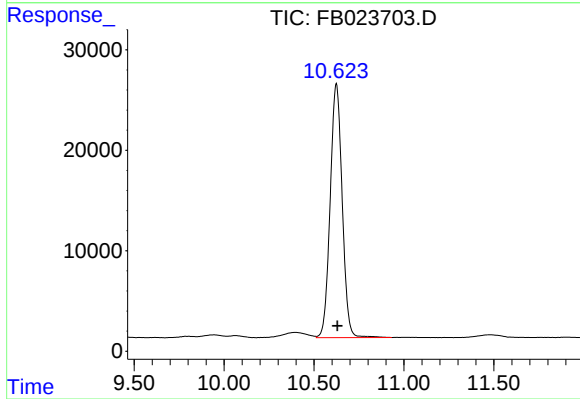


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.006 min
Response: 1173901
Conc: 29.57 ng/ml

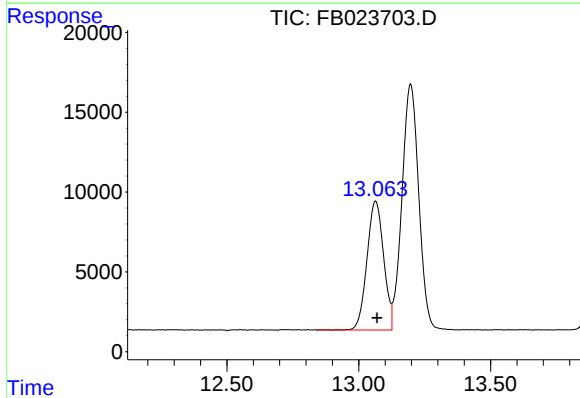


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: -0.006 min
Response: 353572
Conc: 9.51 ng/ml

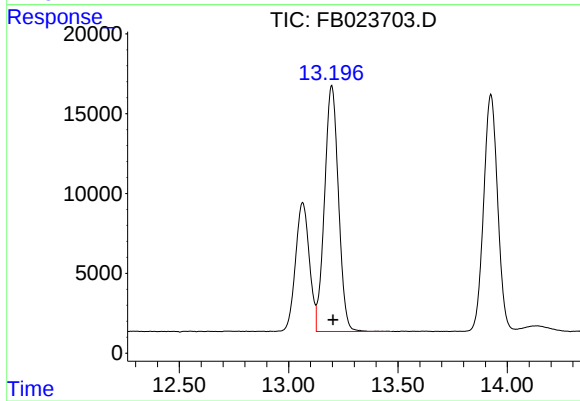


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: -0.006 min
Response: 682770
Conc: 19.12 ng/ml

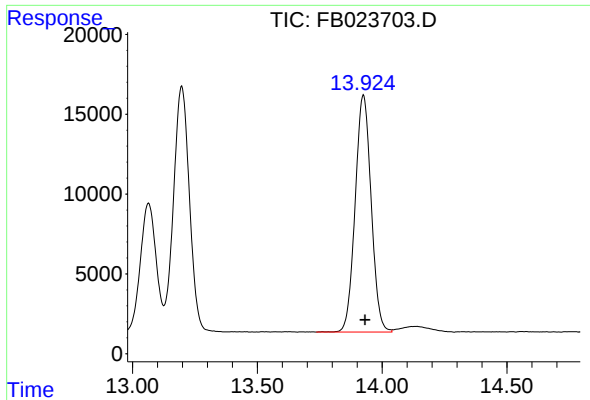

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: -0.006 min
Response: 661376
Conc: 19.18 ng/ml

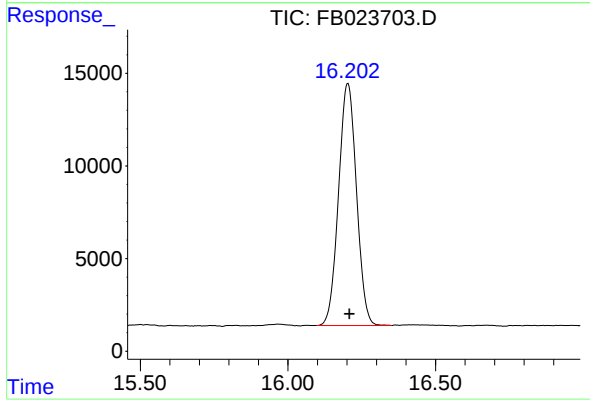

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min
Delta R.T.: -0.006 min
Response: 551804
Conc: 18.85 ng/ml