

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022120\
 Data File : FB023704.D
 Signal(s) : FID2B.CH
 Acq On : 21 Feb 2020 13:39
 Operator : DD/AJ
 Sample : L1636-01MSD
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 21 22:08:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	404108	19.848 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	696127	23.135 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	652783	20.005 ng/ml
3) t n-Heptane	7.752	201103	6.250 ng/ml
4) t Benzene	7.887	375106	9.171 ng/ml
6) t Toluene	10.624	1048971	26.426 ng/ml
7) t Ethylbenzene	13.065	306747	8.251 ng/ml
8) t m-Xylene	13.197	589877	16.518 ng/ml
9) t O-Xylene	13.925	576232	16.707 ng/ml
10) t 1,2,4-Trimethylbenzene	16.204	458774	15.669 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022120\
Data File : FB023704.D
Signal(s) : FID2B.CH
Acq On : 21 Feb 2020 13:39
Operator : DD/AJ
Sample : L1636-01MSD
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 21 22:08:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

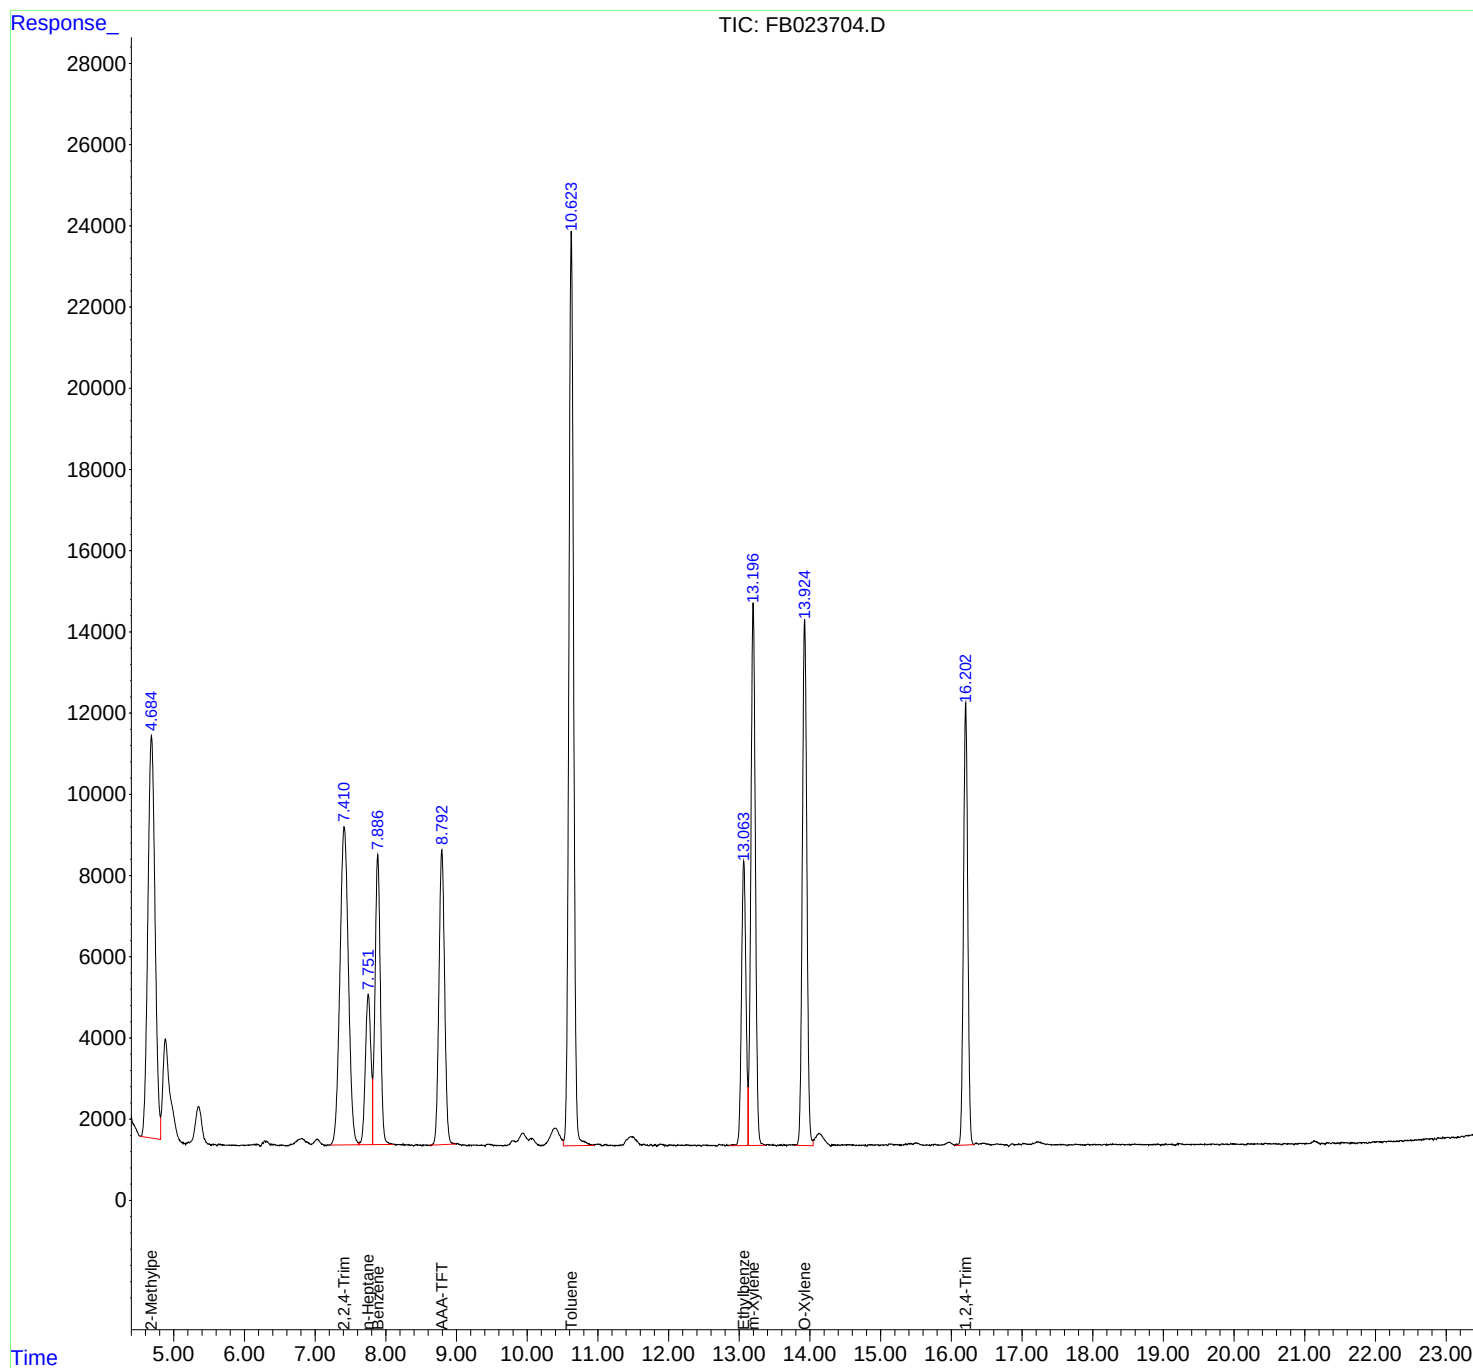

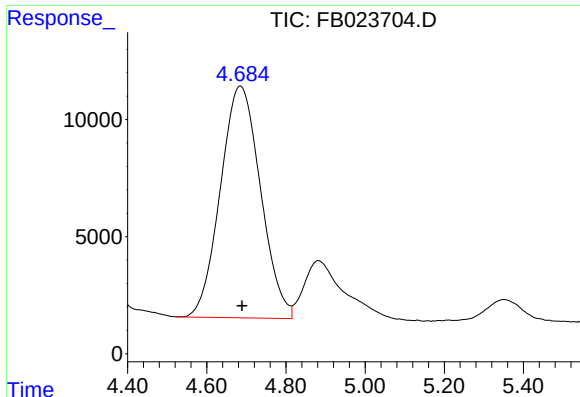


#1 2-Methylpentane

R.T.: 4.685 min
Delta R.T.: -0.004 min
Response: 696127
Conc: 23.13 ng/ml

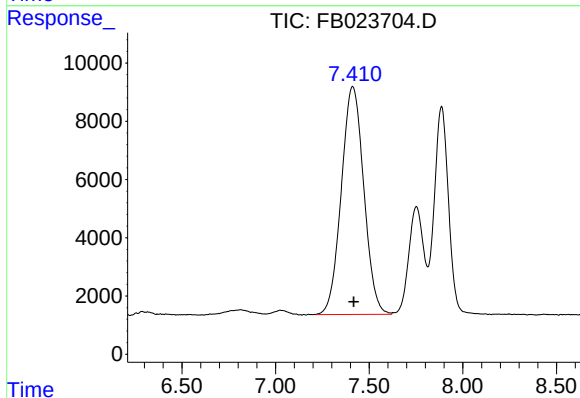


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.006 min
Response: 652783
Conc: 20.00 ng/ml

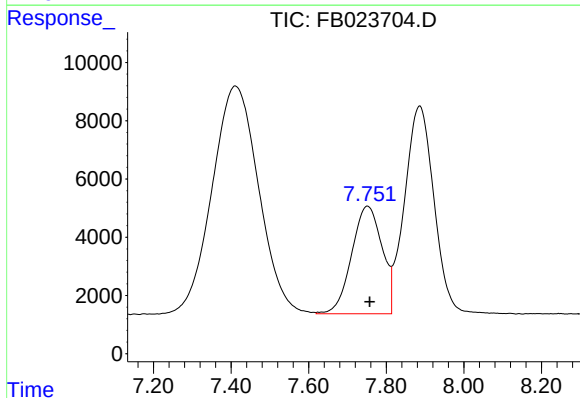


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.005 min
Response: 201103
Conc: 6.25 ng/ml

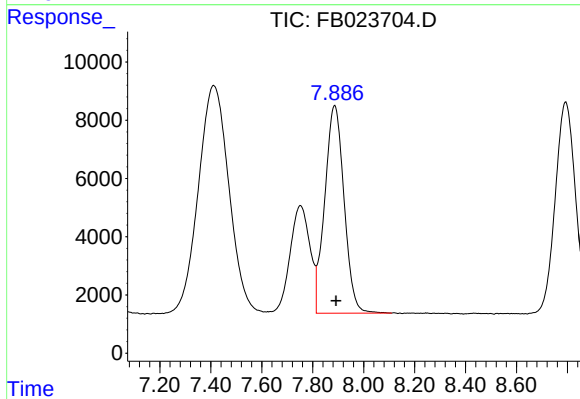


#4 Benzene

R.T.: 7.887 min
Delta R.T.: -0.004 min
Response: 375106
Conc: 9.17 ng/ml

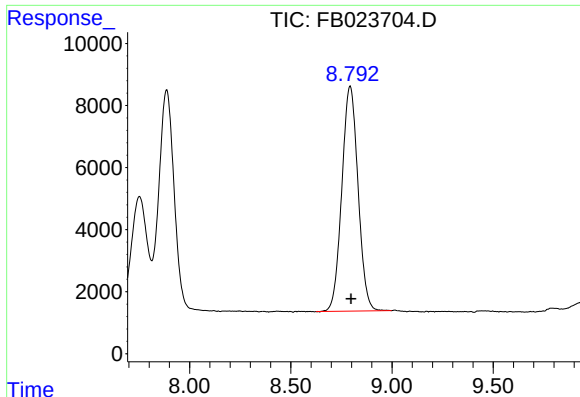


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.005 min
Response: 404108
Conc: 19.85 ng/ml

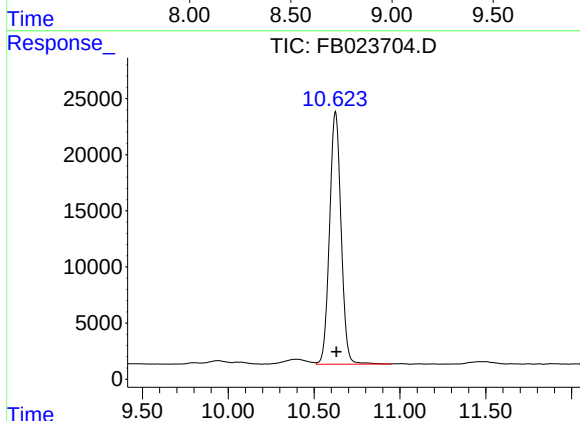


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.006 min
Response: 1048971
Conc: 26.43 ng/ml

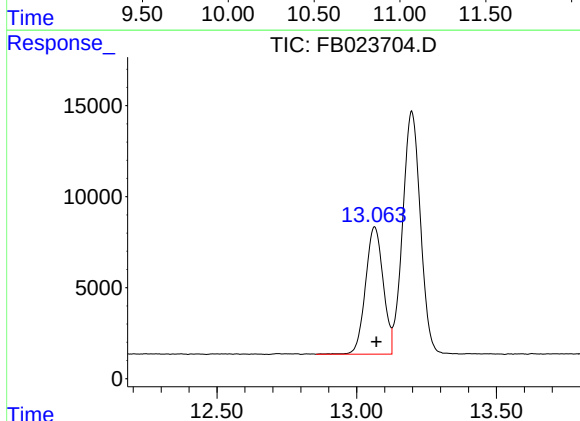


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.006 min
Response: 306747
Conc: 8.25 ng/ml

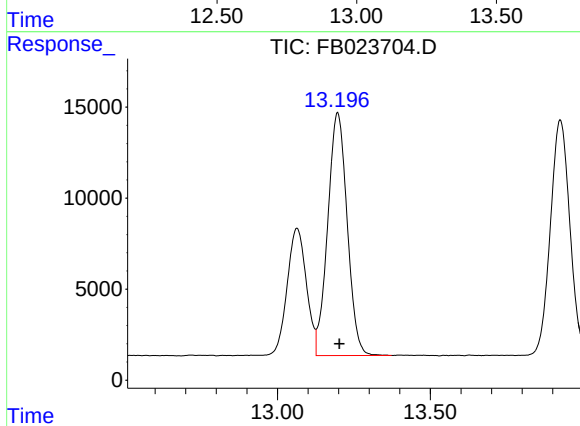


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: -0.006 min
Response: 589877
Conc: 16.52 ng/ml

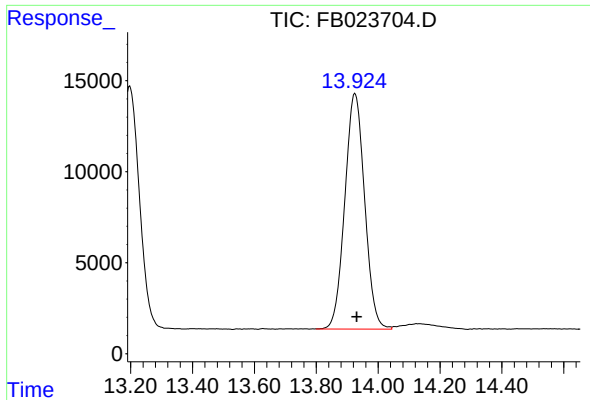

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: -0.006 min
Response: 576232
Conc: 16.71 ng/ml

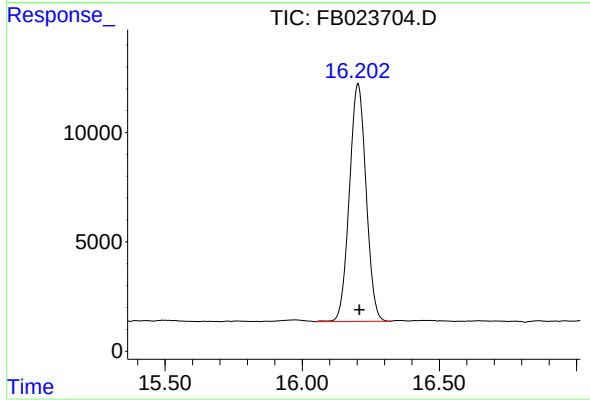

#10 1,2,4-Trimethylbenzene

R.T.: 16.204 min
Delta R.T.: -0.005 min
Response: 458774
Conc: 15.67 ng/ml