

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022120\
 Data File : FB023700.D
 Signal(s) : FID2B.CH
 Acq On : 21 Feb 2020 11:39
 Operator : DD/AJ
 Sample : BSF0221S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 21 22:08:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
 Quant Title :
 QLast Update : Thu Feb 06 11:13:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.791	351646	17.272 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.682	850535	28.266 ng/ml
2) t	2,2,4-Trimethylpentane	7.410	998330	30.594 ng/ml
3) t	n-Heptane	7.750	314040	9.761 ng/ml
4) t	Benzene	7.884	390531	9.548 ng/ml
6) t	Toluene	10.622	1165876	29.371 ng/ml
7) t	Ethylbenzene	13.063	370149	9.957 ng/ml
8) t	m-Xylene	13.196	709114	19.857 ng/ml
9) t	O-Xylene	13.924	684169	19.837 ng/ml
10) t	1,2,4-Trimethylbenzene	16.202	607425	20.746 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022120\
Data File : FB023700.D
Signal(s) : FID2B.CH
Acq On : 21 Feb 2020 11:39
Operator : DD/AJ
Sample : BSF0221S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 21 22:08:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020620.M
Quant Title :
QLast Update : Thu Feb 06 11:13:47 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

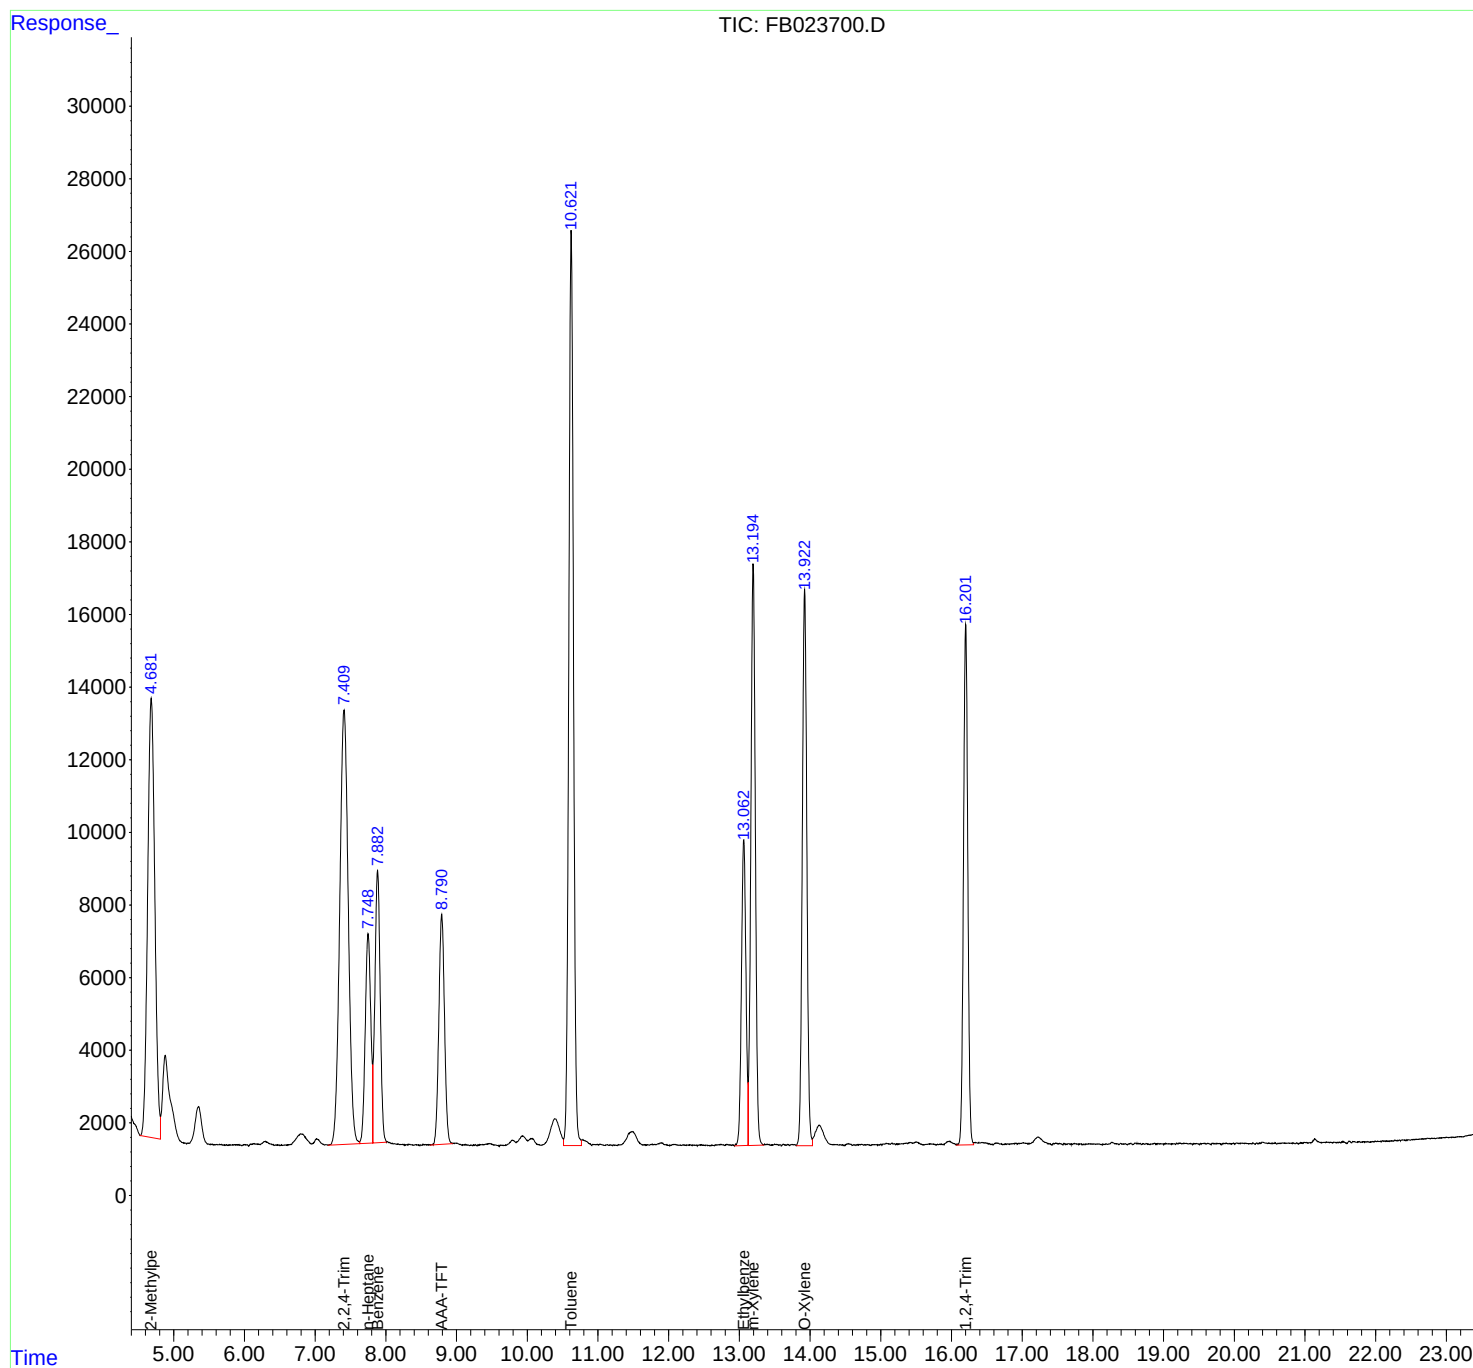

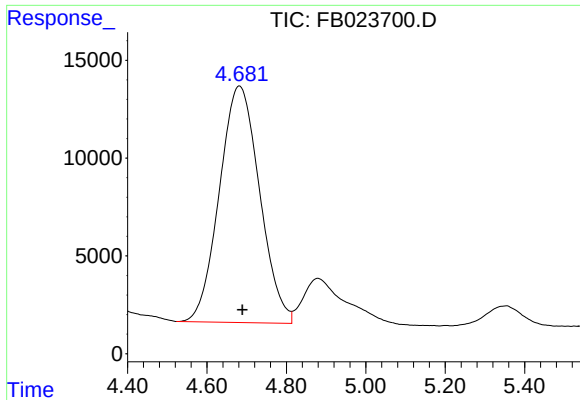


#1 2-Methylpentane

R.T.: 4.682 min
Delta R.T.: -0.007 min
Response: 850535
Conc: 28.27 ng/ml

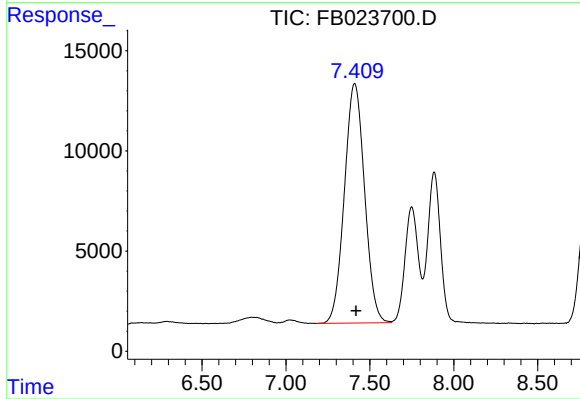


#2 2,2,4-Trimethylpentane

R.T.: 7.410 min
Delta R.T.: -0.007 min
Response: 998330
Conc: 30.59 ng/ml

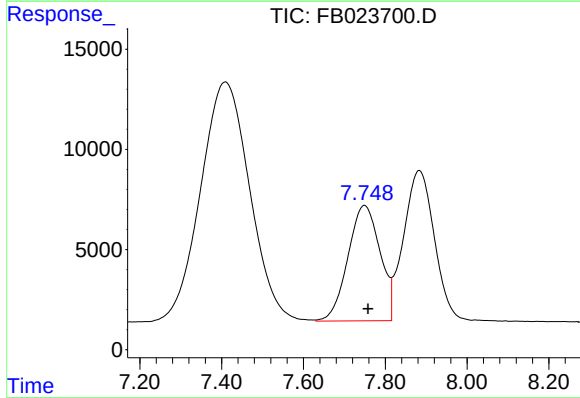


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.008 min
Response: 314040
Conc: 9.76 ng/ml

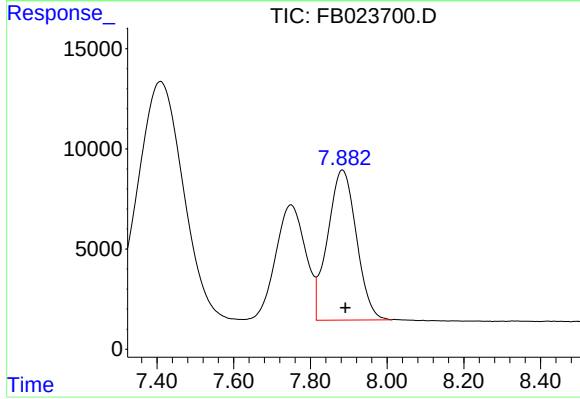


#4 Benzene

R.T.: 7.884 min
Delta R.T.: -0.008 min
Response: 390531
Conc: 9.55 ng/ml

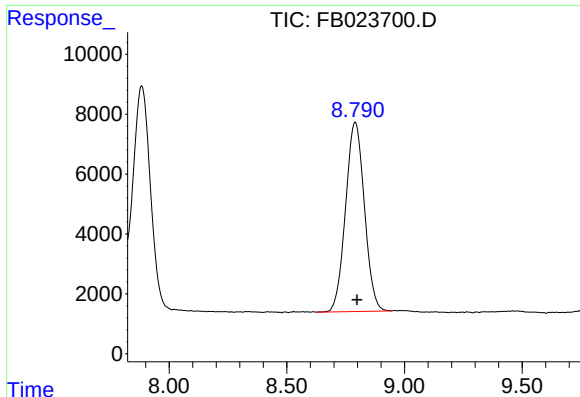


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: -0.008 min
Response: 351646
Conc: 17.27 ng/ml

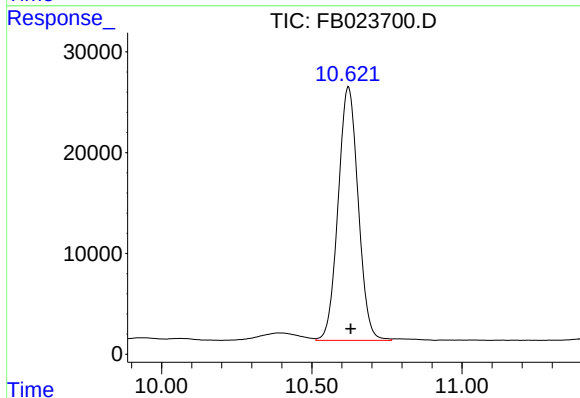


#6 Toluene

R.T.: 10.622 min
Delta R.T.: -0.008 min
Response: 1165876
Conc: 29.37 ng/ml

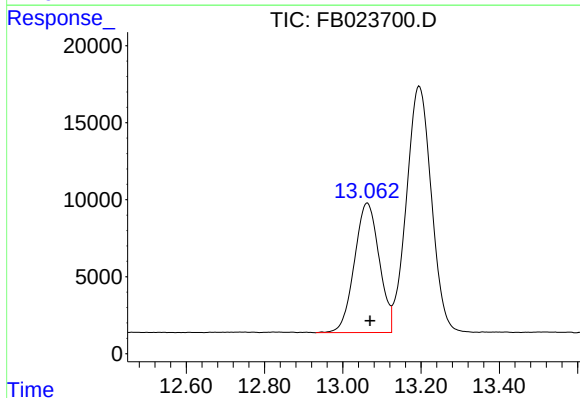


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: -0.007 min
Response: 370149
Conc: 9.96 ng/ml

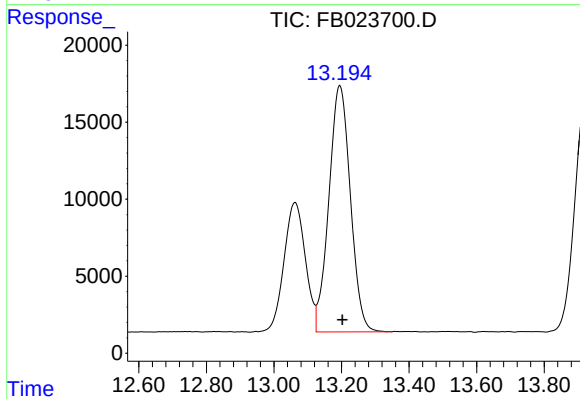

#8 m-Xylene

R.T.: 13.196 min
Delta R.T.: -0.007 min
Response: 709114
Conc: 19.86 ng/ml

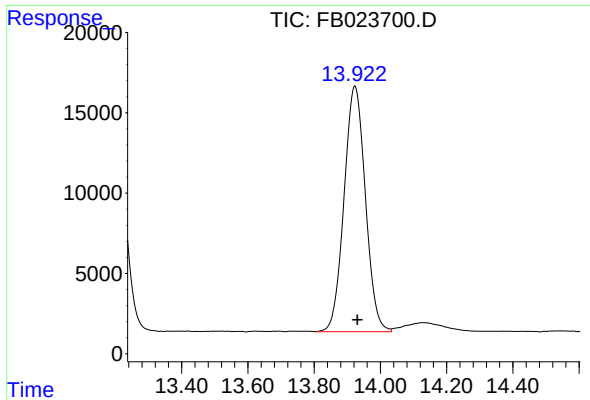


#9 O-Xylene

R.T.: 13.924 min

Delta R.T.: -0.008 min

Response: 684169

Conc: 19.84 ng/ml

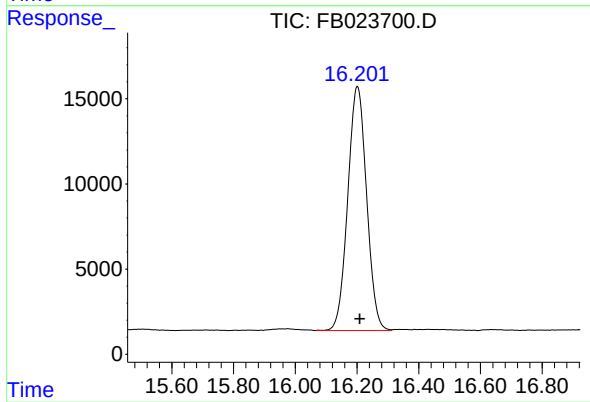

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min

Delta R.T.: -0.007 min

Response: 607425

Conc: 20.75 ng/ml