

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022123\
 Data File : FB029355.D
 Signal(s) : FID2B.CH
 Acq On : 21 Feb 2023 17:45
 Operator : YP/AJ
 Sample : 01627-01
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 22 05:00:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.792	237142	24.655 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.710	55936	3.525 ng/ml
2) t	2,2,4-Trimethylpentane	7.419	64588	3.750 ng/ml
3) t	n-Heptane	7.757	22641	1.251 ng/ml
4) t	Benzene	7.889	26066	1.251 ng/ml
6) t	Toluene	10.622	76878	3.794 ng/ml
7) t	Ethylbenzene	13.059	23338	1.223 ng/ml
8) t	m-Xylene	13.189	47718	2.517 ng/ml
9) t	O-Xylene	13.917	47027	2.577 ng/ml
10) t	1,2,4-Trimethylbenzene	16.193	48423	2.573 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022123\
Data File : FB029355.D
Signal(s) : FID2B.CH
Acq On : 21 Feb 2023 17:45
Operator : YP/AJ
Sample : 01627-01
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 22 05:00:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

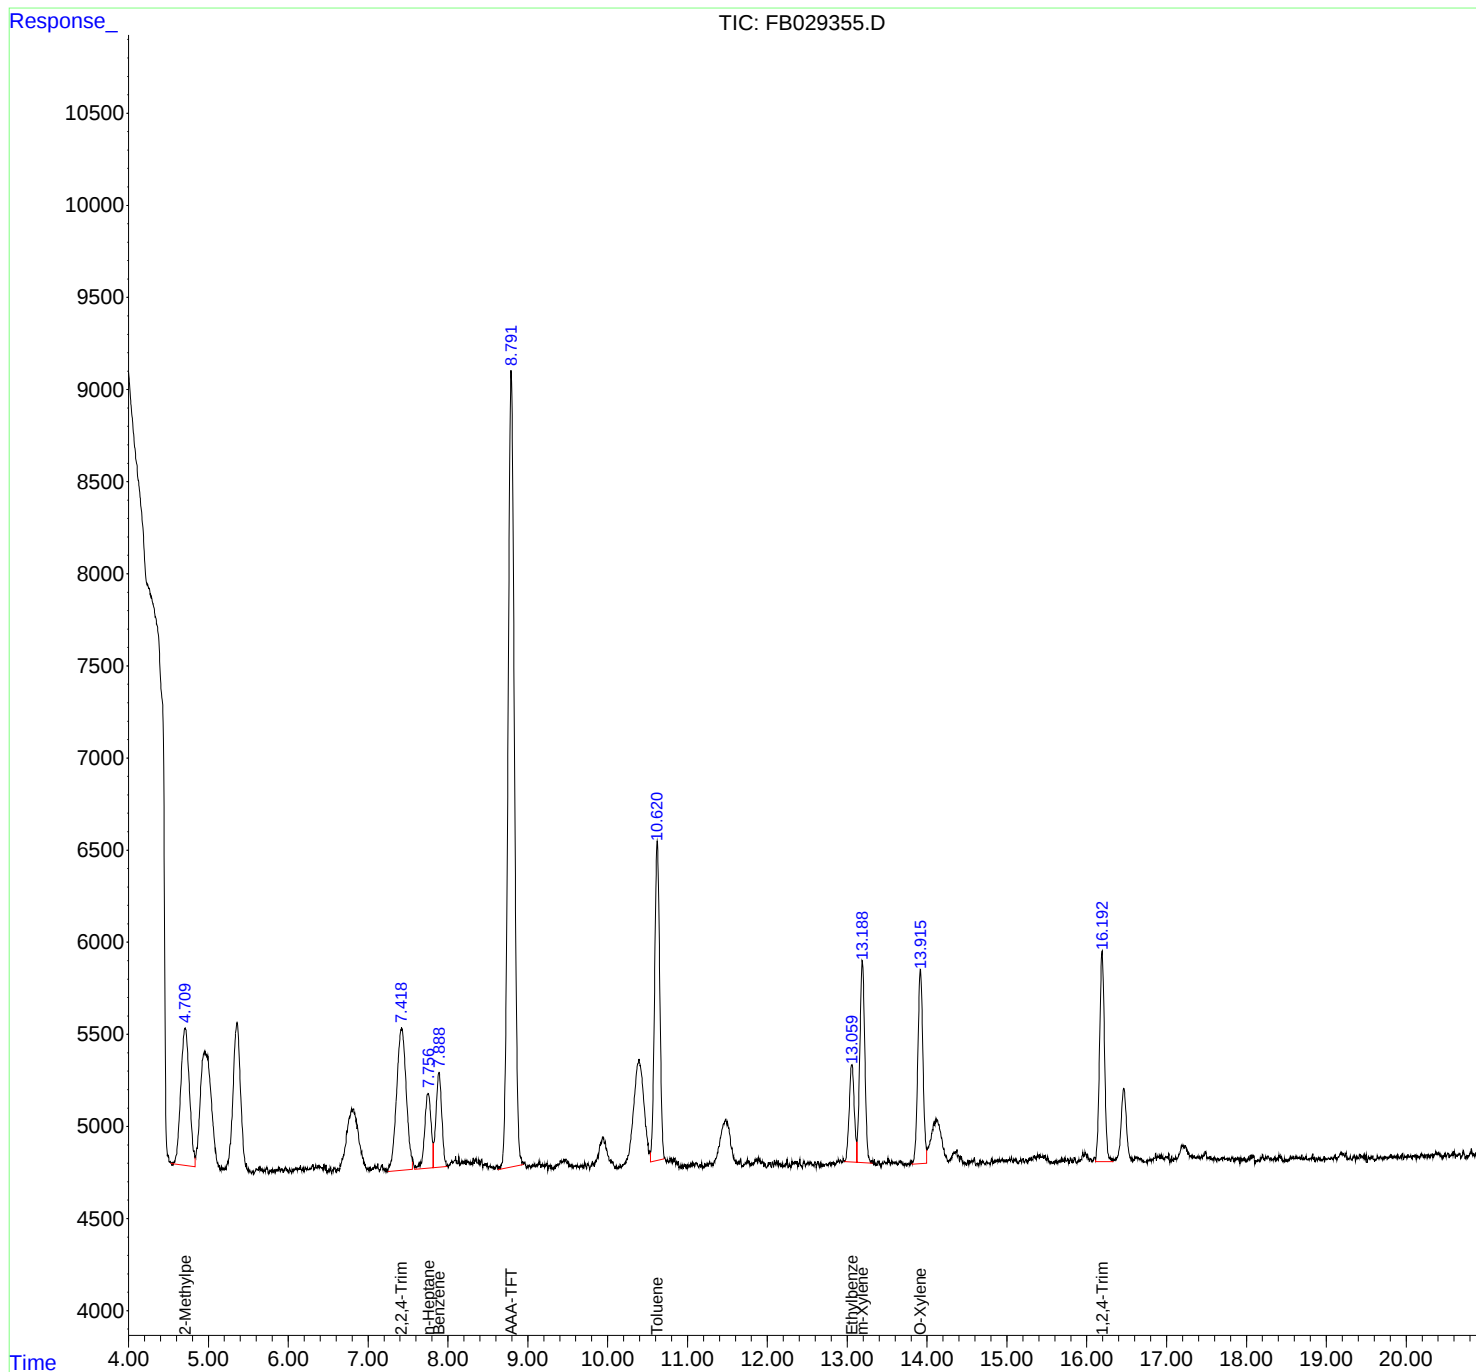

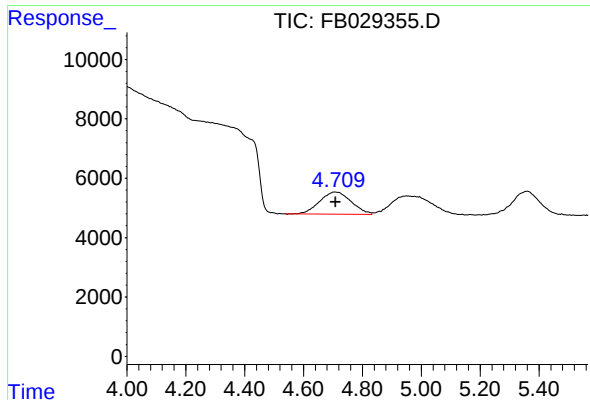


#1 2-Methylpentane

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 55936
Conc: 3.53 ng/ml

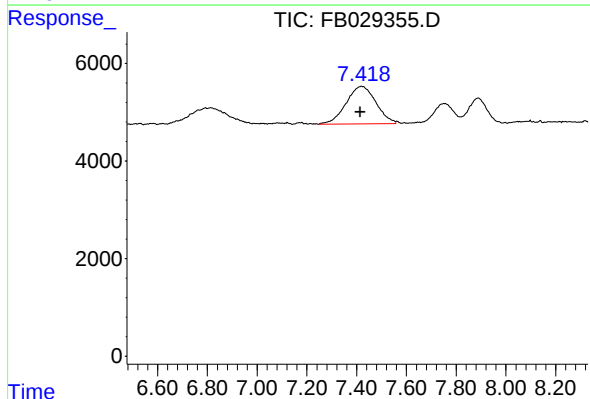


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.005 min
Response: 64588
Conc: 3.75 ng/ml

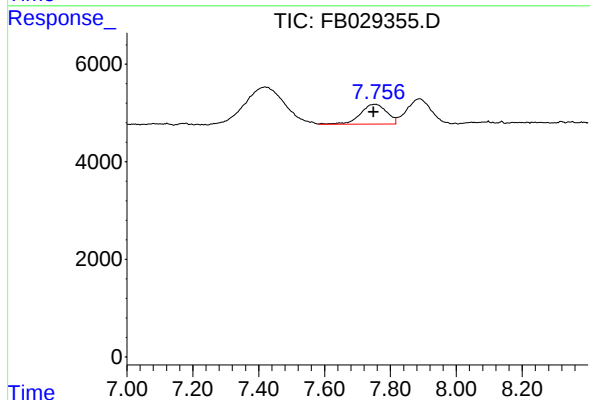


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.008 min
Response: 22641
Conc: 1.25 ng/ml

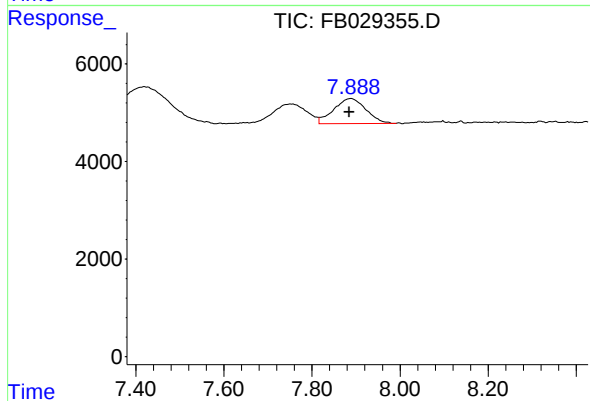


#4 Benzene

R.T.: 7.889 min
Delta R.T.: 0.005 min
Response: 26066
Conc: 1.25 ng/ml

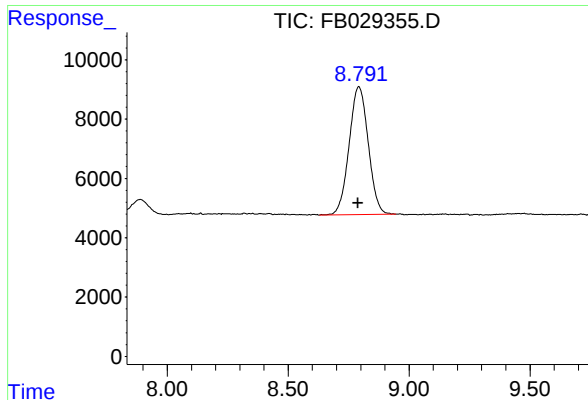


#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: 0.003 min
Response: 237142
Conc: 24.66 ng/ml

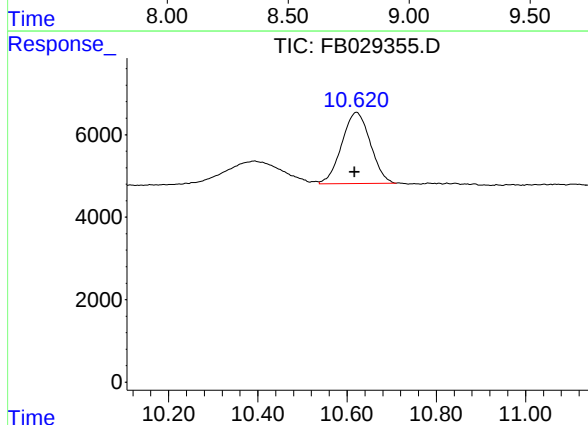


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.005 min
Response: 76878
Conc: 3.79 ng/ml

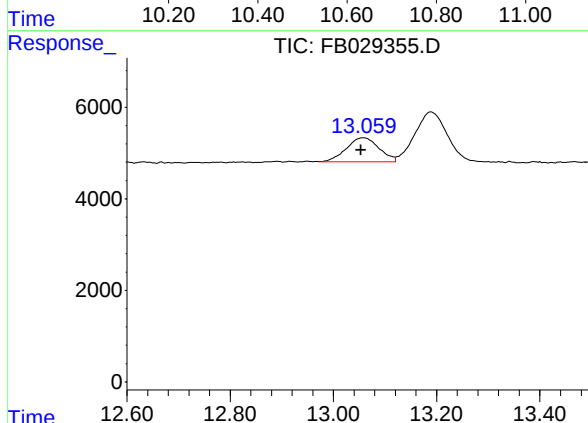


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.006 min
Response: 23338
Conc: 1.22 ng/ml

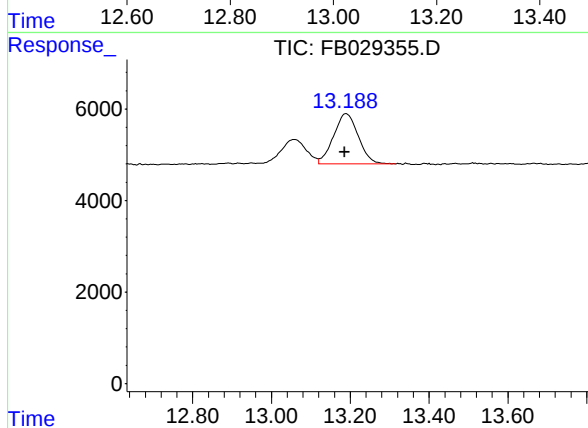


#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: 0.003 min
Response: 47718
Conc: 2.52 ng/ml

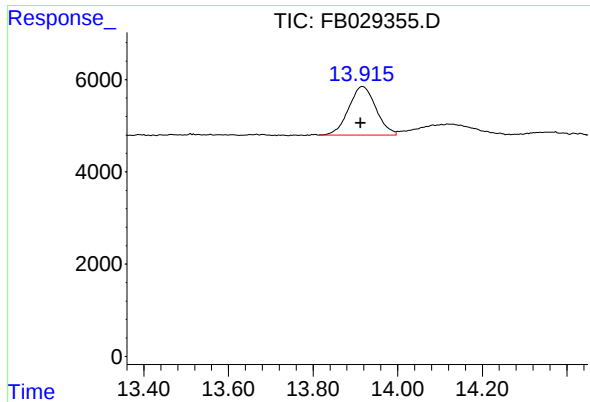

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.005 min
Response: 47027
Conc: 2.58 ng/ml

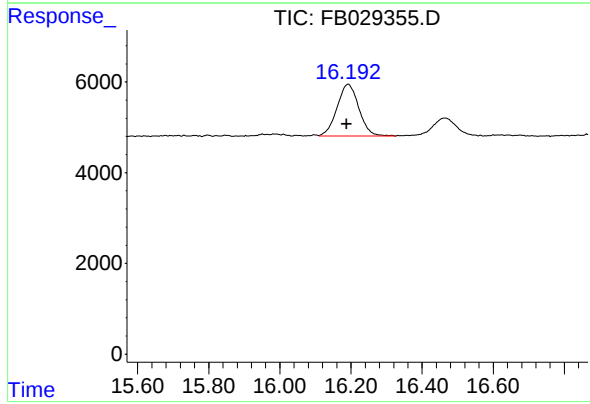

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.005 min
Response: 48423
Conc: 2.57 ng/ml