

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022123\
 Data File : FB029356.D
 Signal(s) : FID2B.CH
 Acq On : 21 Feb 2023 18:22
 Operator : YP/AJ
 Sample : 01627-01
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 22 05:00:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	195957	20.373 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	101260	6.382 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	108932	6.325 ng/ml
3) t n-Heptane	7.755	38238	2.113 ng/ml
4) t Benzene	7.886	44524	2.138 ng/ml
6) t Toluene	10.621	133789	6.602 ng/ml
7) t Ethylbenzene	13.060	40689	2.132 ng/ml
8) t m-Xylene	13.191	80980	4.272 ng/ml
9) t O-Xylene	13.919	80842	4.431 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	85094	4.522 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022123\
Data File : FB029356.D
Signal(s) : FID2B.CH
Acq On : 21 Feb 2023 18:22
Operator : YP/AJ
Sample : 01627-01
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 22 05:00:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

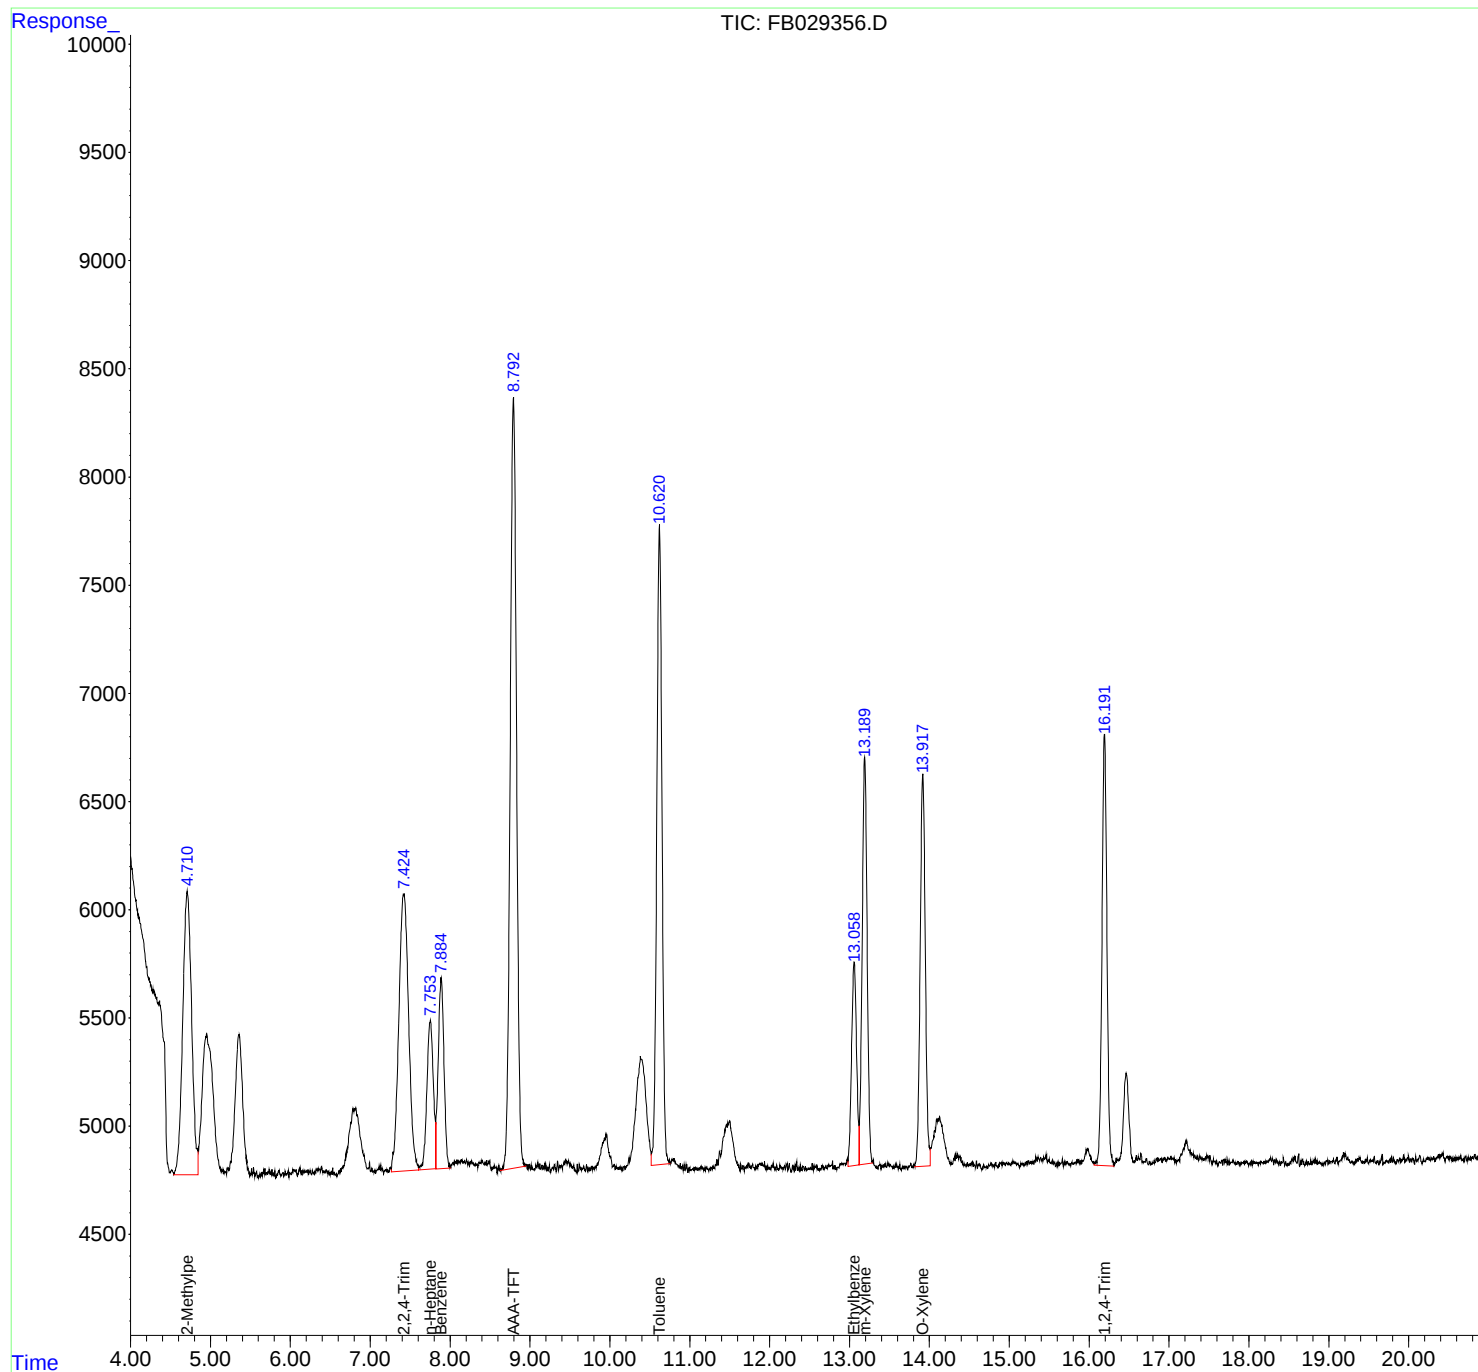

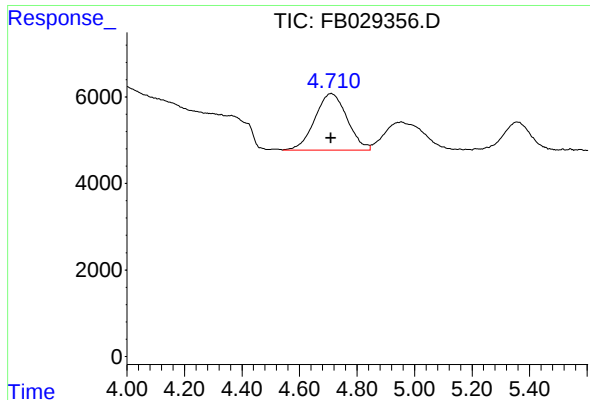


#1 2-Methylpentane

R.T.: 4.711 min
Delta R.T.: 0.002 min
Response: 101260
Conc: 6.38 ng/ml

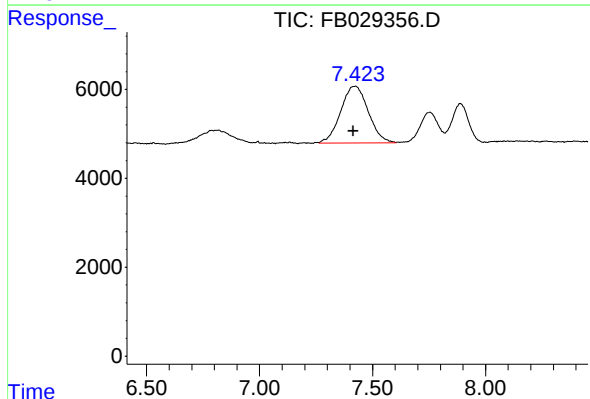


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: 0.011 min
Response: 108932
Conc: 6.32 ng/ml

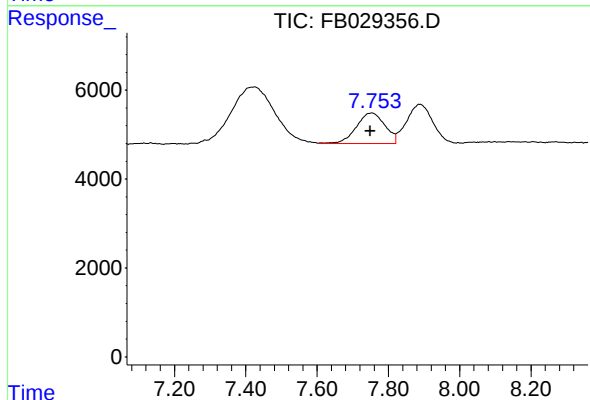


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.006 min
Response: 38238
Conc: 2.11 ng/ml

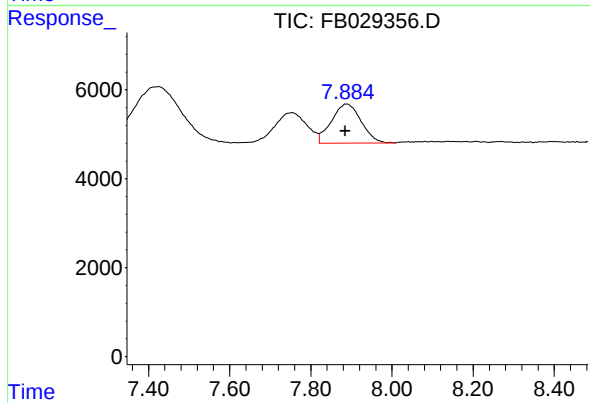


#4 Benzene

R.T.: 7.886 min
Delta R.T.: 0.002 min
Response: 44524
Conc: 2.14 ng/ml

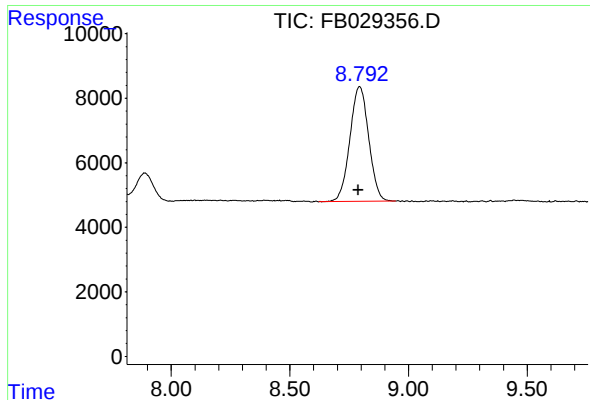


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: 0.005 min
Response: 195957
Conc: 20.37 ng/ml

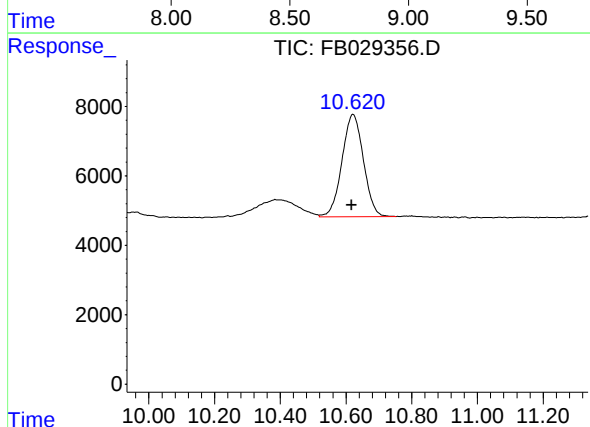


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.004 min
Response: 133789
Conc: 6.60 ng/ml

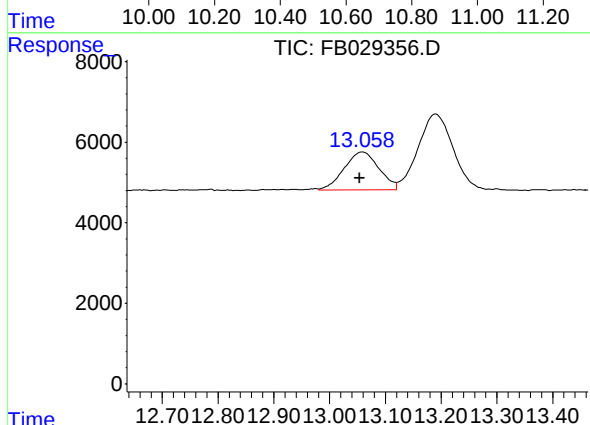


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.006 min
Response: 40689
Conc: 2.13 ng/ml

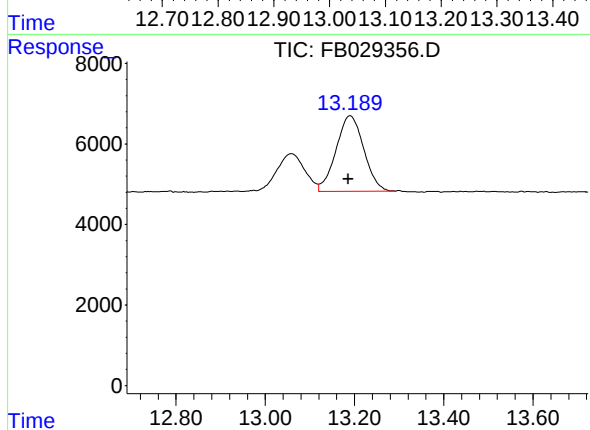


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: 0.005 min
Response: 80980
Conc: 4.27 ng/ml

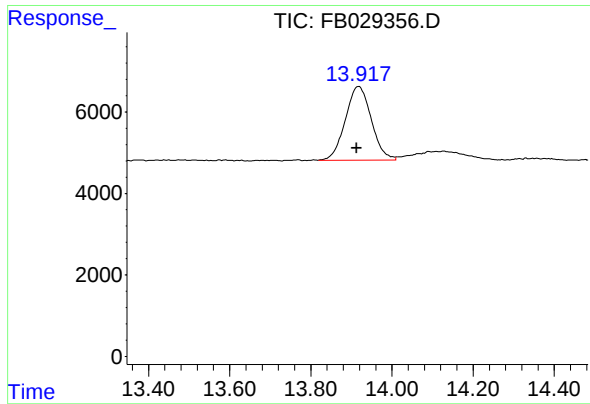

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.006 min
Response: 80842
Conc: 4.43 ng/ml

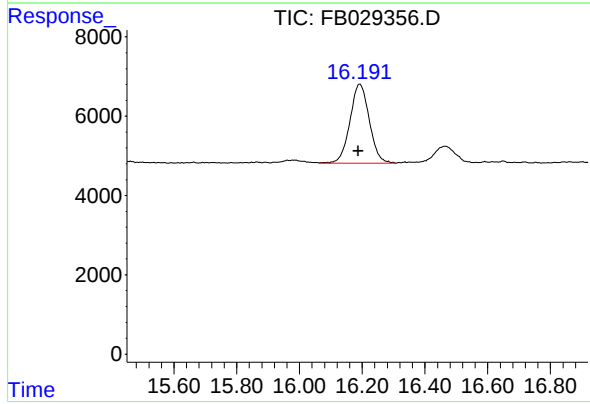

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.005 min
Response: 85094
Conc: 4.52 ng/ml