

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022219\
 Data File : FB019872.D
 Signal(s) : FID2B.CH
 Acq On : 22 Feb 2019 9:51
 Operator : MJ/SJ
 Sample : BSF0222S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 22 22:45:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
 Quant Title :
 QLast Update : Tue Jan 29 12:07:12 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.038	203013	17.367 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.894	575424	33.236 ng/ml
2) t	2,2,4-Trimethylpentane	7.653	563808	33.998 ng/ml
3) t	n-Heptane	7.993	179115	11.115 ng/ml
4) t	Benzene	8.130	196290	10.407 ng/ml
6) t	Toluene	10.884	524305	29.973 ng/ml
7) t	Ethylbenzene	13.336	209756	9.558 ng/ml
8) t	m-Xylene	13.469	435542	19.030 ng/ml
9) t	O-Xylene	14.201	420282	18.817 ng/ml
10) t	1,2,4-Trimethylbenzene	16.487	434097	18.735 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022219\
Data File : FB019872.D
Signal(s) : FID2B.CH
Acq On : 22 Feb 2019 9:51
Operator : MJ/SJ
Sample : BSF0222S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 22 22:45:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB012919.M
Quant Title :
QLast Update : Tue Jan 29 12:07:12 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

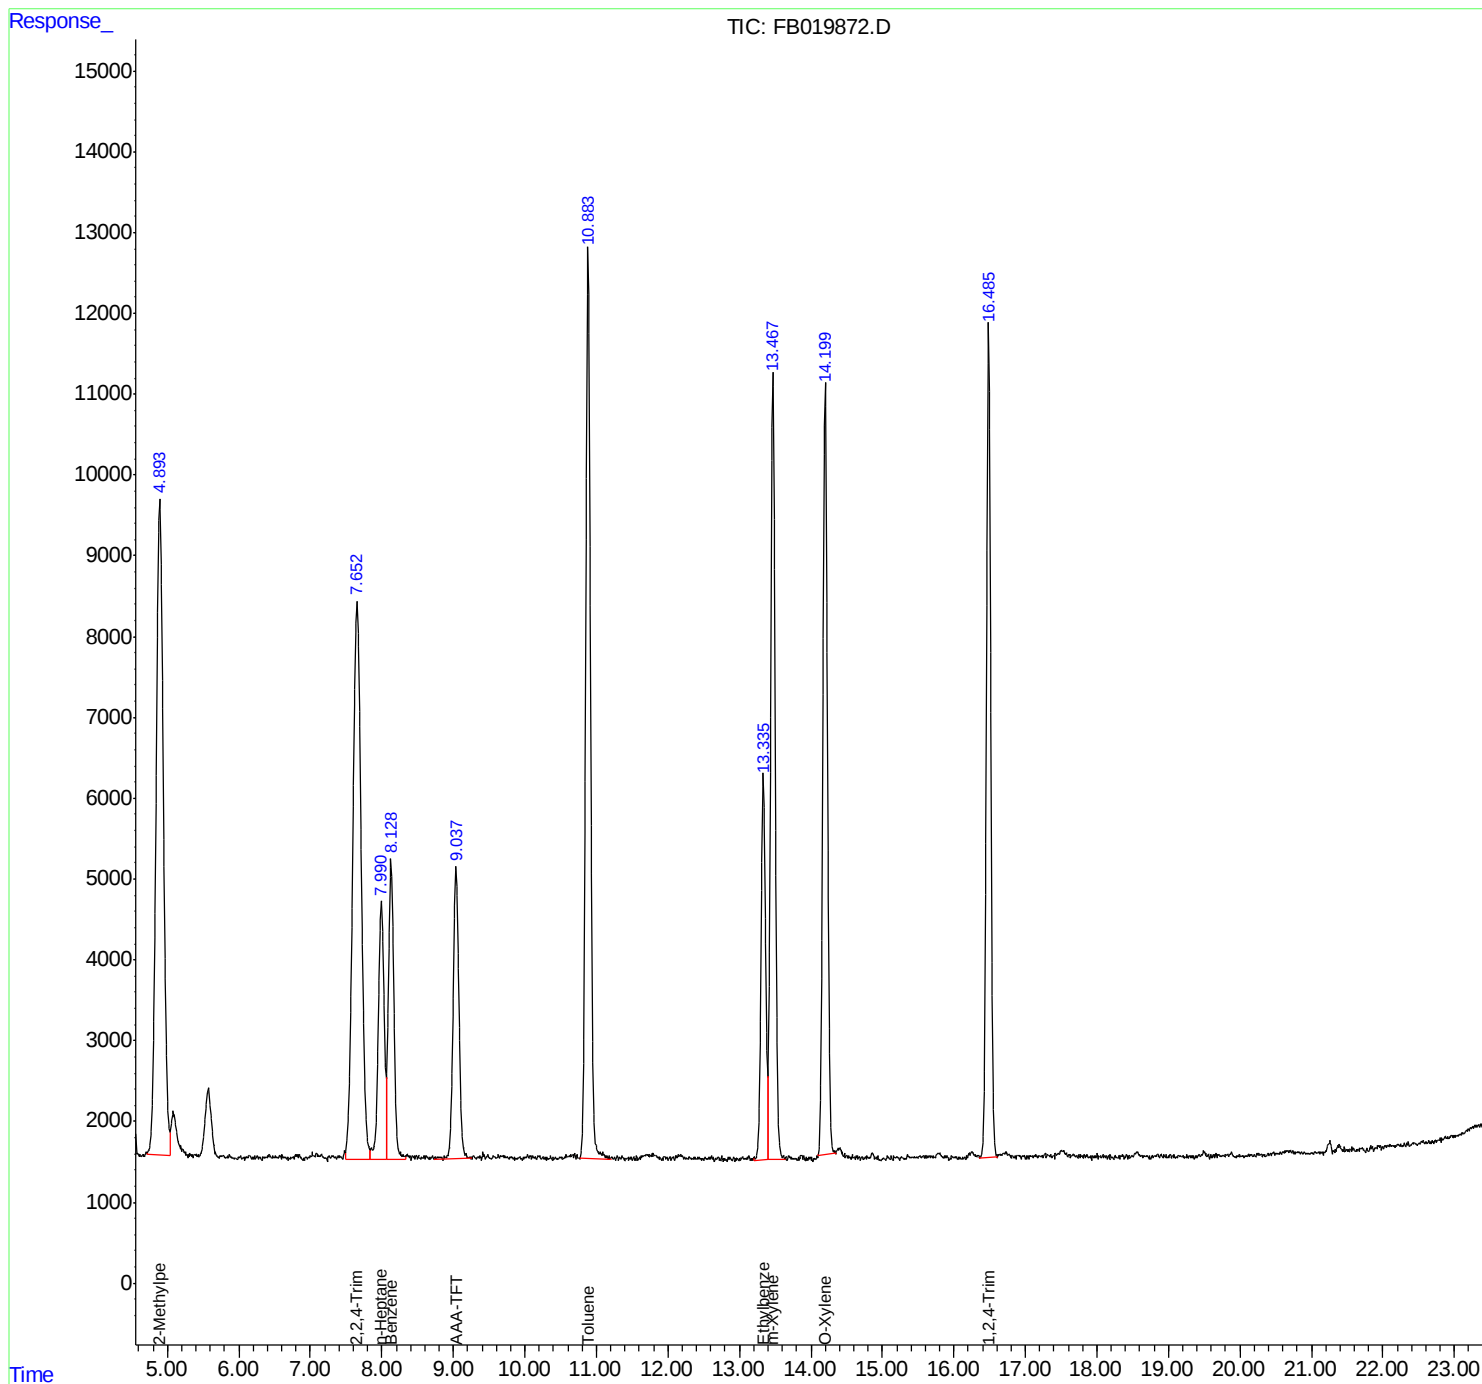

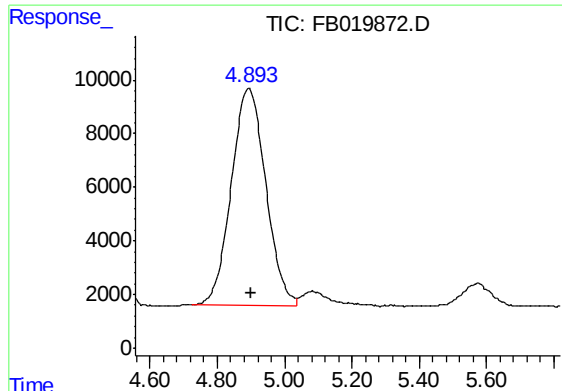


#1 2-Methylpentane

R.T.: 4.894 min
Delta R.T.: -0.008 min
Response: 575424
Conc: 33.24 ng/ml

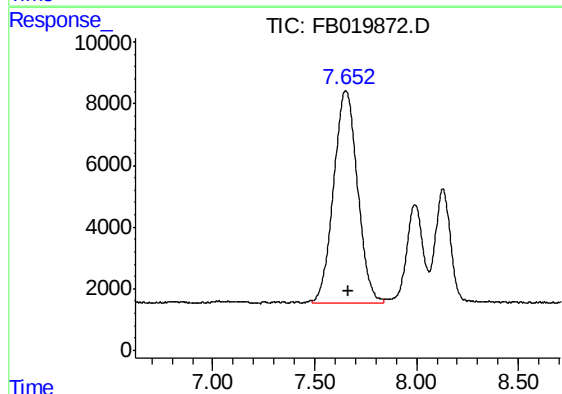


#2 2,2,4-Trimethylpentane

R.T.: 7.653 min
Delta R.T.: -0.011 min
Response: 563808
Conc: 34.00 ng/ml

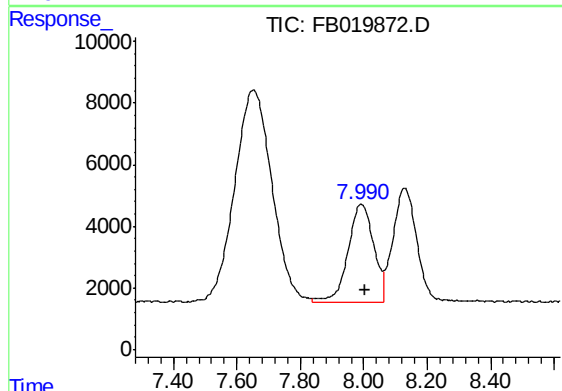


#3 n-Heptane

R.T.: 7.993 min
Delta R.T.: -0.012 min
Response: 179115
Conc: 11.11 ng/ml

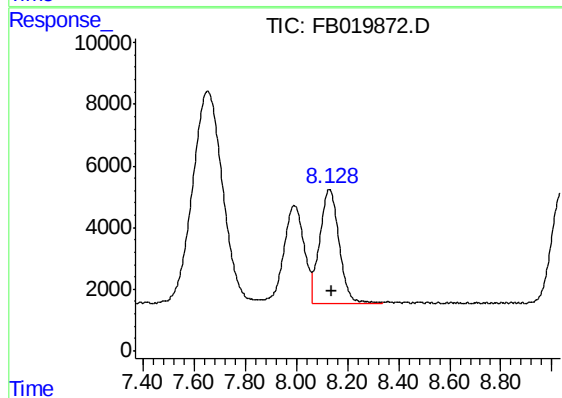


#4 Benzene

R.T.: 8.130 min
Delta R.T.: -0.011 min
Response: 196290
Conc: 10.41 ng/ml

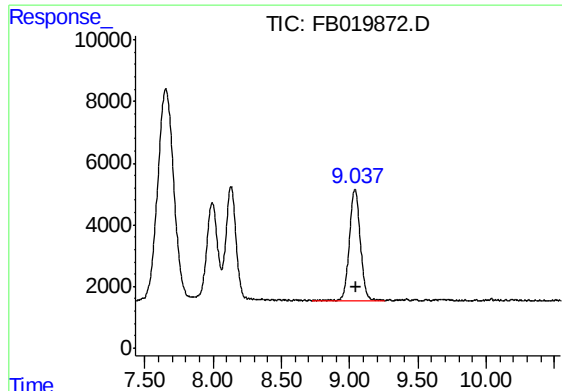


#5 AAA-TFT

R.T.: 9.038 min
Delta R.T.: -0.012 min
Response: 203013
Conc: 17.37 ng/ml

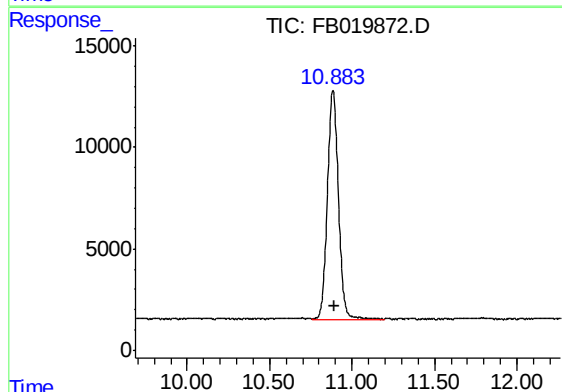


#6 Toluene

R.T.: 10.884 min
Delta R.T.: -0.012 min
Response: 524305
Conc: 29.97 ng/ml

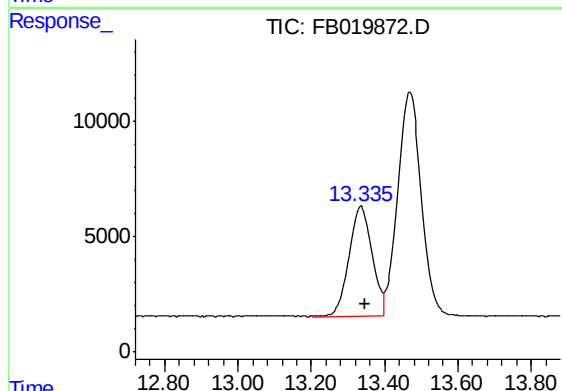


#7 Ethylbenzene

R.T.: 13.336 min
Delta R.T.: -0.013 min
Response: 209756
Conc: 9.56 ng/ml

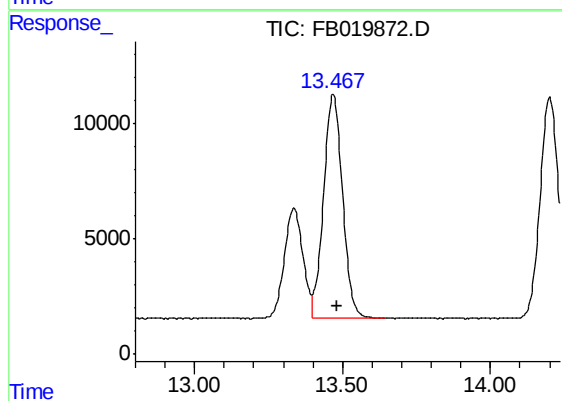


#8 m-Xylene

R.T.: 13.469 min
Delta R.T.: -0.013 min
Response: 435542
Conc: 19.03 ng/ml

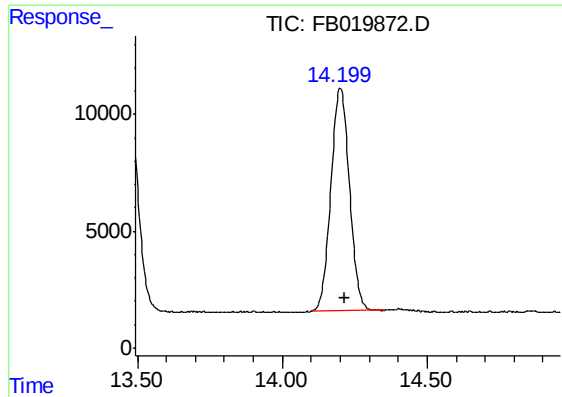

#9 O-Xylene

R.T.: 14.201 min
Delta R.T.: -0.013 min
Response: 420282
Conc: 18.82 ng/ml

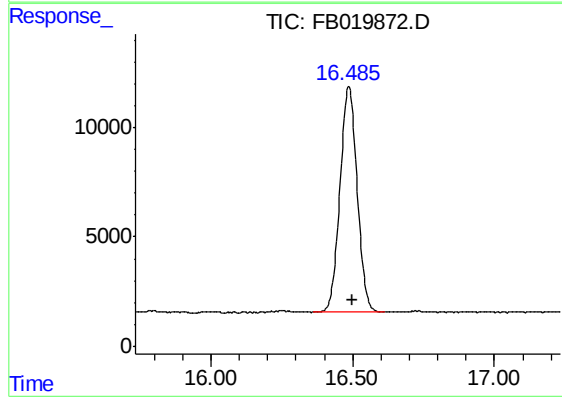

#10 1,2,4-Trimethylbenzene

R.T.: 16.487 min
Delta R.T.: -0.013 min
Response: 434097
Conc: 18.74 ng/ml