

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022221\
 Data File : FB025442.D
 Signal(s) : FID2B.CH
 Acq On : 22 Feb 2021 16:02
 Operator : DD/AJ
 Sample : M1431-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Feb 23 03:02:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
 Quant Title :
 QLast Update : Mon Feb 22 11:51:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.805	475847	18.760 ng/ml
Target Compounds			
4) t Benzene	7.901	38725	0.838 ng/ml
6) t Toluene	10.637	3150631	70.469 ng/ml
7) t Ethylbenzene	13.084	20962	0.519 ng/ml
8) t m-Xylene	13.209	47097	1.171 ng/ml
9) t O-Xylene	13.929	36085	0.932 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022221\
Data File : FB025442.D
Signal(s) : FID2B.CH
Acq On : 22 Feb 2021 16:02
Operator : DD/AJ
Sample : M1431-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Feb 23 03:02:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

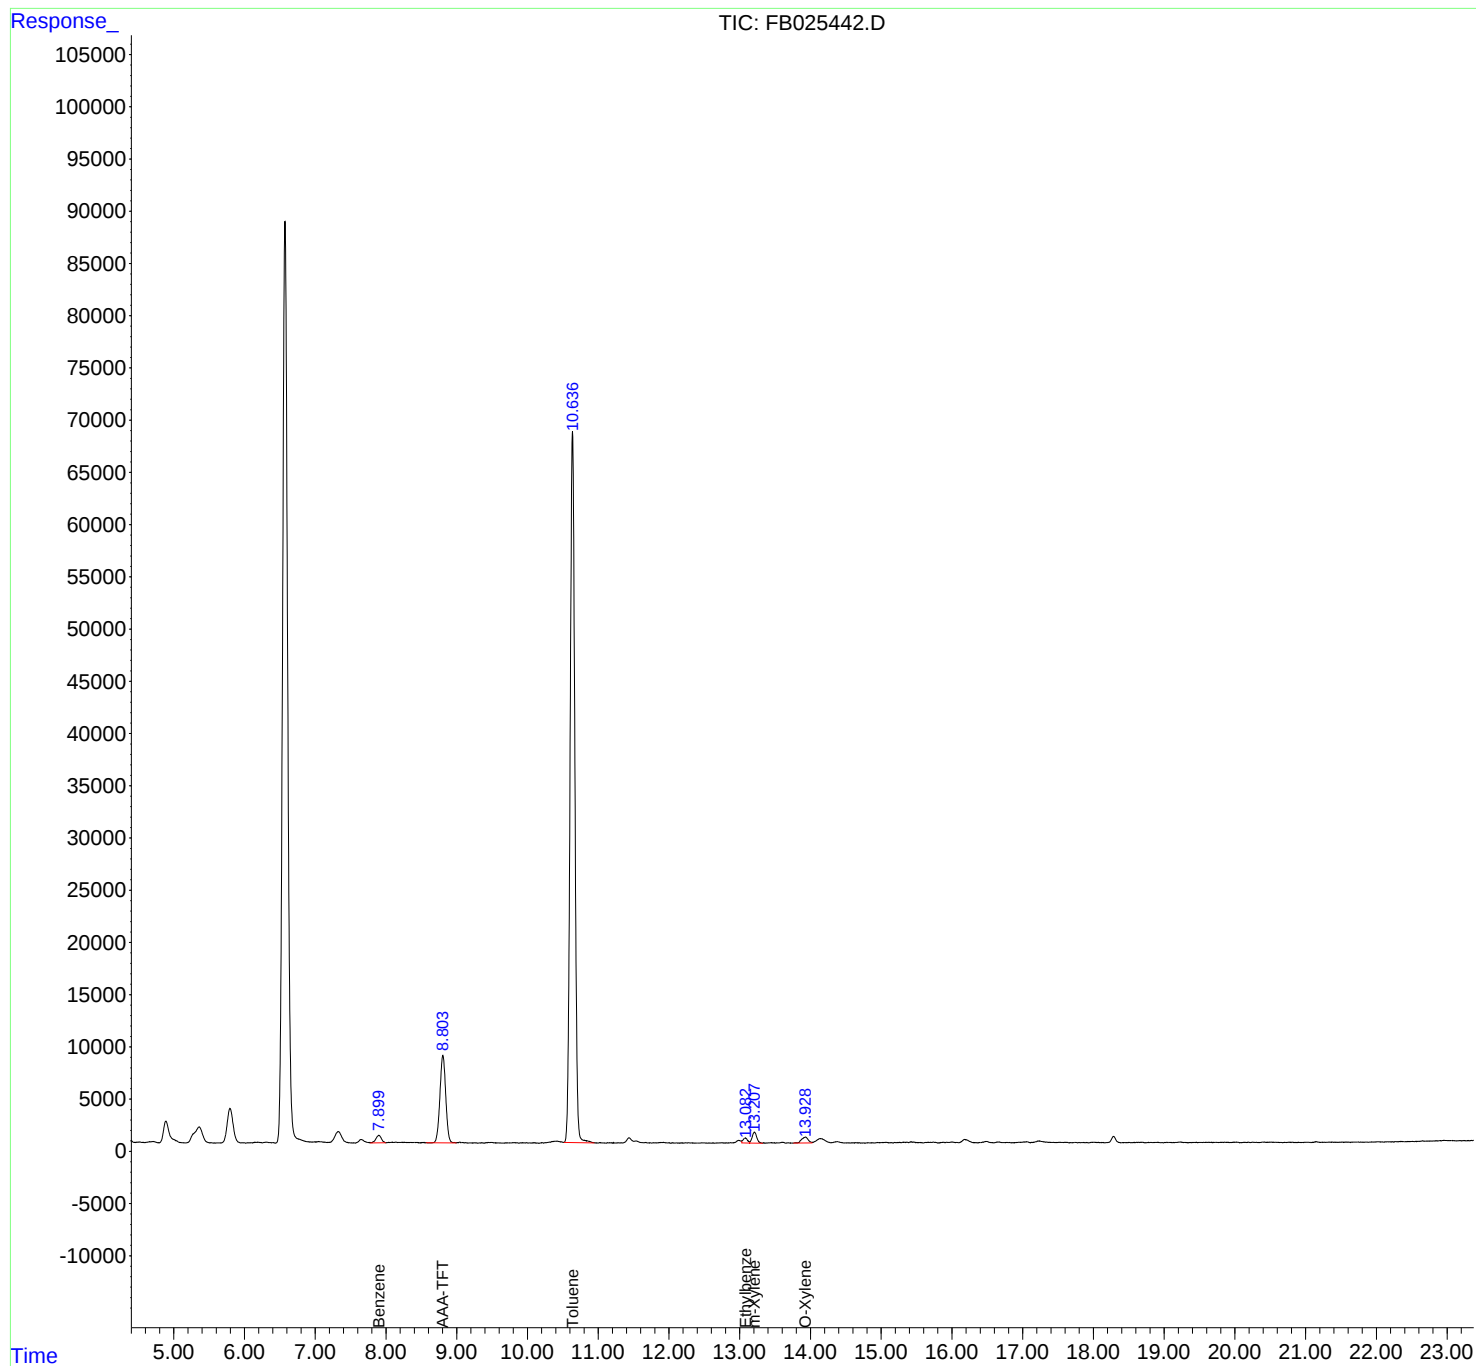


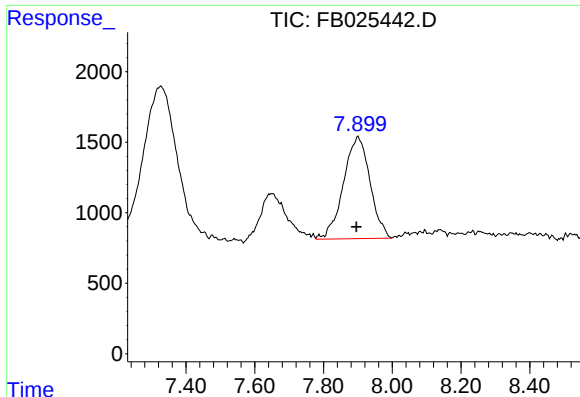

#4 Benzene


R.T.: 7.901 min
Delta R.T.: 0.005 min
Response: 38725
Conc: 0.84 ng/ml

Instrument :
FID_B
ClientSampleId :

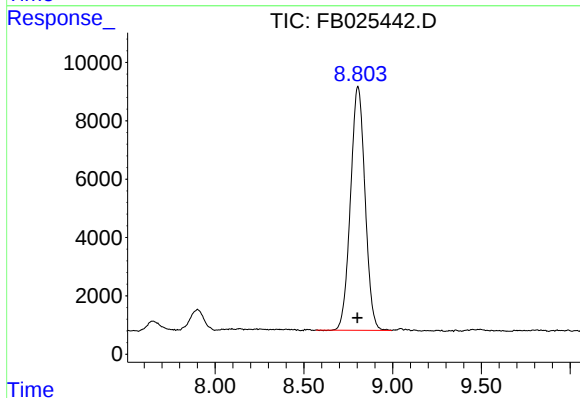


#5 AAA-TFT

R.T.: 8.805 min
Delta R.T.: 0.003 min
Response: 475847
Conc: 18.76 ng/ml

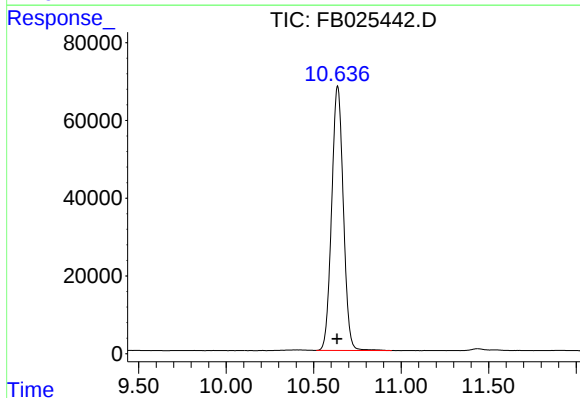


#6 Toluene

R.T.: 10.637 min
Delta R.T.: 0.004 min
Response: 3150631
Conc: 70.47 ng/ml

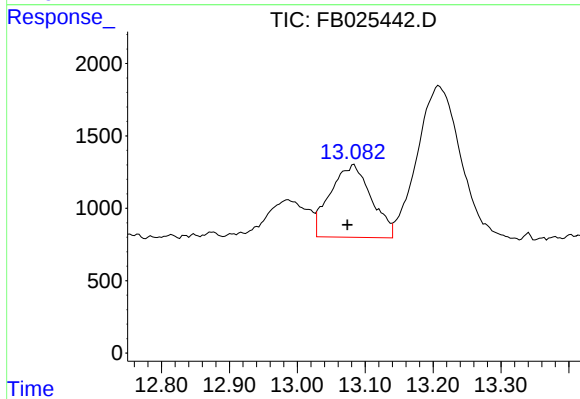

#7 Ethylbenzene


R.T.: 13.084 min
Delta R.T.: 0.010 min
Response: 20962
Conc: 0.52 ng/ml

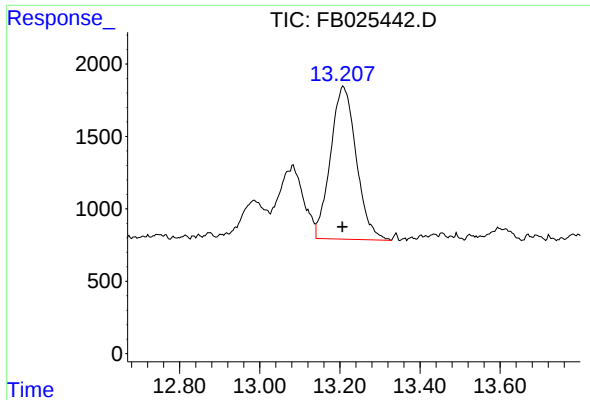

#8 m-Xylene

R.T.: 13.209 min
Delta R.T.: 0.002 min
Response: 47097
Conc: 1.17 ng/ml

Instrument :
FID_B
ClientSampleId :

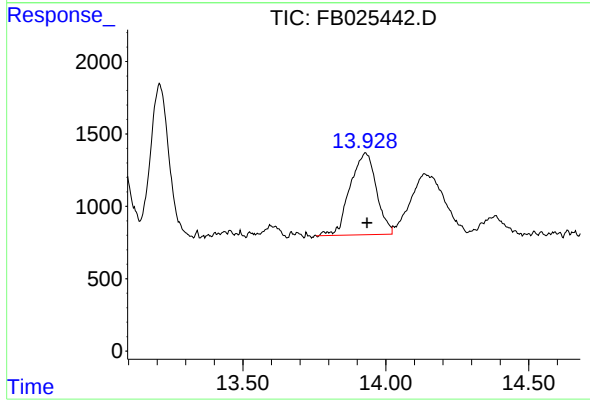

#9 o-Xylene

R.T.: 13.929 min
Delta R.T.: -0.005 min
Response: 36085
Conc: 0.93 ng/ml