

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022221\
 Data File : FB025435.D
 Signal(s) : FID2B.CH
 Acq On : 22 Feb 2021 10:33
 Operator : DD/AJ
 Sample : BSF0222S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0222S1

Integration File: Calibration.e
 Quant Time: Feb 23 03:01:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
 Quant Title :
 QLast Update : Mon Feb 22 11:51:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	495555	19.537 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	1050752	29.813 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	1152513	31.038 ng/ml
3) t n-Heptane	7.758	374523	10.346 ng/ml
4) t Benzene	7.893	452373	9.792 ng/ml
6) t Toluene	10.631	1312309	29.352 ng/ml
7) t Ethylbenzene	13.072	405492	10.047 ng/ml
8) t m-Xylene	13.205	807694	20.078 ng/ml
9) t O-Xylene	13.932	781531	20.190 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	671801	20.013 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022221\
Data File : FB025435.D
Signal(s) : FID2B.CH
Acq On : 22 Feb 2021 10:33
Operator : DD/AJ
Sample : BSF0222S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0222S1

Integration File: Calibration.e
Quant Time: Feb 23 03:01:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

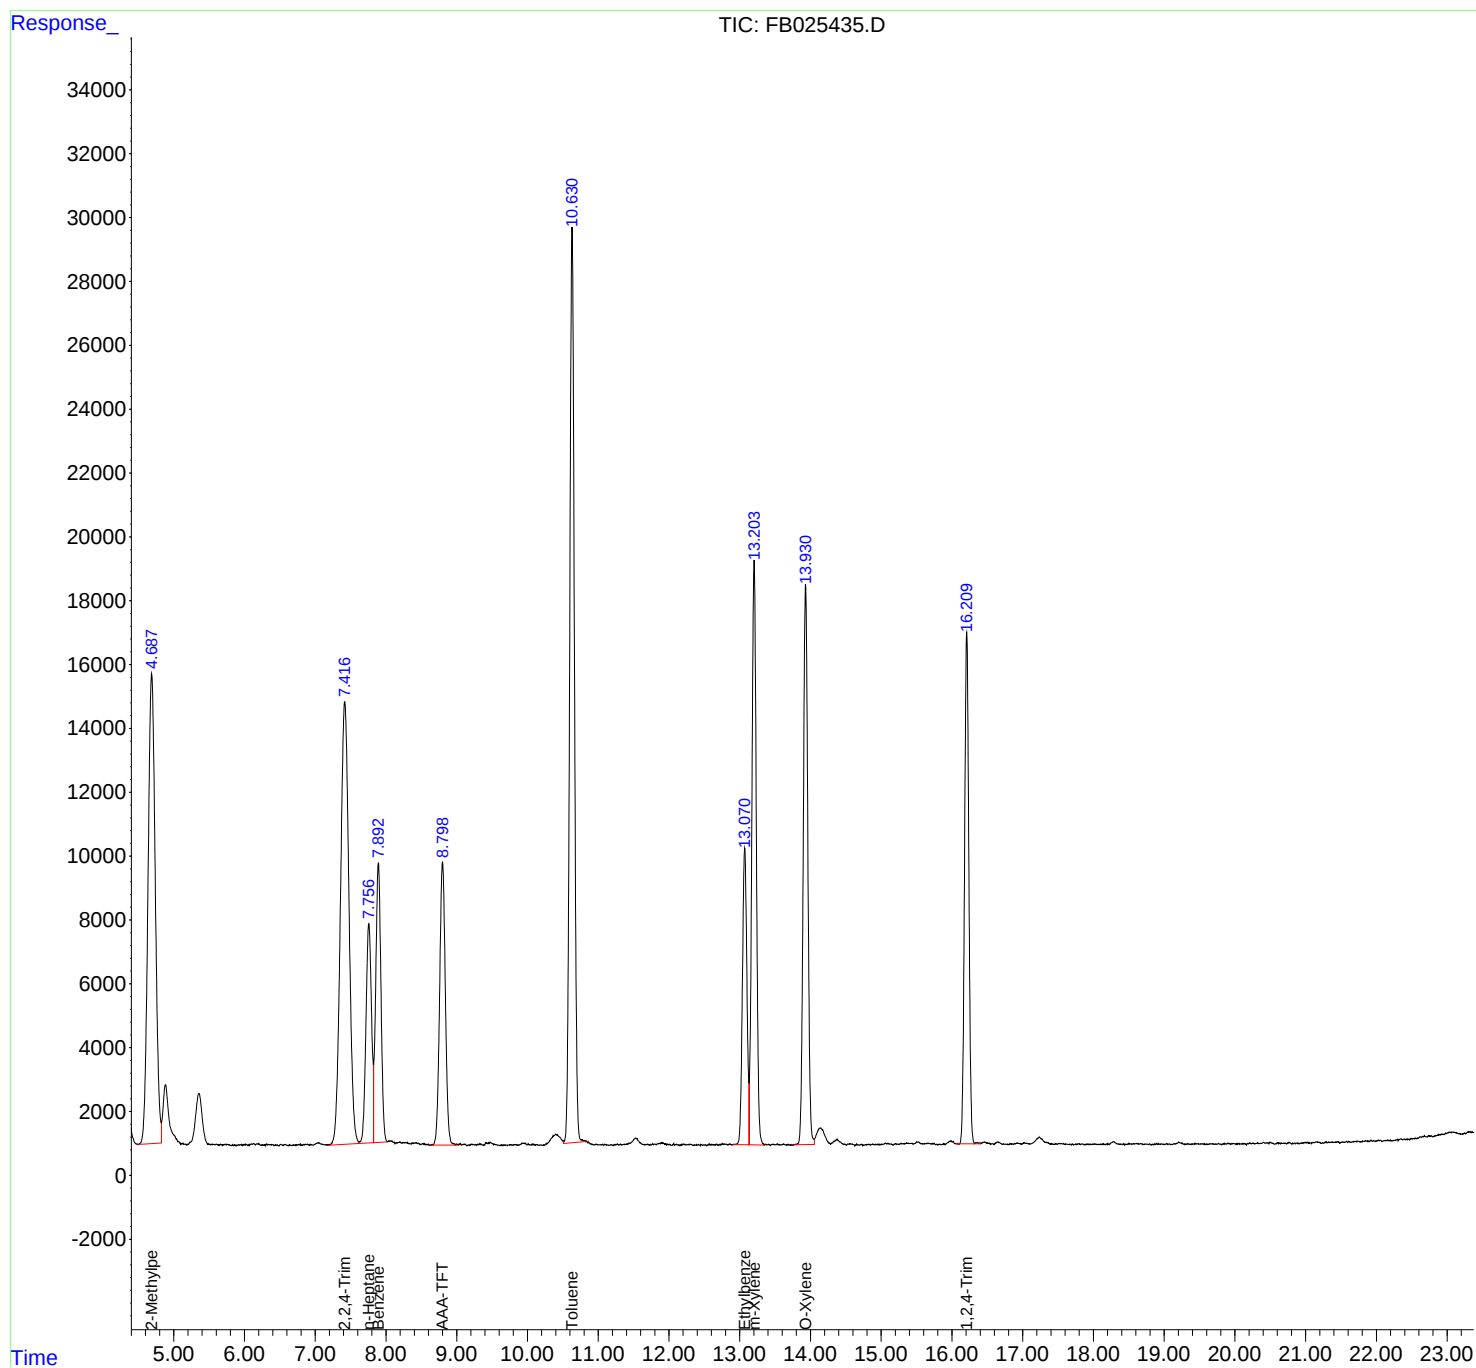


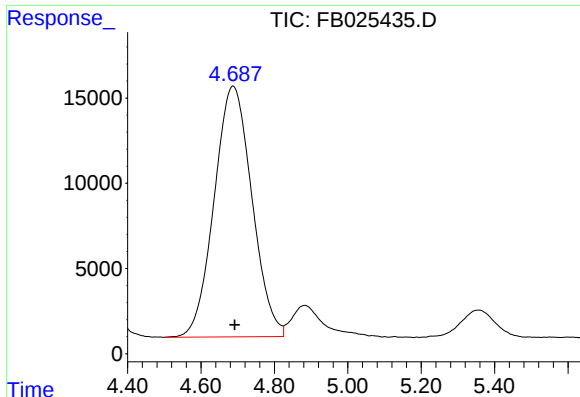

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: -0.004 min
Response: 1050752
Conc: 29.81 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0222S1

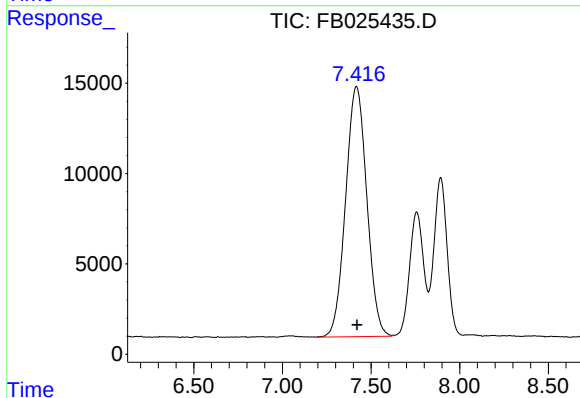


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.004 min
Response: 1152513
Conc: 31.04 ng/ml

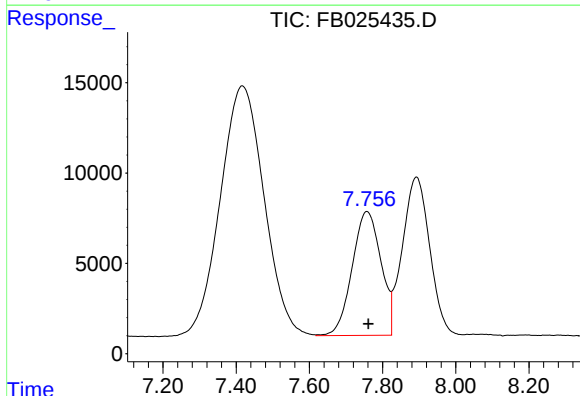


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: -0.003 min
Response: 374523
Conc: 10.35 ng/ml

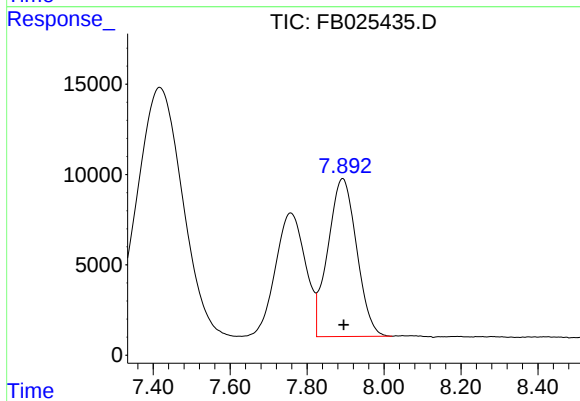

#4 Benzene


R.T.: 7.893 min
Delta R.T.: -0.002 min
Response: 452373
Conc: 9.79 ng/ml

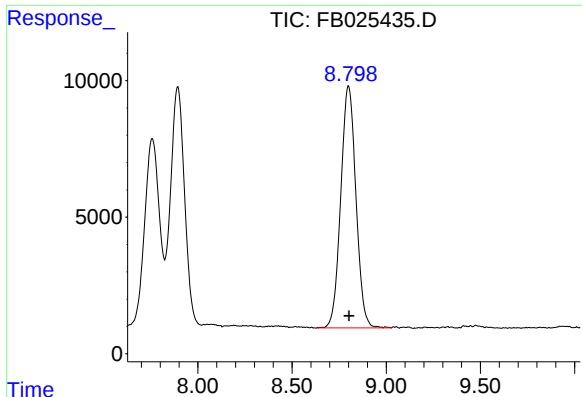

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: -0.002 min
Response: 495555
Conc: 19.54 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0222S1

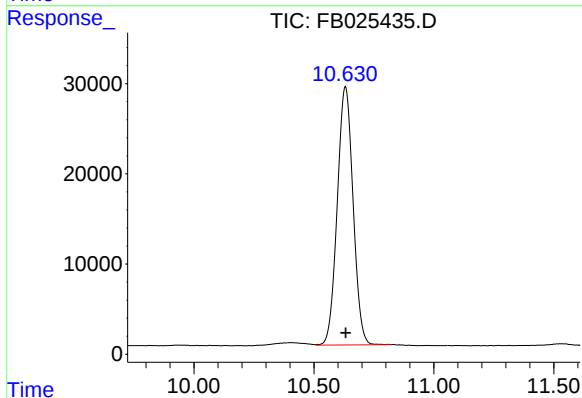


#6 Toluene

R.T.: 10.631 min
Delta R.T.: -0.002 min
Response: 1312309
Conc: 29.35 ng/ml

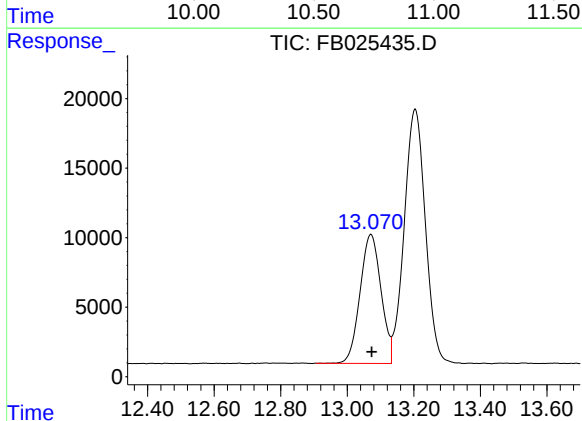


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: -0.002 min
Response: 405492
Conc: 10.05 ng/ml

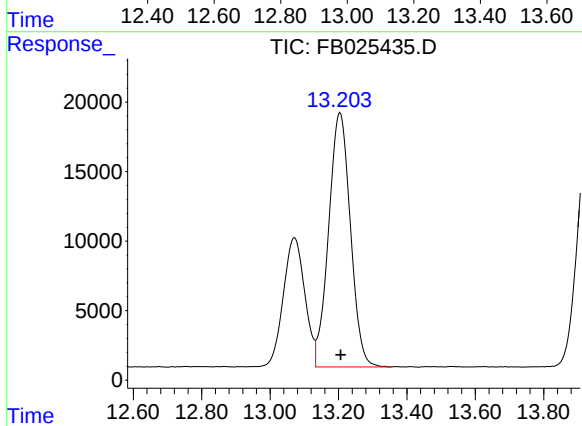

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: -0.002 min
Response: 807694
Conc: 20.08 ng/ml

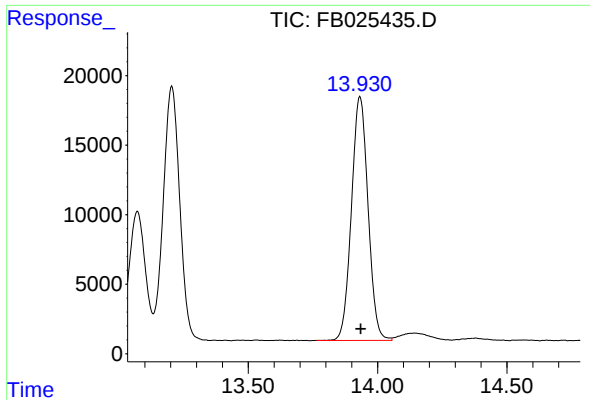

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: -0.002 min
Response: 781531
Conc: 20.19 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0222S1

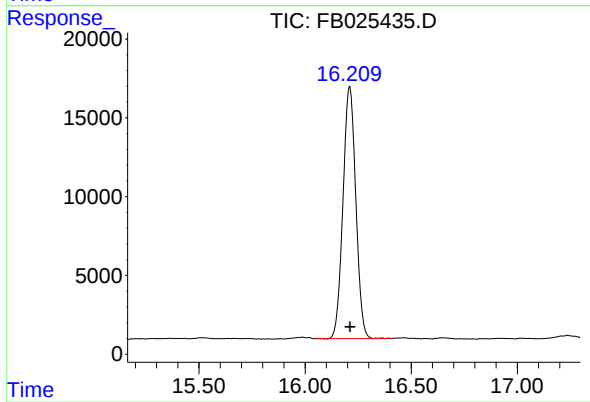

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: -0.002 min
Response: 671801
Conc: 20.01 ng/ml