

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022221\
 Data File : FB025437.D
 Signal(s) : FID2B.CH
 Acq On : 22 Feb 2021 13:30
 Operator : DD/AJ
 Sample : M1422-01MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BU-03-021621MS

Integration File: Calibration.e
 Quant Time: Feb 23 03:01:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
 Quant Title :
 QLast Update : Mon Feb 22 11:51:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.803	479417	18.901 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	950672	26.973 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	1005581	27.081 ng/ml
3) t n-Heptane	7.761	329163	9.093 ng/ml
4) t Benzene	7.896	429242	9.292 ng/ml
6) t Toluene	10.634	1220902	27.308 ng/ml
7) t Ethylbenzene	13.075	372446	9.228 ng/ml
8) t m-Xylene	13.207	745461	18.531 ng/ml
9) t O-Xylene	13.935	714628	18.462 ng/ml
10) t 1,2,4-Trimethylbenzene	16.213	610492	18.187 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022221\
Data File : FB025437.D
Signal(s) : FID2B.CH
Acq On : 22 Feb 2021 13:30
Operator : DD/AJ
Sample : M1422-01MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BU-03-021621MS

Integration File: Calibration.e
Quant Time: Feb 23 03:01:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

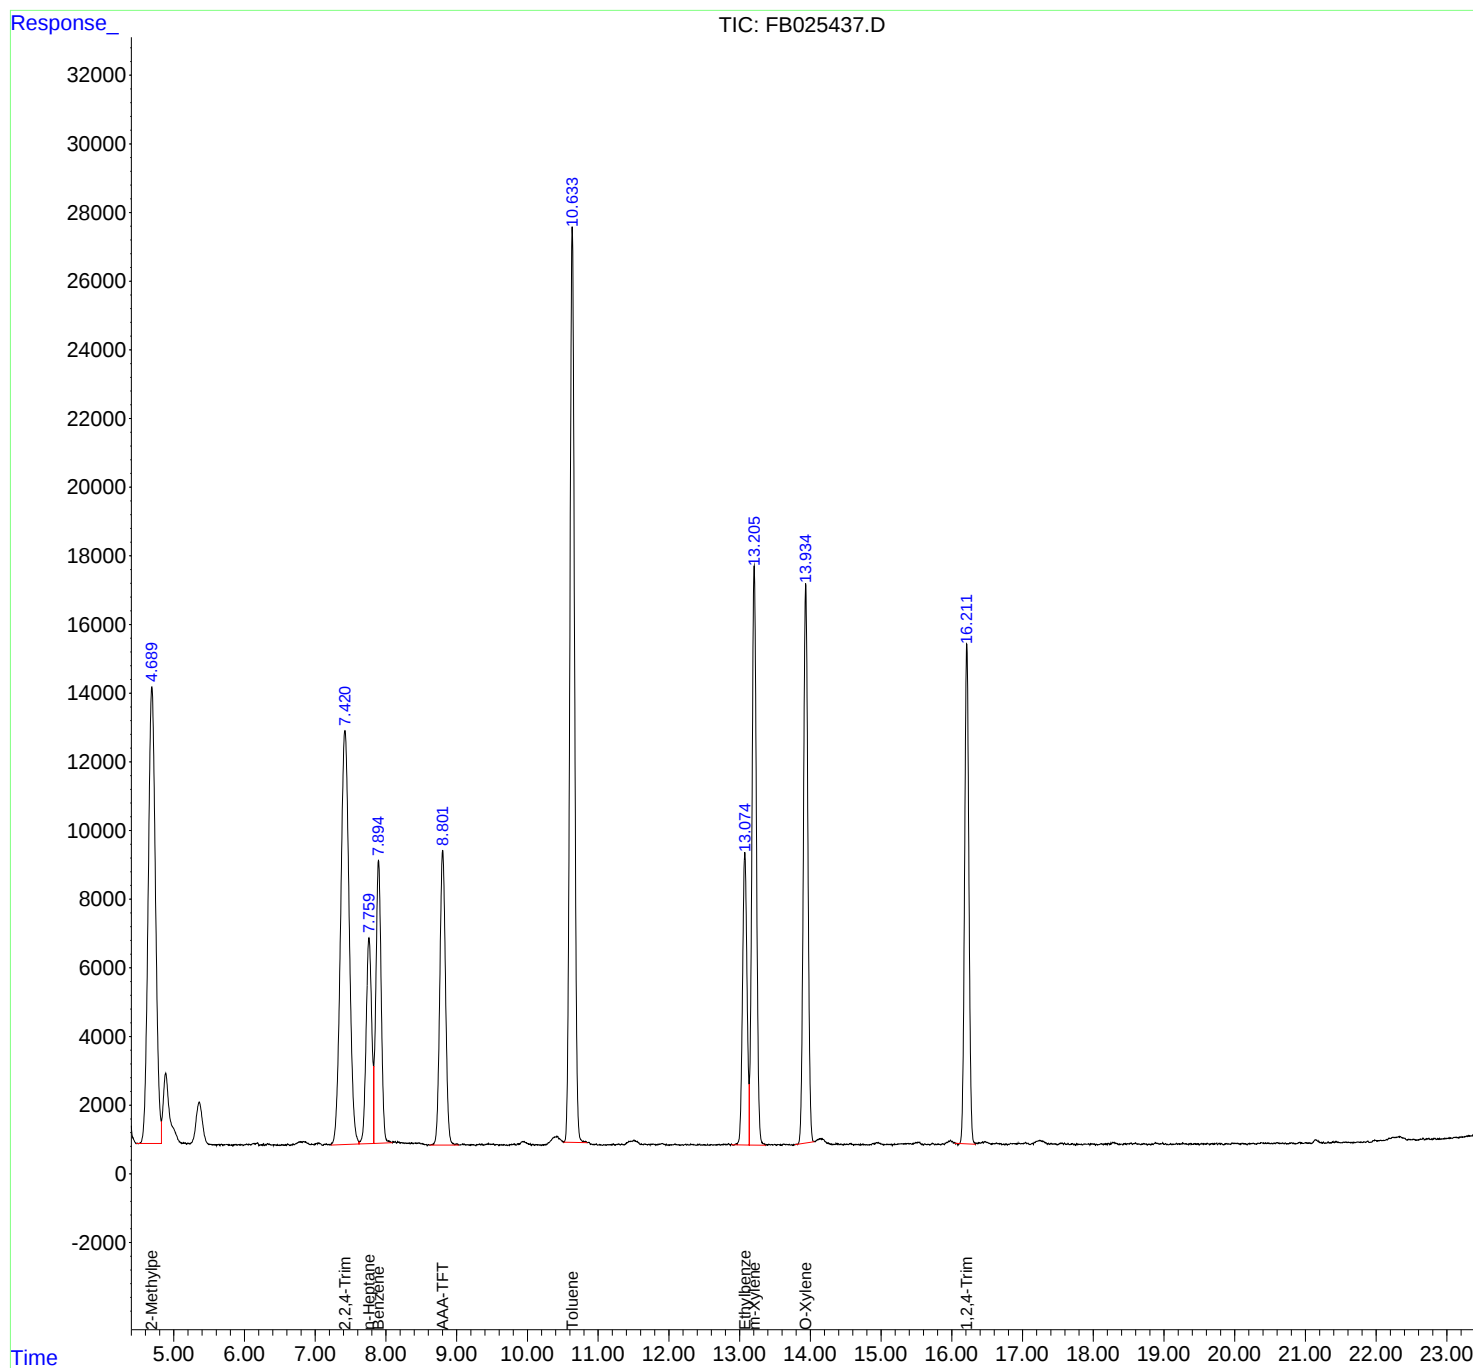


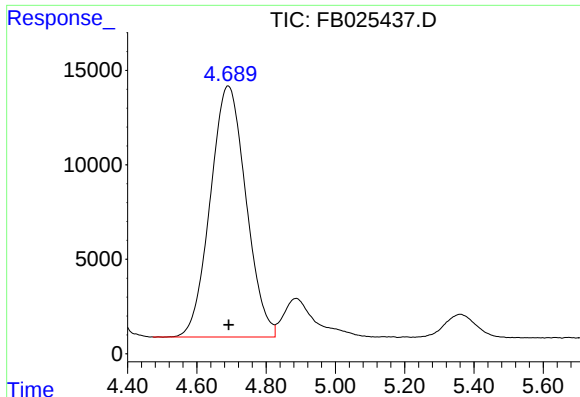

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: -0.001 min
Response: 950672
Conc: 26.97 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-021621MS

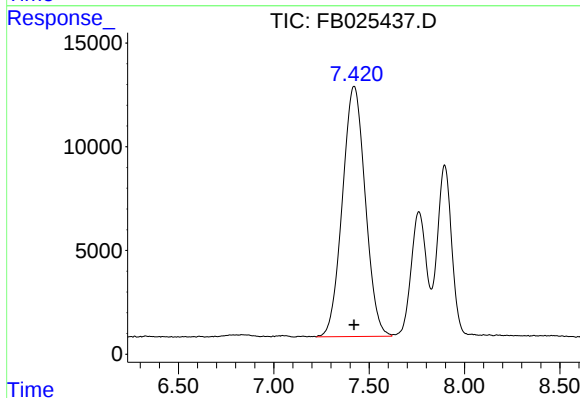


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: 0.000 min
Response: 1005581
Conc: 27.08 ng/ml

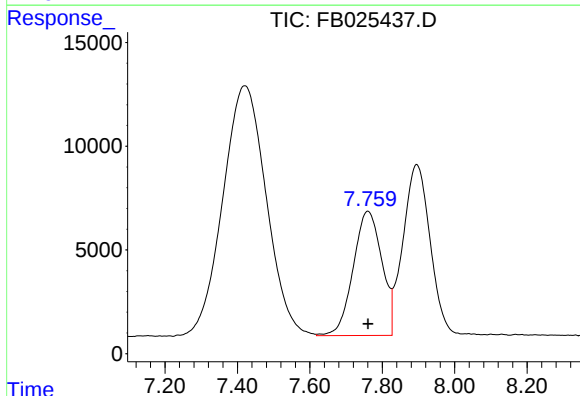


#3 n-Heptane

R.T.: 7.761 min
Delta R.T.: 0.000 min
Response: 329163
Conc: 9.09 ng/ml

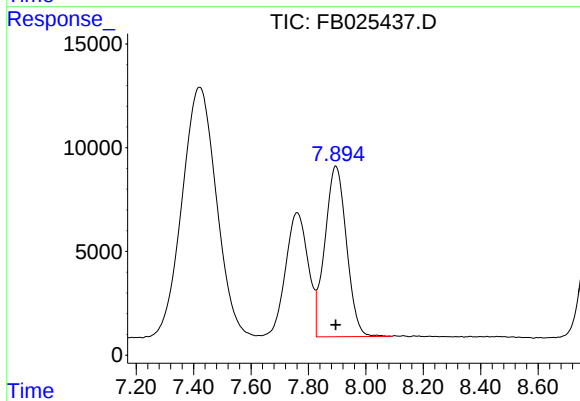

#4 Benzene


R.T.: 7.896 min
Delta R.T.: 0.000 min
Response: 429242
Conc: 9.29 ng/ml

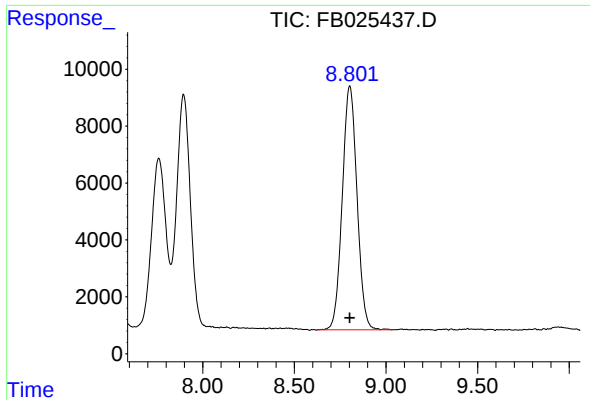

#5 AAA-TFT


R.T.: 8.803 min
Delta R.T.: 0.000 min
Response: 479417
Conc: 18.90 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-021621MS

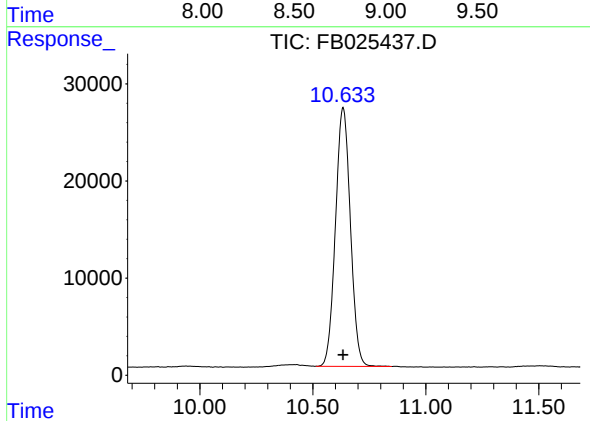


#6 Toluene

R.T.: 10.634 min
Delta R.T.: 0.000 min
Response: 1220902
Conc: 27.31 ng/ml

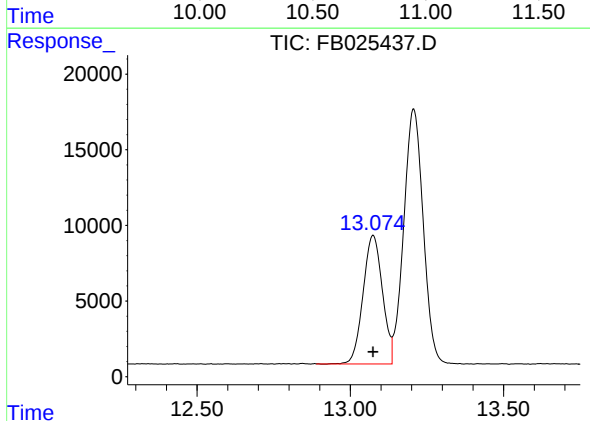


#7 Ethylbenzene

R.T.: 13.075 min
Delta R.T.: 0.000 min
Response: 372446
Conc: 9.23 ng/ml

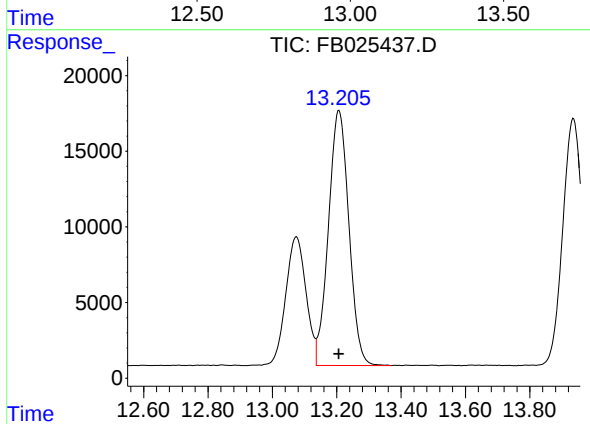

#8 m-Xylene


R.T.: 13.207 min
Delta R.T.: 0.000 min
Response: 745461
Conc: 18.53 ng/ml

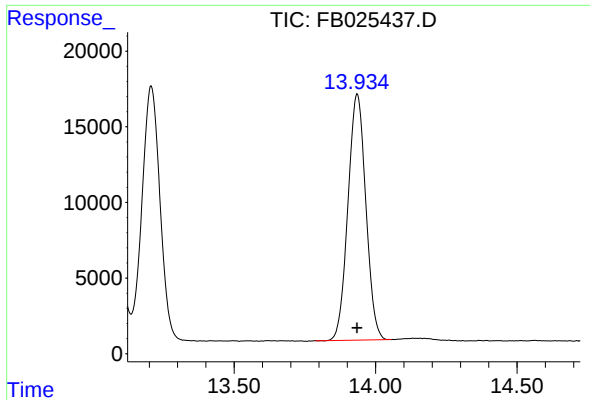

#9 O-Xylene

R.T.: 13.935 min
Delta R.T.: 0.001 min
Response: 714628
Conc: 18.46 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-021621MS

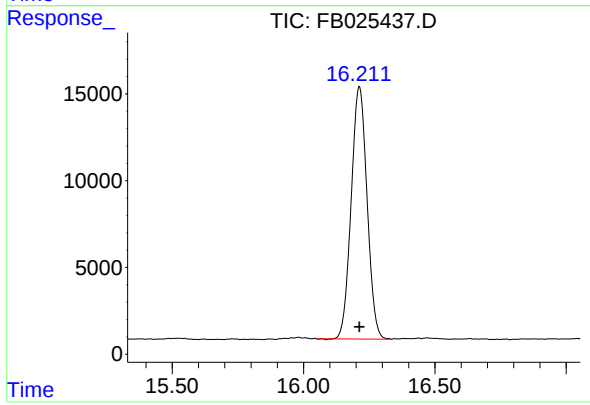

#10 1,2,4-Trimethylbenzene

R.T.: 16.213 min
Delta R.T.: 0.000 min
Response: 610492
Conc: 18.19 ng/ml