

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022221\
 Data File : FB025443.D
 Signal(s) : FID2B.CH
 Acq On : 22 Feb 2021 16:32
 Operator : DD/AJ
 Sample : M1422-01MSD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BU-03-021621MSD

Integration File: Calibration.e
 Quant Time: Feb 23 03:02:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
 Quant Title :
 QLast Update : Mon Feb 22 11:51:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.806	473076	18.651 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.693	930570	26.403 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	990685	26.680 ng/ml
3) t n-Heptane	7.764	324224	8.956 ng/ml
4) t Benzene	7.899	410026	8.876 ng/ml
6) t Toluene	10.637	1170269	26.175 ng/ml
7) t Ethylbenzene	13.077	350469	8.684 ng/ml
8) t m-Xylene	13.210	709908	17.647 ng/ml
9) t O-Xylene	13.938	678114	17.519 ng/ml
10) t 1,2,4-Trimethylbenzene	16.215	584505	17.412 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022221\
Data File : FB025443.D
Signal(s) : FID2B.CH
Acq On : 22 Feb 2021 16:32
Operator : DD/AJ
Sample : M1422-01MSD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BU-03-021621MSD

Integration File: Calibration.e
Quant Time: Feb 23 03:02:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021921.M
Quant Title :
QLast Update : Mon Feb 22 11:51:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

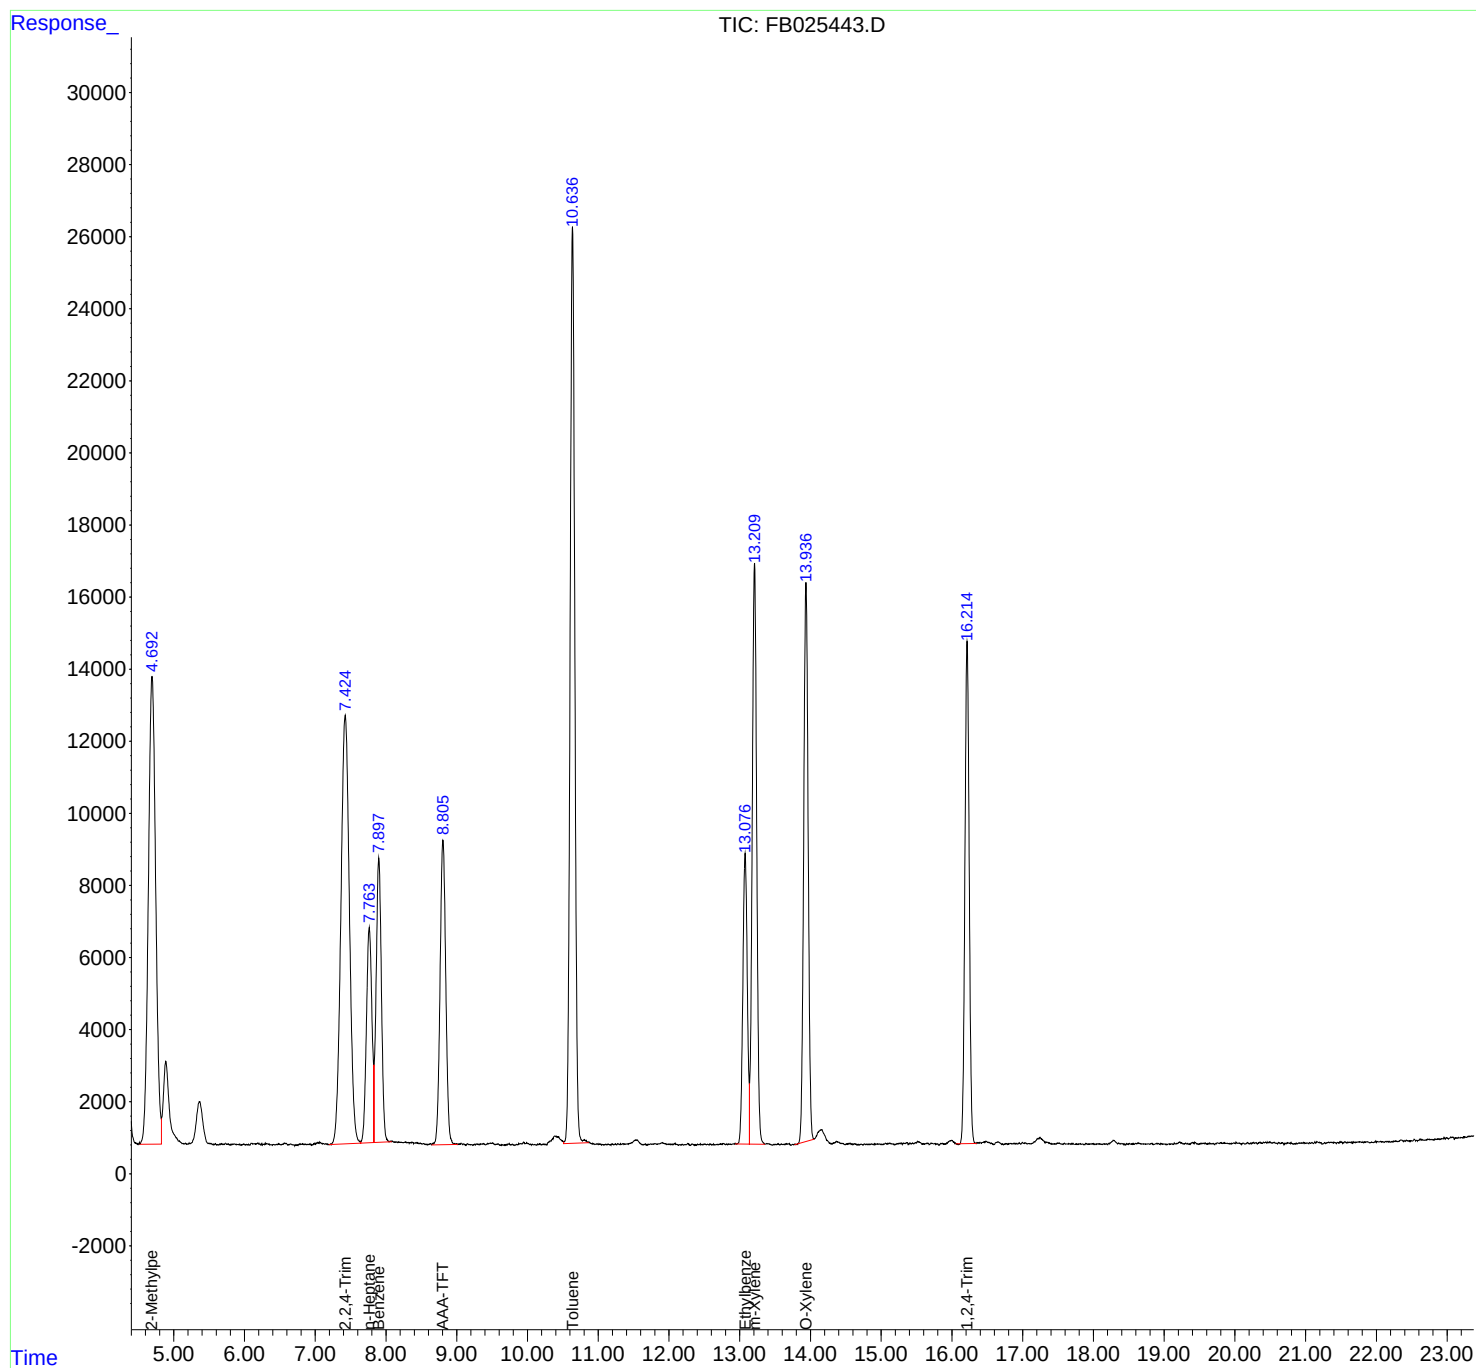


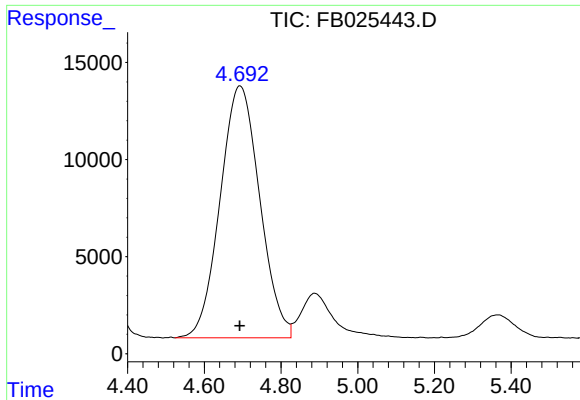

#1 2-Methylpentane


R.T.: 4.693 min
Delta R.T.: 0.001 min
Response: 930570
Conc: 26.40 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-021621MSD

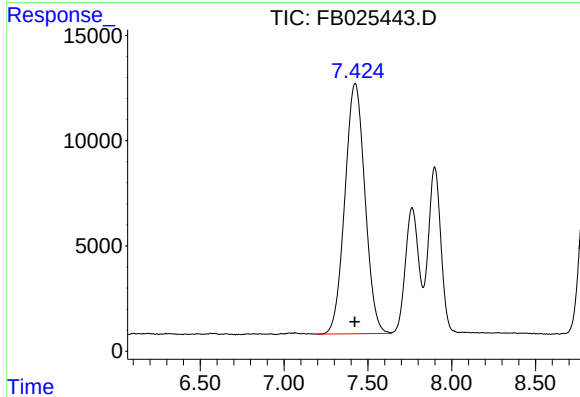


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: 0.004 min
Response: 990685
Conc: 26.68 ng/ml

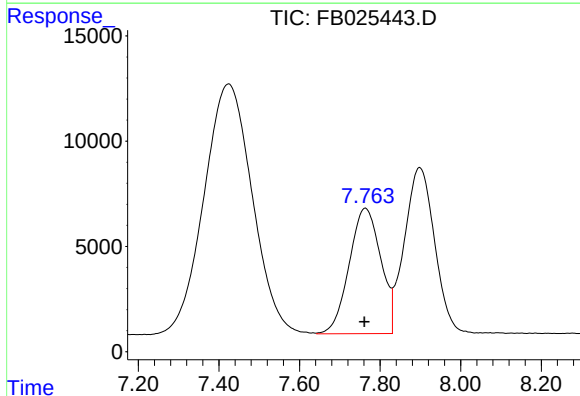


#3 n-Heptane

R.T.: 7.764 min
Delta R.T.: 0.003 min
Response: 324224
Conc: 8.96 ng/ml

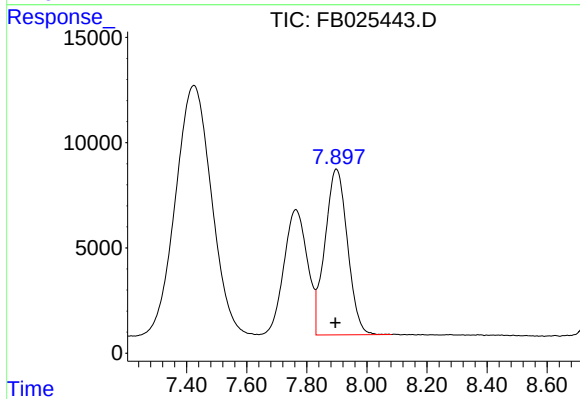

#4 Benzene


R.T.: 7.899 min
Delta R.T.: 0.003 min
Response: 410026
Conc: 8.88 ng/ml

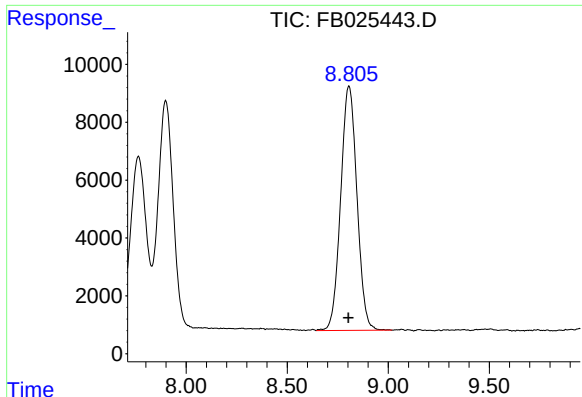

#5 AAA-TFT


R.T.: 8.806 min
Delta R.T.: 0.004 min
Response: 473076
Conc: 18.65 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-021621MSD

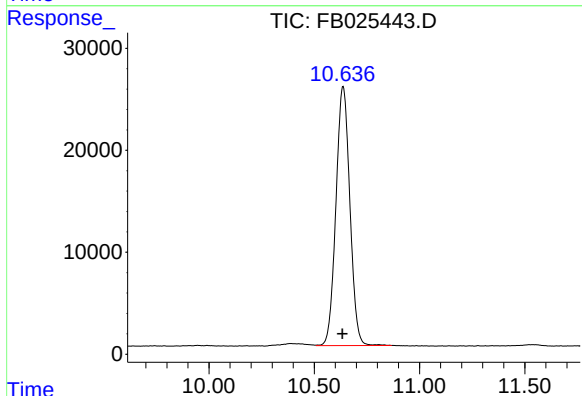


#6 Toluene

R.T.: 10.637 min
Delta R.T.: 0.004 min
Response: 1170269
Conc: 26.18 ng/ml

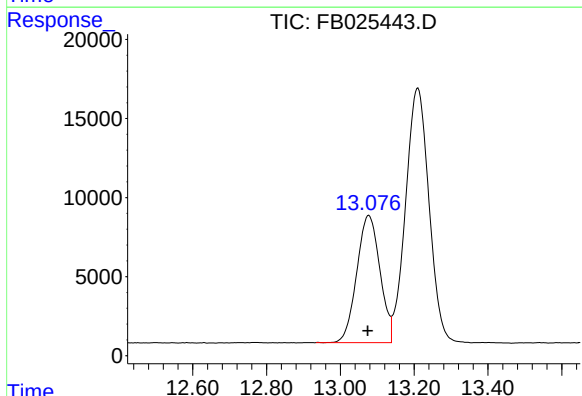


#7 Ethylbenzene

R.T.: 13.077 min
Delta R.T.: 0.003 min
Response: 350469
Conc: 8.68 ng/ml

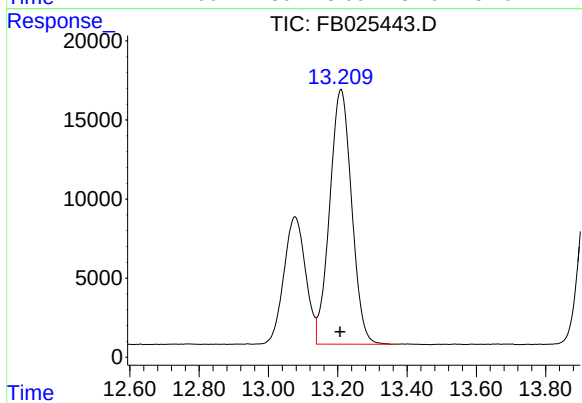

#8 m-Xylene


R.T.: 13.210 min
Delta R.T.: 0.003 min
Response: 709908
Conc: 17.65 ng/ml

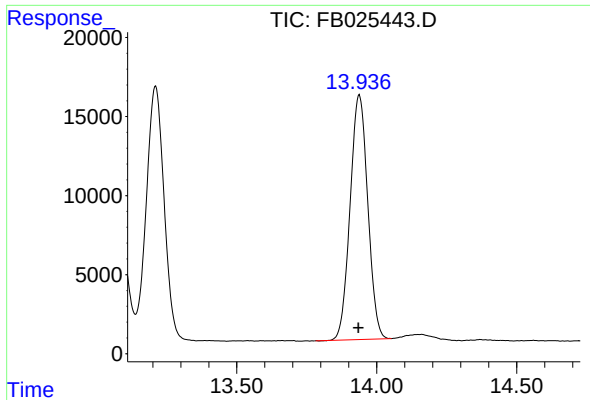

#9 O-Xylene

R.T.: 13.938 min
Delta R.T.: 0.003 min
Response: 678114
Conc: 17.52 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-021621MSD

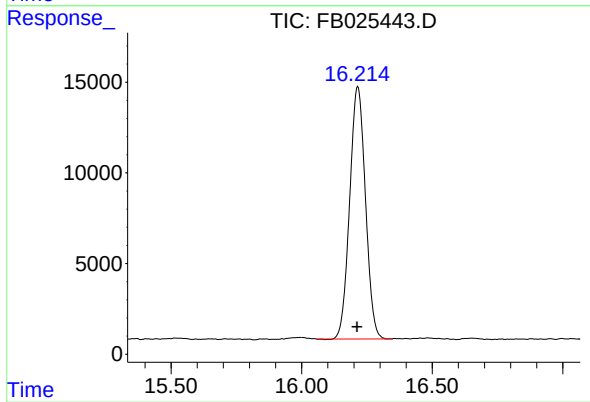

#10 1,2,4-Trimethylbenzene

R.T.: 16.215 min
Delta R.T.: 0.003 min
Response: 584505
Conc: 17.41 ng/ml