

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022222\
 Data File : FB026641.D
 Signal(s) : FID2B.CH
 Acq On : 22 Feb 2022 13:57
 Operator : AJ/MA
 Sample : BSF0222S1
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0222S1

Integration File: Calibration.e
 Quant Time: Feb 23 00:21:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021122.M
 Quant Title :
 QLast Update : Fri Feb 11 12:15:14 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	230453	22.313 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	488493	31.367 ng/ml
2) t 2,2,4-Trimethylpentane	7.437	596135	32.743 ng/ml
3) t n-Heptane	7.749	160351	9.050 ng/ml
4) t Benzene	7.886	203701	9.976 ng/ml
6) t Toluene	10.620	591383	30.115 ng/ml
7) t Ethylbenzene	13.057	188375	10.199 ng/ml
8) t m-Xylene	13.189	385112	20.896 ng/ml
9) t O-Xylene	13.916	388764	21.618 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	412596	22.345 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022222\
Data File : FB026641.D
Signal(s) : FID2B.CH
Acq On : 22 Feb 2022 13:57
Operator : AJ/MA
Sample : BSF0222S1
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0222S1

Integration File: Calibration.e
Quant Time: Feb 23 00:21:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021122.M
Quant Title :
QLast Update : Fri Feb 11 12:15:14 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

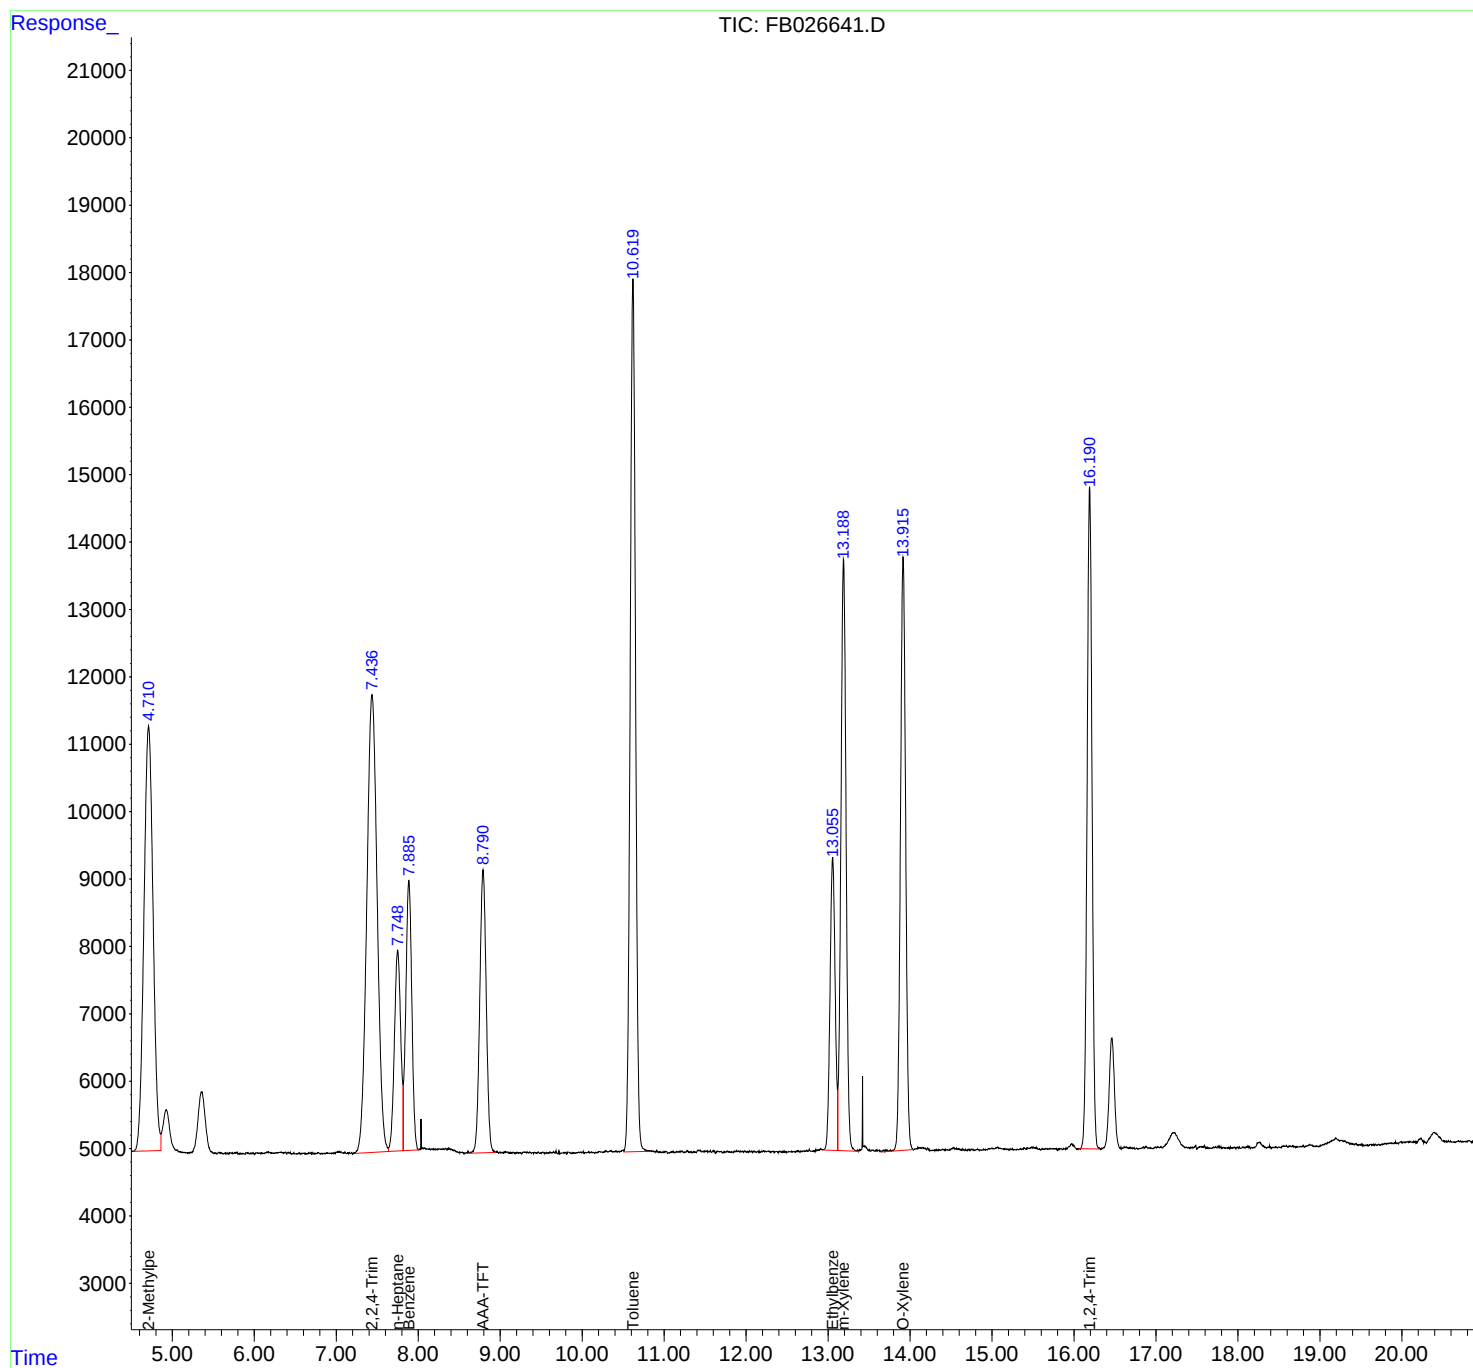


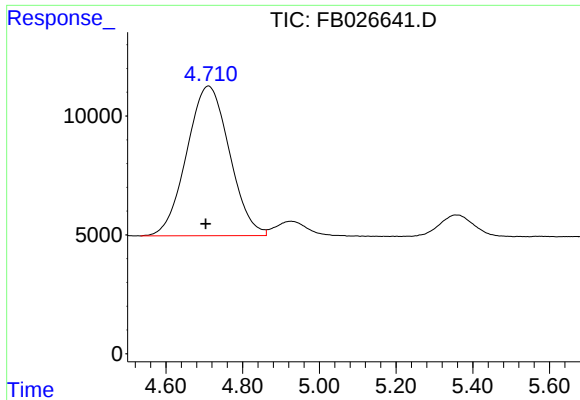

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.008 min
Response: 488493
Conc: 31.37 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0222S1

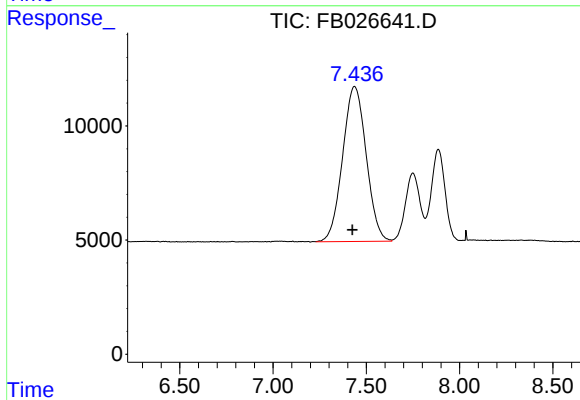


#2 2,2,4-Trimethylpentane

R.T.: 7.437 min
Delta R.T.: 0.012 min
Response: 596135
Conc: 32.74 ng/ml

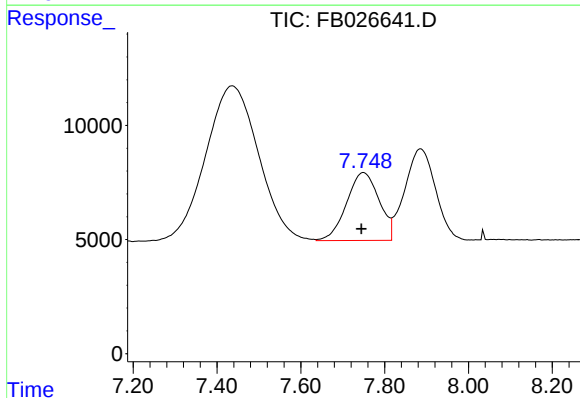


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.004 min
Response: 160351
Conc: 9.05 ng/ml

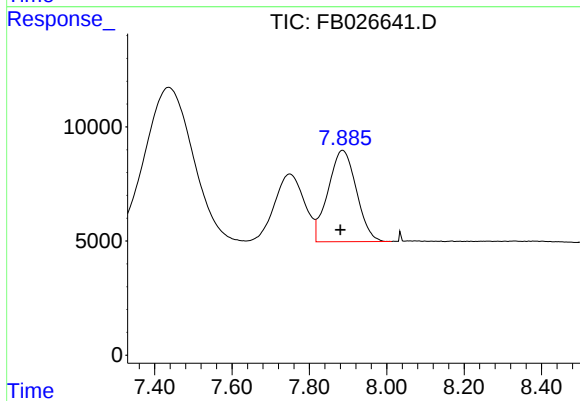

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.006 min
Response: 203701
Conc: 9.98 ng/ml

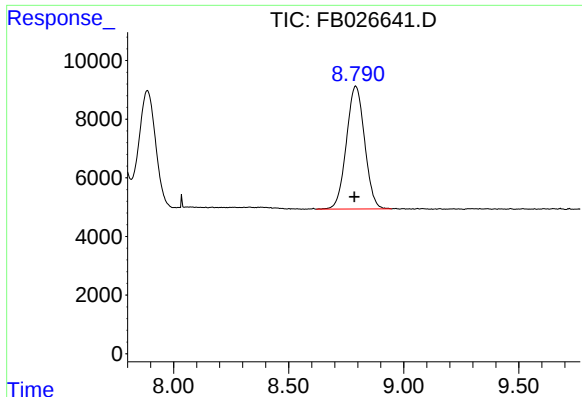

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.005 min
Response: 230453
Conc: 22.31 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0222S1

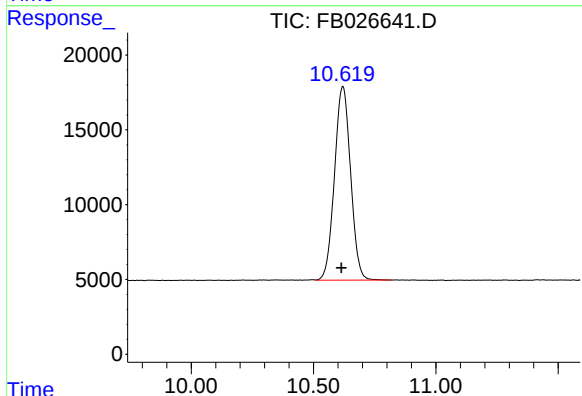


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.007 min
Response: 591383
Conc: 30.11 ng/ml

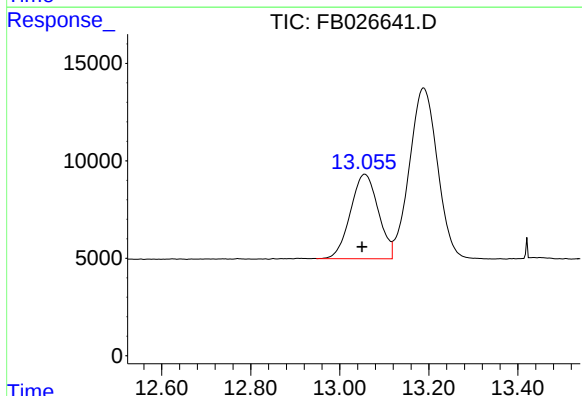


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.006 min
Response: 188375
Conc: 10.20 ng/ml

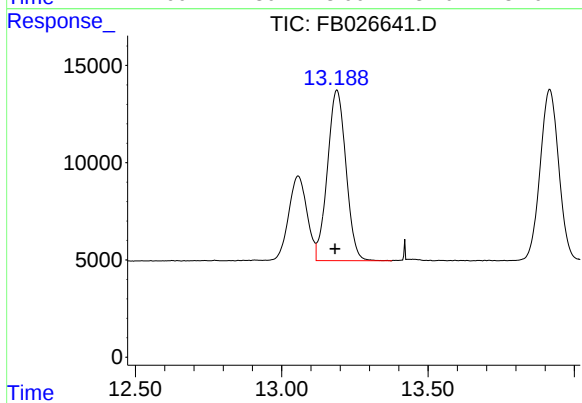

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.006 min
Response: 385112
Conc: 20.90 ng/ml

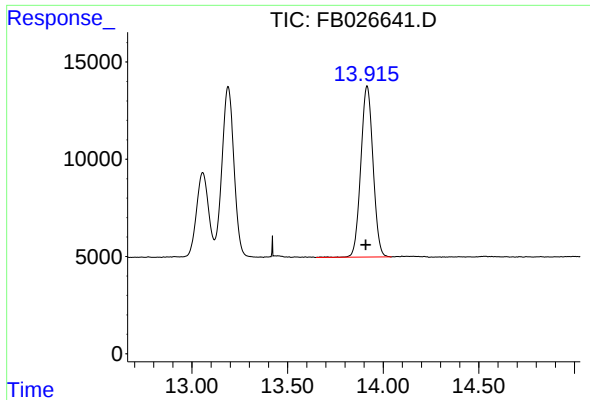

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.006 min
Response: 388764
Conc: 21.62 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0222S1

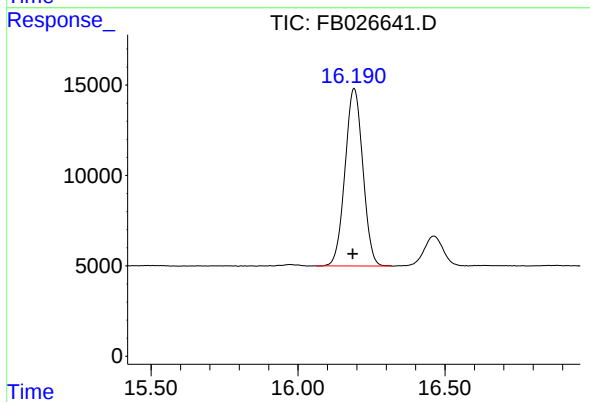

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.006 min
Response: 412596
Conc: 22.34 ng/ml