

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022222\
 Data File : FB026643.D
 Signal(s) : FID2B.CH
 Acq On : 22 Feb 2022 15:13
 Operator : AJ/MA
 Sample : N1614-01MS
 Misc : 5.05G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 WASTE-BUILDINGMS

Integration File: Calibration.e
 Quant Time: Feb 23 00:21:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021122.M
 Quant Title :
 QLast Update : Fri Feb 11 12:15:14 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	253837	24.577 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	550834	35.370 ng/ml
2) t 2,2,4-Trimethylpentane	7.448	626649	34.419 ng/ml
3) t n-Heptane	7.751	207755	11.726 ng/ml
4) t Benzene	7.888	227047	11.120 ng/ml
6) t Toluene	10.621	646083	32.900 ng/ml
7) t Ethylbenzene	13.058	199230	10.787 ng/ml
8) t m-Xylene	13.191	393539	21.353 ng/ml
9) t O-Xylene	13.918	372438	20.710 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	355636	19.260 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022222\
Data File : FB026643.D
Signal(s) : FID2B.CH
Acq On : 22 Feb 2022 15:13
Operator : AJ/MA
Sample : N1614-01MS
Misc : 5.05G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
WASTE-BUILDINGMS

Integration File: Calibration.e
Quant Time: Feb 23 00:21:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB021122.M
Quant Title :
QLast Update : Fri Feb 11 12:15:14 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

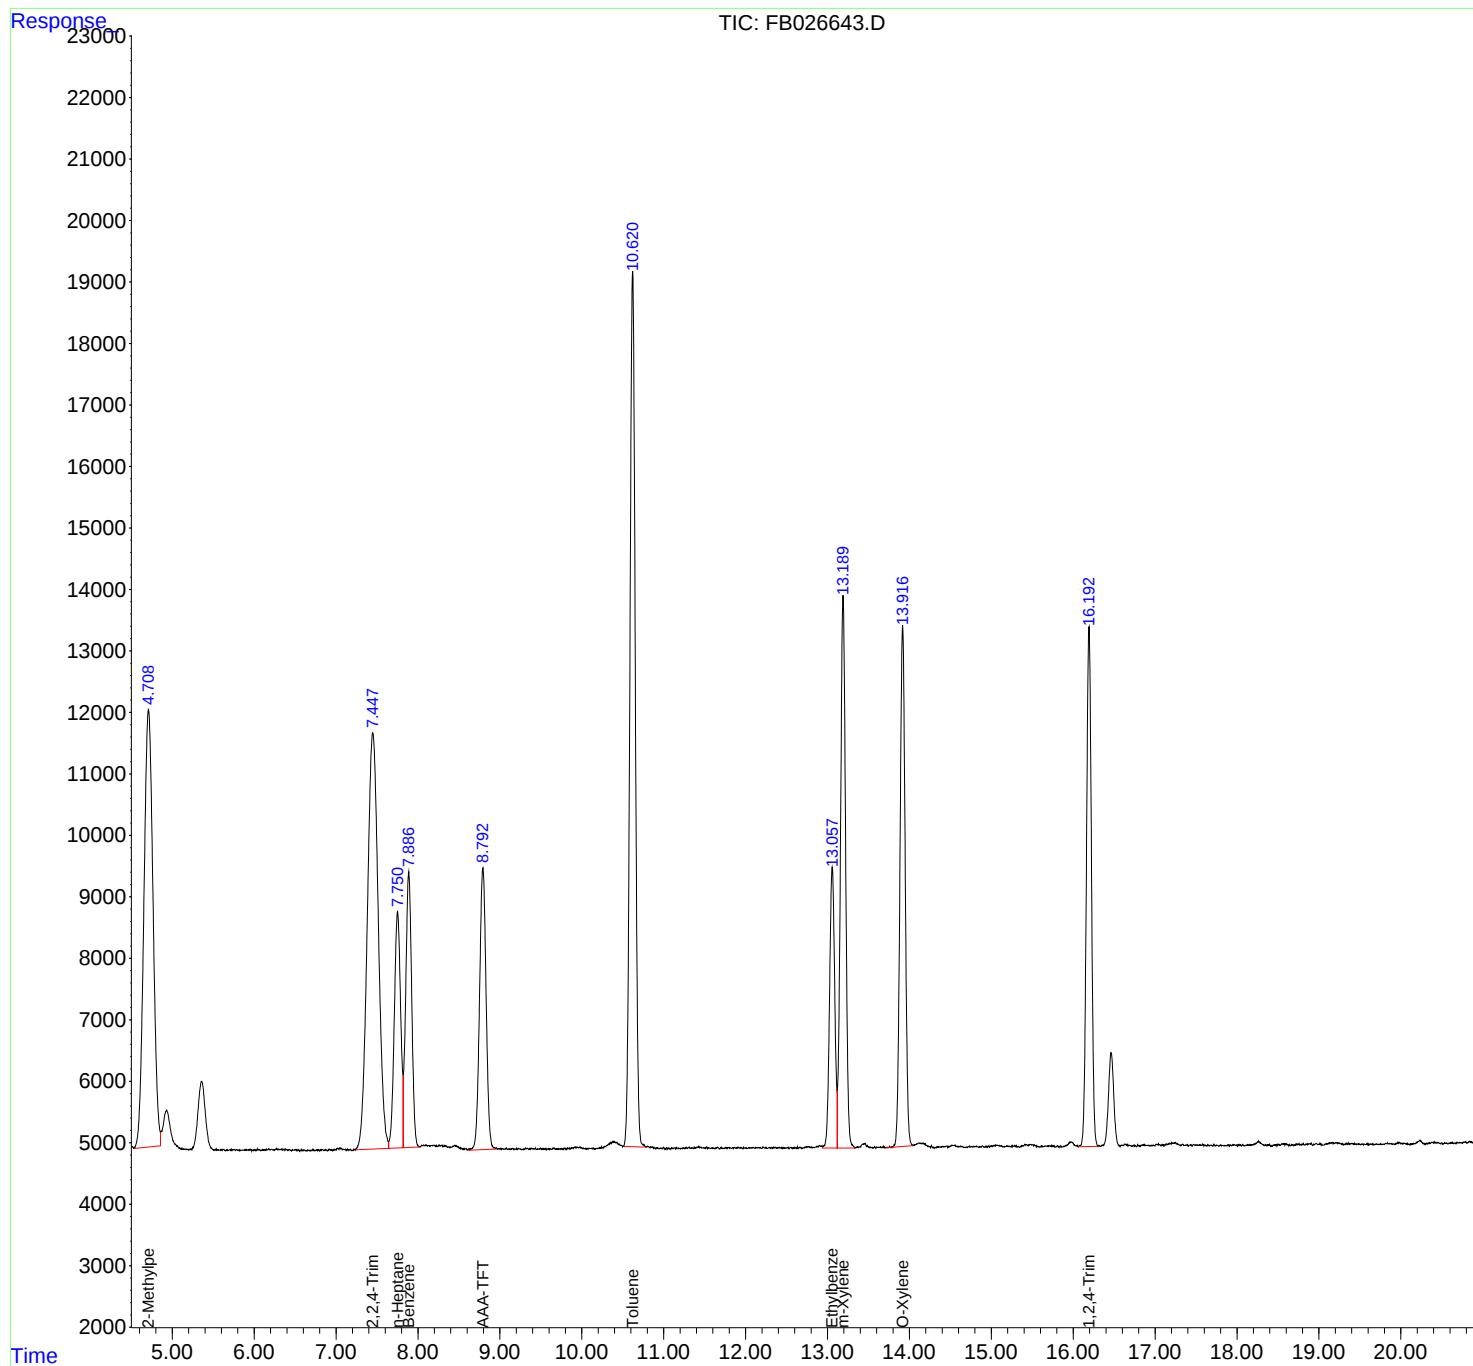


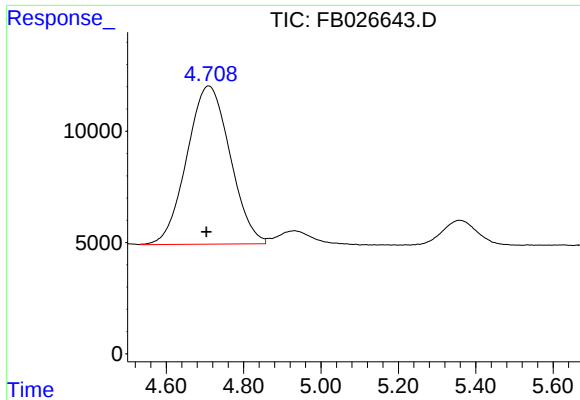

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.006 min
Response: 550834
Conc: 35.37 ng/ml

Instrument :
FID_B
ClientSampleId :
WASTE-BUILDINGMS

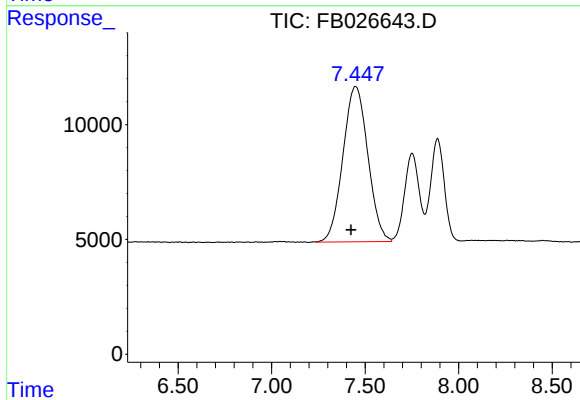


#2 2,2,4-Trimethylpentane

R.T.: 7.448 min
Delta R.T.: 0.023 min
Response: 626649
Conc: 34.42 ng/ml

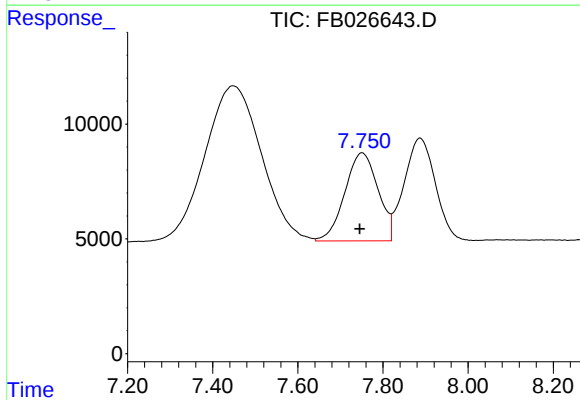


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.006 min
Response: 207755
Conc: 11.73 ng/ml

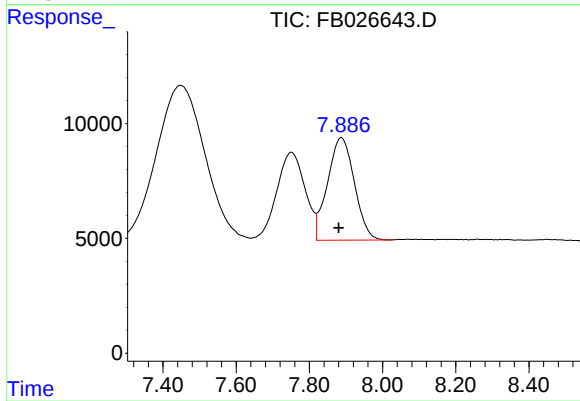

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.007 min
Response: 227047
Conc: 11.12 ng/ml

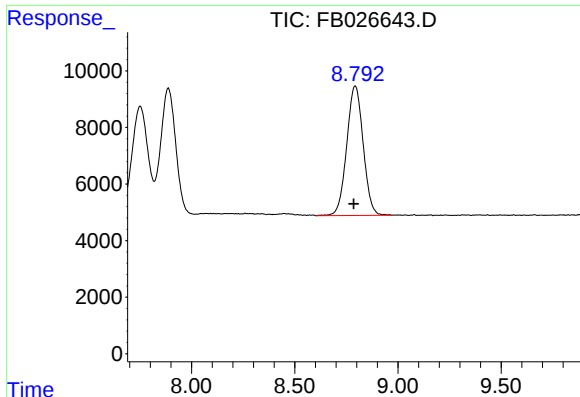

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.007 min
Response: 253837
Conc: 24.58 ng/ml

Instrument :
FID_B
ClientSampleId :
WASTE-BUILDINGMS

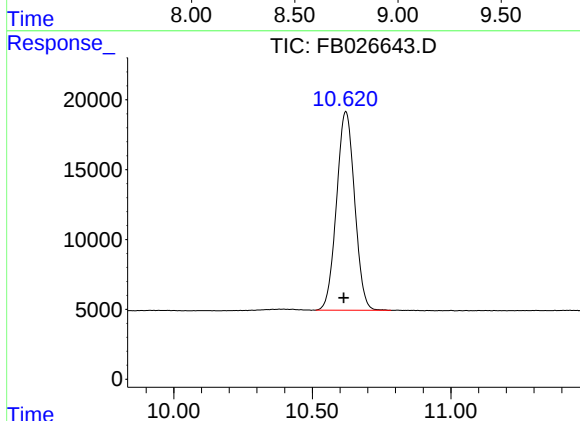


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.008 min
Response: 646083
Conc: 32.90 ng/ml

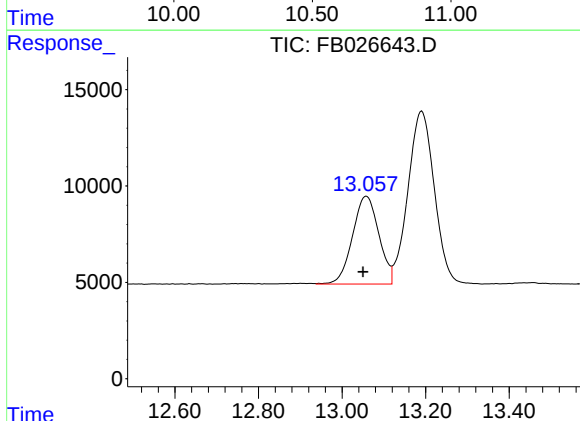


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.008 min
Response: 199230
Conc: 10.79 ng/ml

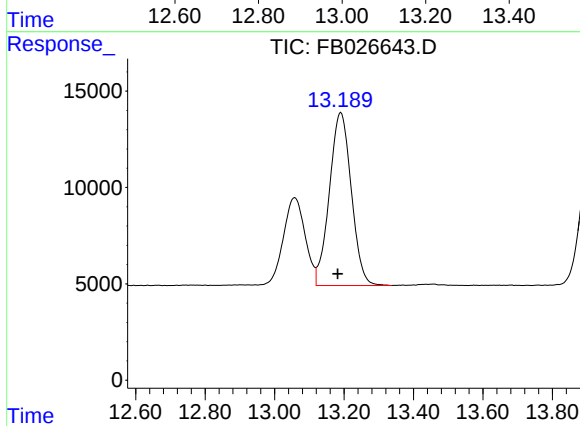

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.008 min
Response: 393539
Conc: 21.35 ng/ml

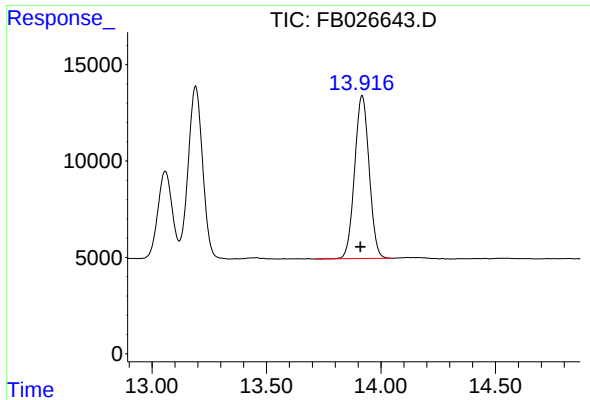

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.008 min
Response: 372438
Conc: 20.71 ng/ml

Instrument :
FID_B
ClientSampleId :
WASTE-BUILDINGMS

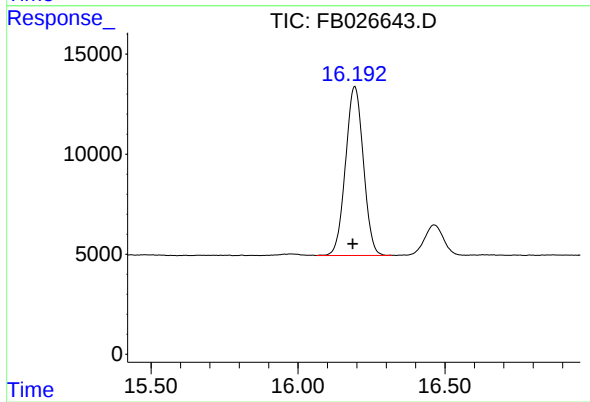

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.008 min
Response: 355636
Conc: 19.26 ng/ml