

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022223\
 Data File : FB029370.D
 Signal(s) : FID2B.CH
 Acq On : 22 Feb 2023 16:00
 Operator : YP/AJ
 Sample : 01627-08
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 23 00:25:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	220013	22.874 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	107403	6.769 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	126179	7.326 ng/ml
3) t n-Heptane	7.749	43264	2.391 ng/ml
4) t Benzene	7.886	51629	2.479 ng/ml
6) t Toluene	10.620	153148	7.557 ng/ml
7) t Ethylbenzene	13.057	48914	2.563 ng/ml
8) t m-Xylene	13.189	95727	5.049 ng/ml
9) t O-Xylene	13.916	93039	5.099 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	94107	5.001 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022223\
Data File : FB029370.D
Signal(s) : FID2B.CH
Acq On : 22 Feb 2023 16:00
Operator : YP/AJ
Sample : 01627-08
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 23 00:25:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

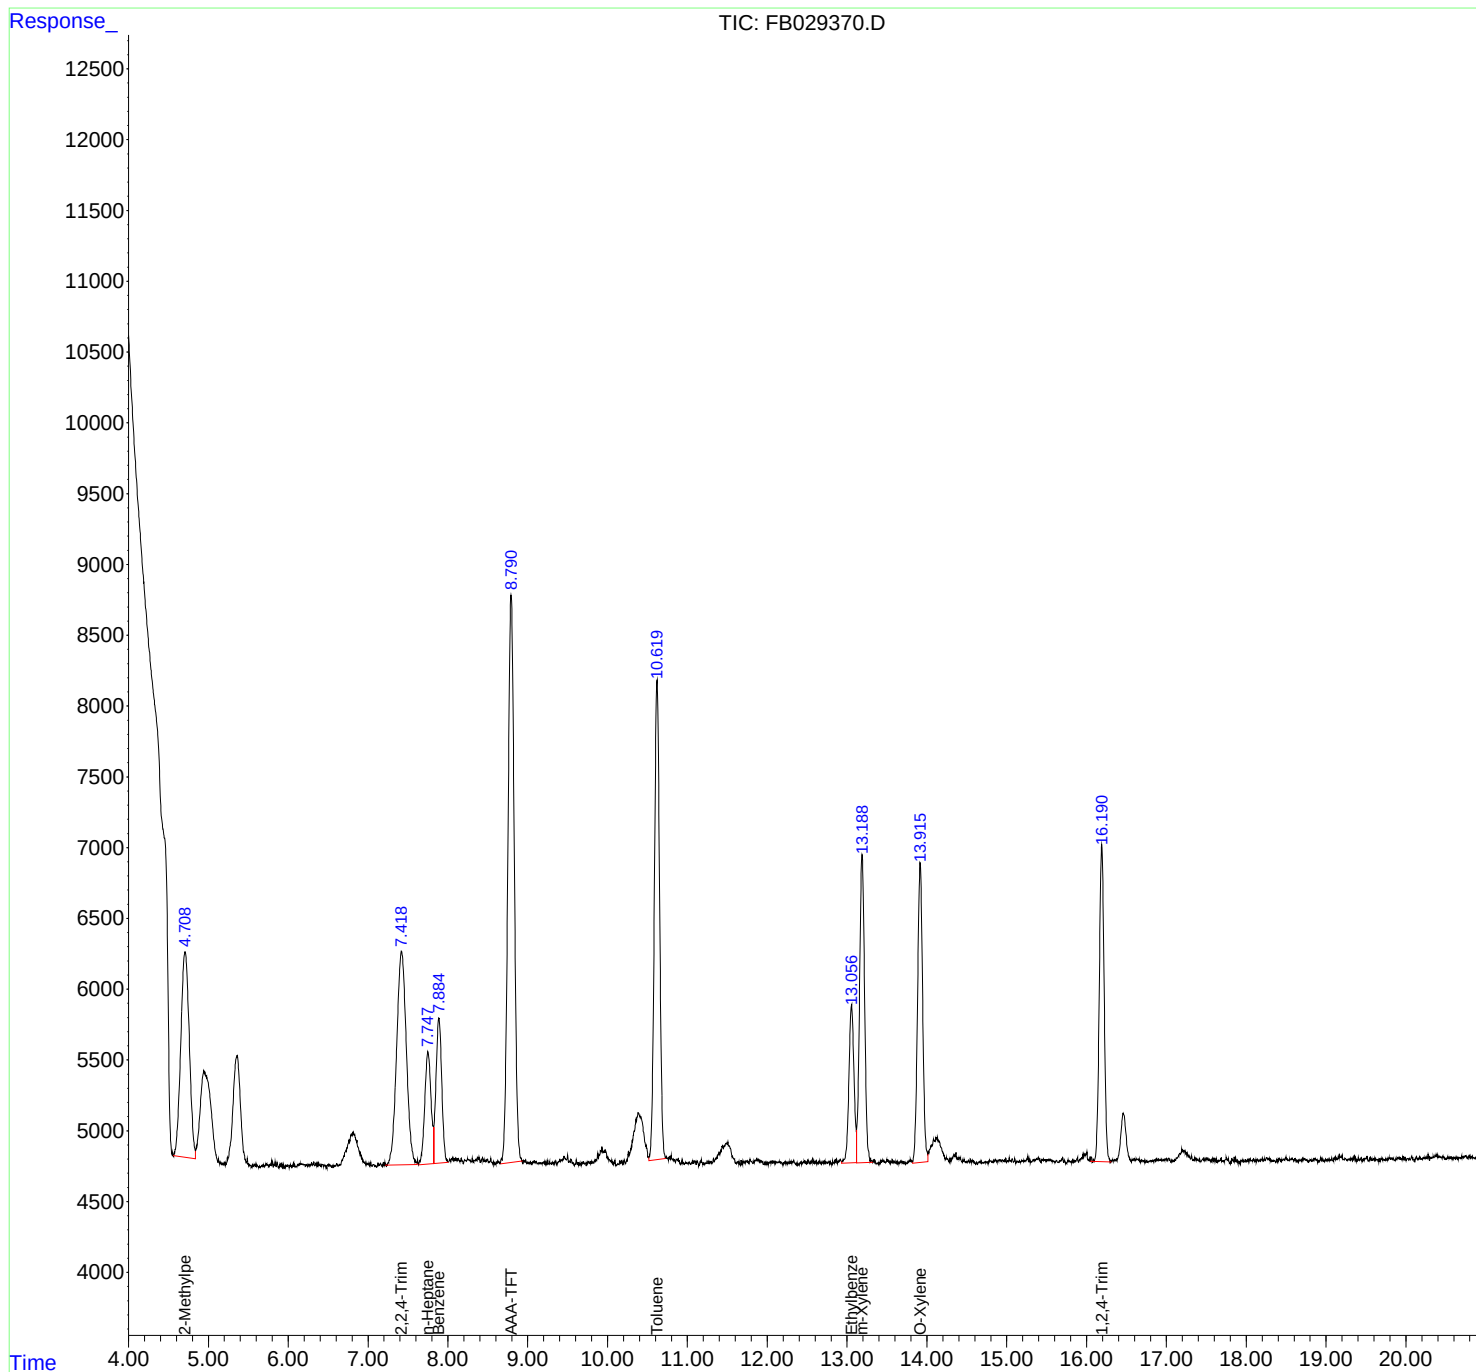

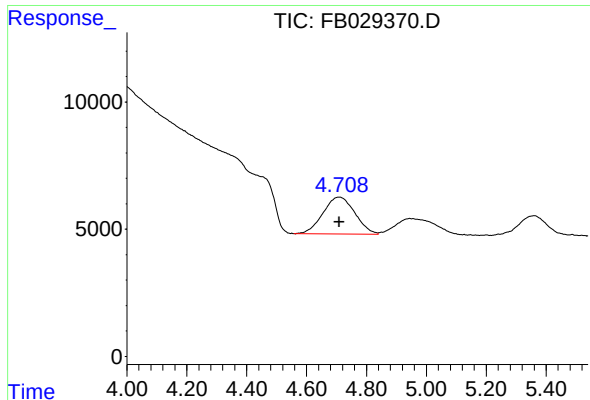


#1 2-Methylpentane

R.T.: 4.709 min
Delta R.T.: 0.000 min
Response: 107403
Conc: 6.77 ng/ml

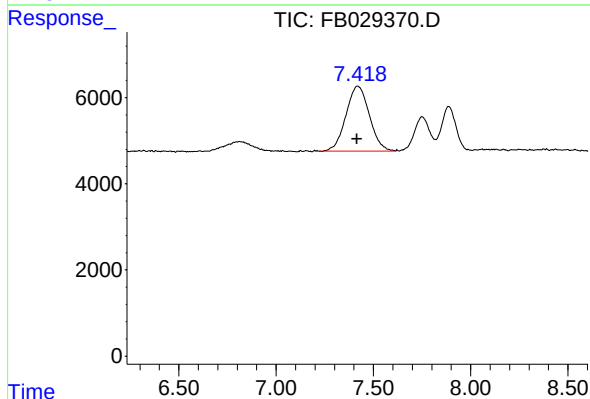


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.005 min
Response: 126179
Conc: 7.33 ng/ml

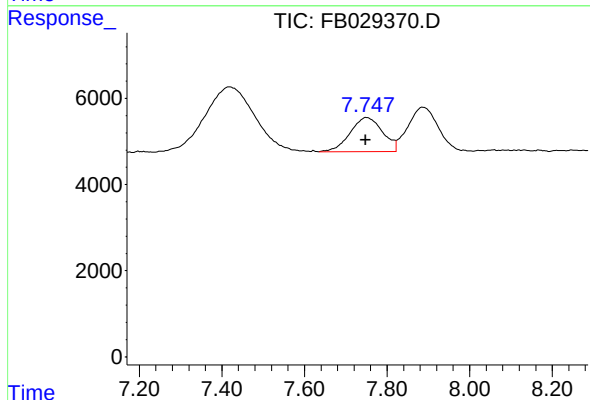


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 43264
Conc: 2.39 ng/ml

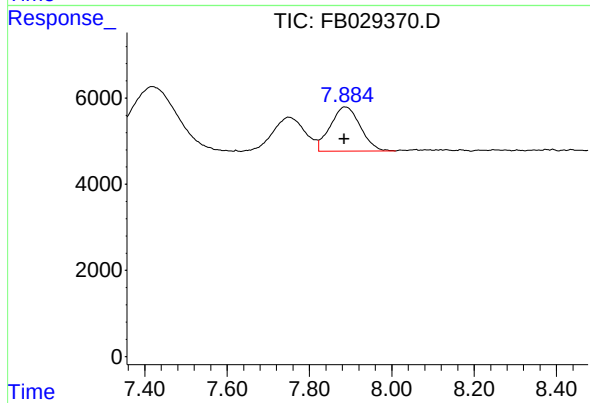


#4 Benzene

R.T.: 7.886 min
Delta R.T.: 0.002 min
Response: 51629
Conc: 2.48 ng/ml

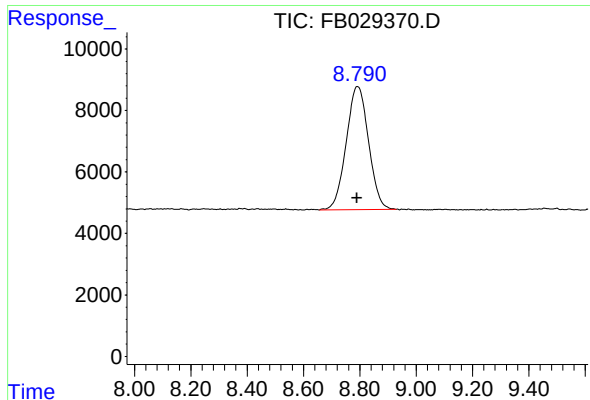


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.002 min
Response: 220013
Conc: 22.87 ng/ml

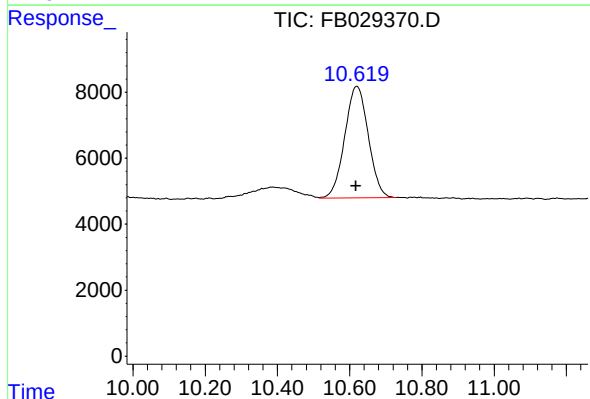


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.003 min
Response: 153148
Conc: 7.56 ng/ml

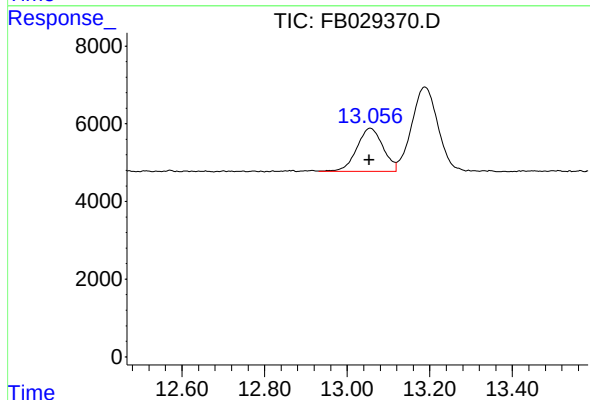


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.003 min
Response: 48914
Conc: 2.56 ng/ml

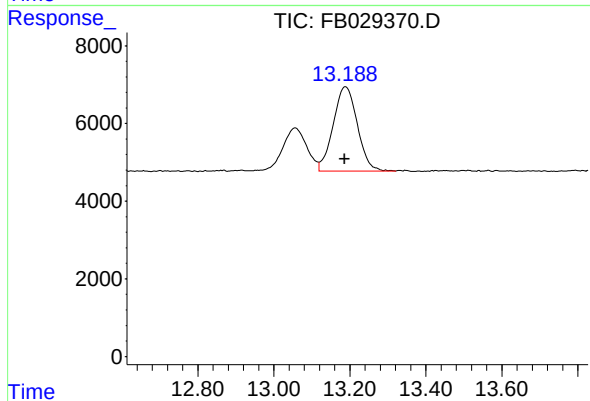


#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: 0.003 min
Response: 95727
Conc: 5.05 ng/ml

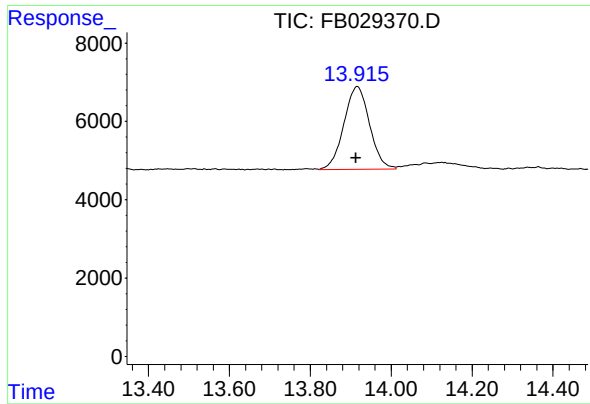

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.004 min
Response: 93039
Conc: 5.10 ng/ml

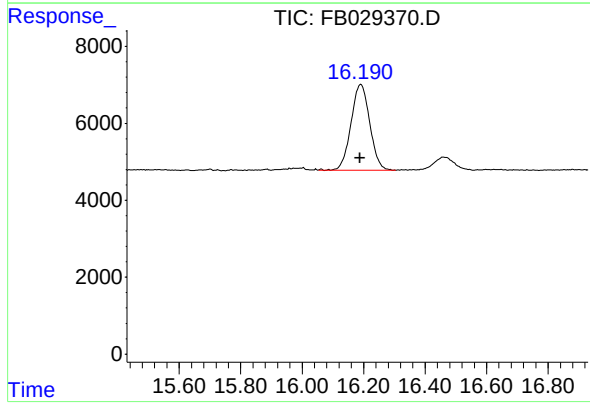

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.003 min
Response: 94107
Conc: 5.00 ng/ml