

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022223\
 Data File : FB029362.D
 Signal(s) : FID2B.CH
 Acq On : 22 Feb 2023 10:53
 Operator : YP/AJ
 Sample : BSF0222S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 23 00:24:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	211489	21.988 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	451685	28.467 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	518781	30.121 ng/ml
3) t n-Heptane	7.747	171031	9.452 ng/ml
4) t Benzene	7.883	207234	9.949 ng/ml
6) t Toluene	10.616	599925	29.604 ng/ml
7) t Ethylbenzene	13.053	193579	10.142 ng/ml
8) t m-Xylene	13.185	382558	20.179 ng/ml
9) t O-Xylene	13.912	369407	20.246 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	374368	19.893 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022223\
Data File : FB029362.D
Signal(s) : FID2B.CH
Acq On : 22 Feb 2023 10:53
Operator : YP/AJ
Sample : BSF0222S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 23 00:24:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

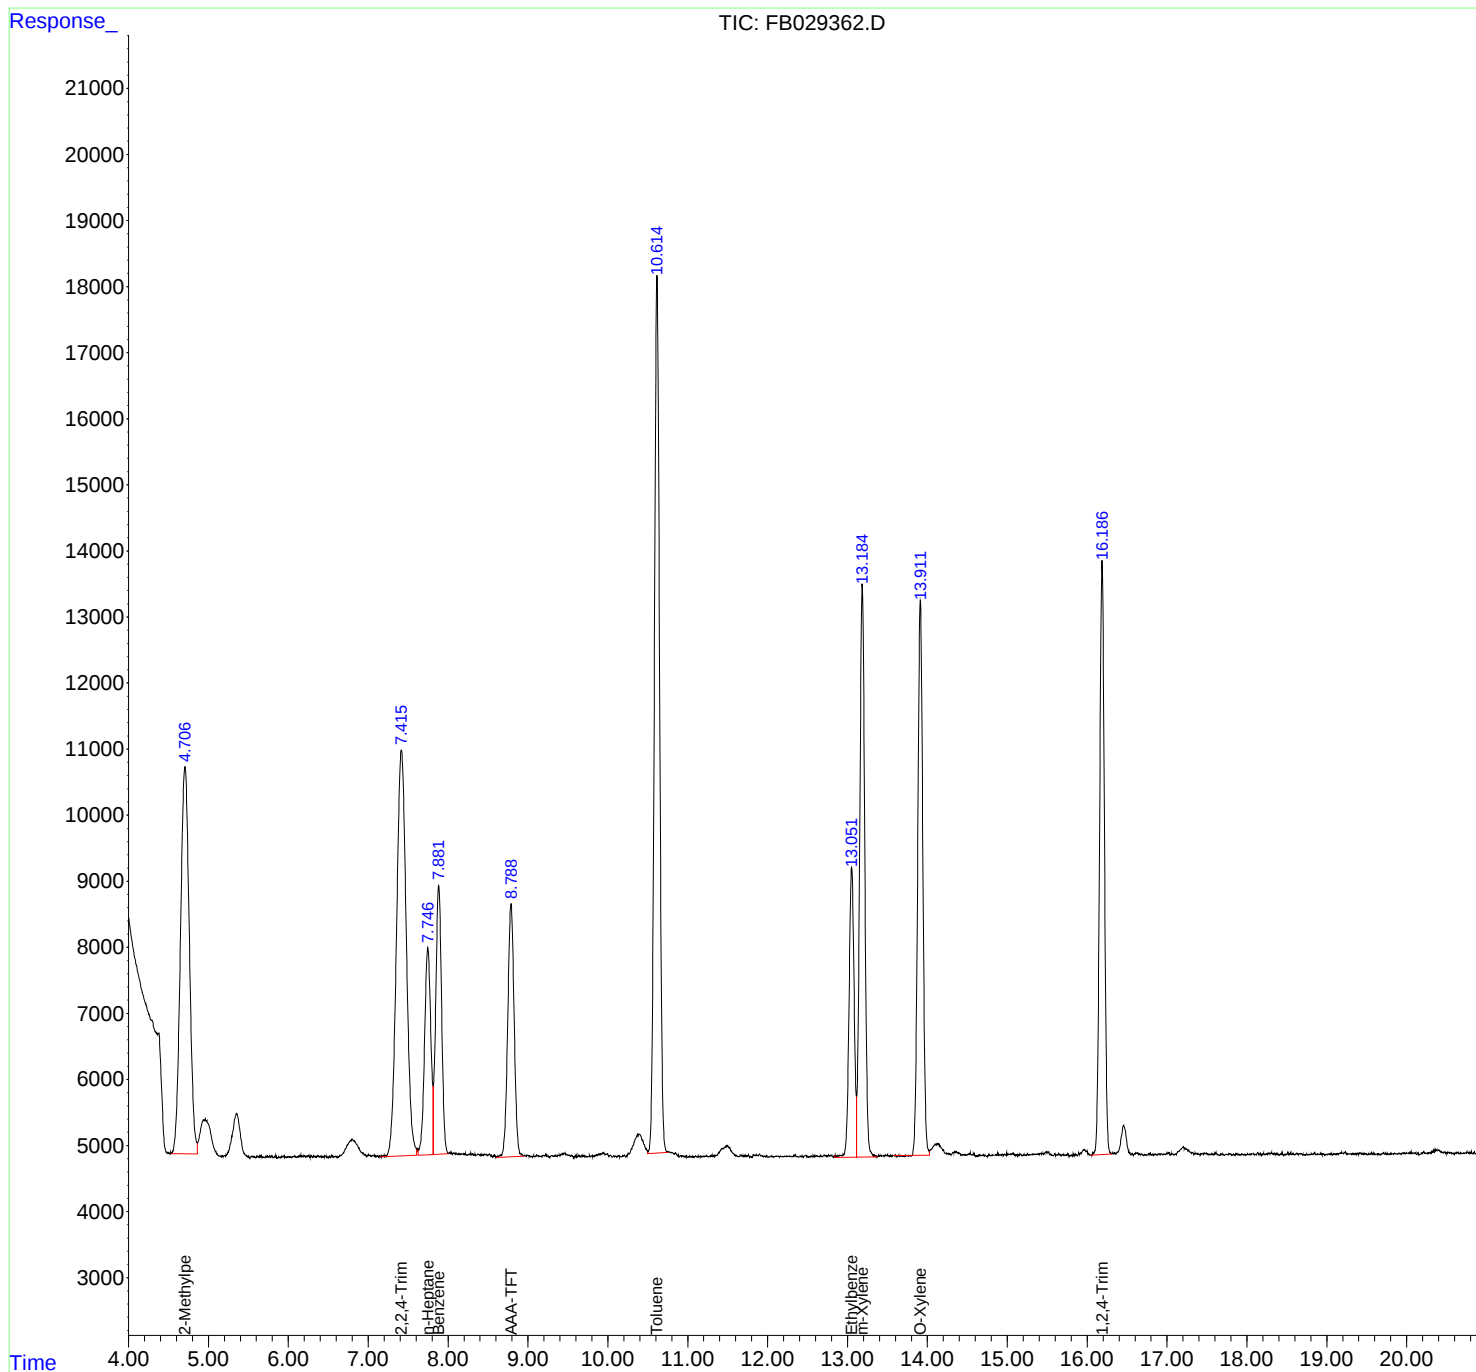

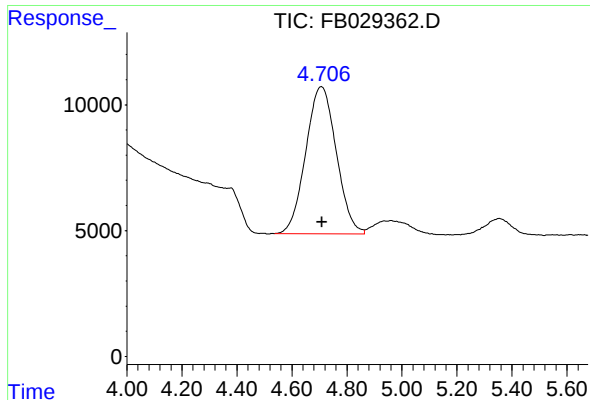


#1 2-Methylpentane

R.T.: 4.707 min
Delta R.T.: -0.002 min
Response: 451685
Conc: 28.47 ng/ml

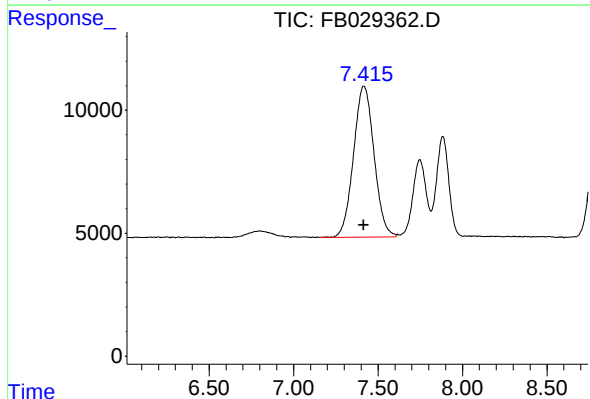


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.001 min
Response: 518781
Conc: 30.12 ng/ml

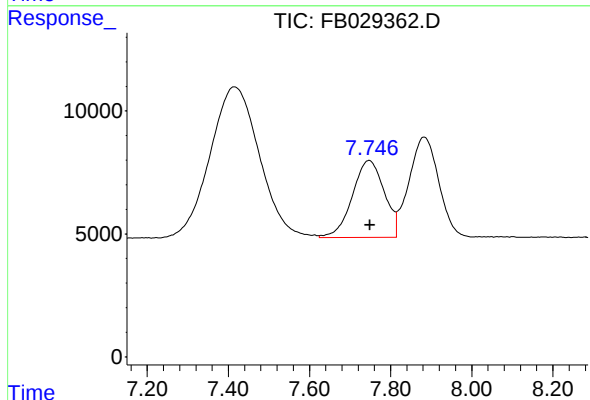


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.001 min
Response: 171031
Conc: 9.45 ng/ml

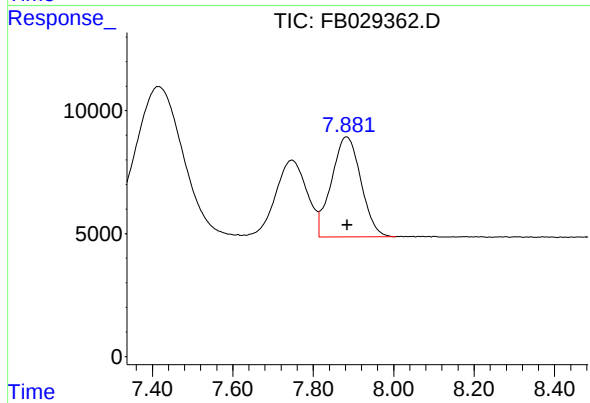


#4 Benzene

R.T.: 7.883 min
Delta R.T.: -0.002 min
Response: 207234
Conc: 9.95 ng/ml

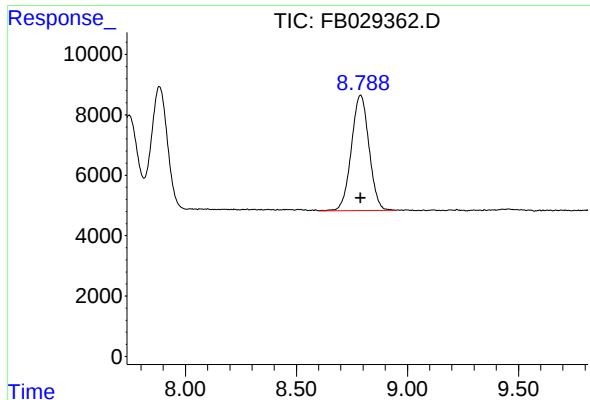


#5 AAA-TFT

R.T.: 8.789 min
Delta R.T.: 0.000 min
Response: 211489
Conc: 21.99 ng/ml

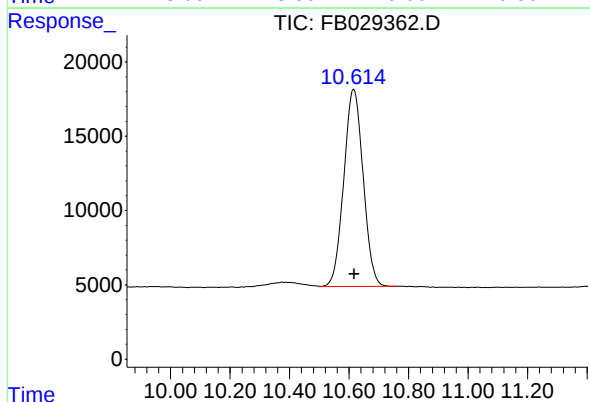


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.001 min
Response: 599925
Conc: 29.60 ng/ml

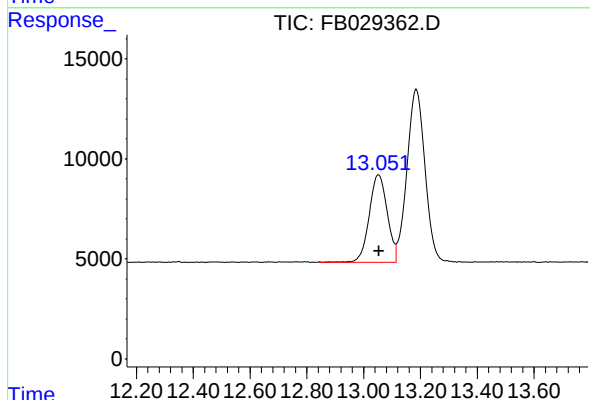


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.001 min
Response: 193579
Conc: 10.14 ng/ml

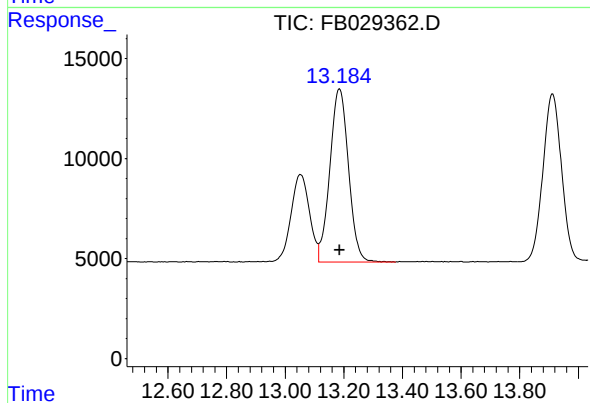


#8 m-Xylene

R.T.: 13.185 min
Delta R.T.: 0.000 min
Response: 382558
Conc: 20.18 ng/ml

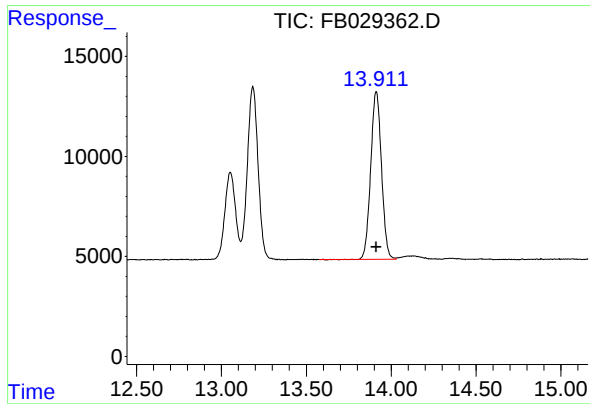

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: 0.000 min
Response: 369407
Conc: 20.25 ng/ml

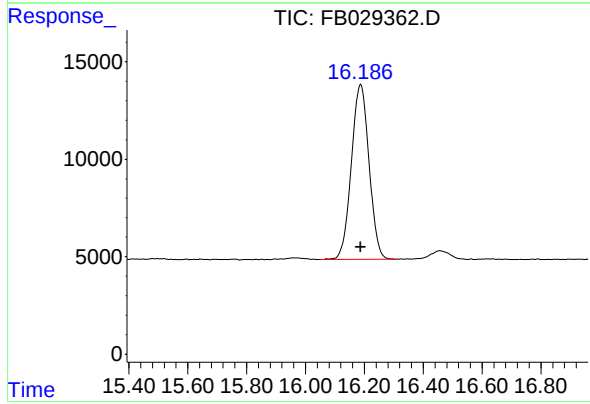

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: 0.000 min
Response: 374368
Conc: 19.89 ng/ml