

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022223\
 Data File : FB029363.D
 Signal(s) : FID2B.CH
 Acq On : 22 Feb 2023 11:30
 Operator : YP/AJ
 Sample : 01627-01
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 23 00:24:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	211103	21.948 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.694	25617	1.614 ng/mlm
2) t 2,2,4-Trimethylpentane	7.416	32386	1.880 ng/mlm
3) t n-Heptane	7.727	11441	0.632 ng/mlm
4) t Benzene	7.883	12920	0.620 ng/ml
6) t Toluene	10.616	36462	1.799 ng/ml
7) t Ethylbenzene	13.057	11576	0.607 ng/ml
8) t m-Xylene	13.186	23594	1.245 ng/ml
9) t O-Xylene	13.914	22710	1.245 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	28000	1.488 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022223\
Data File : FB029363.D
Signal(s) : FID2B.CH
Acq On : 22 Feb 2023 11:30
Operator : YP/AJ
Sample : 01627-01
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 23 00:24:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

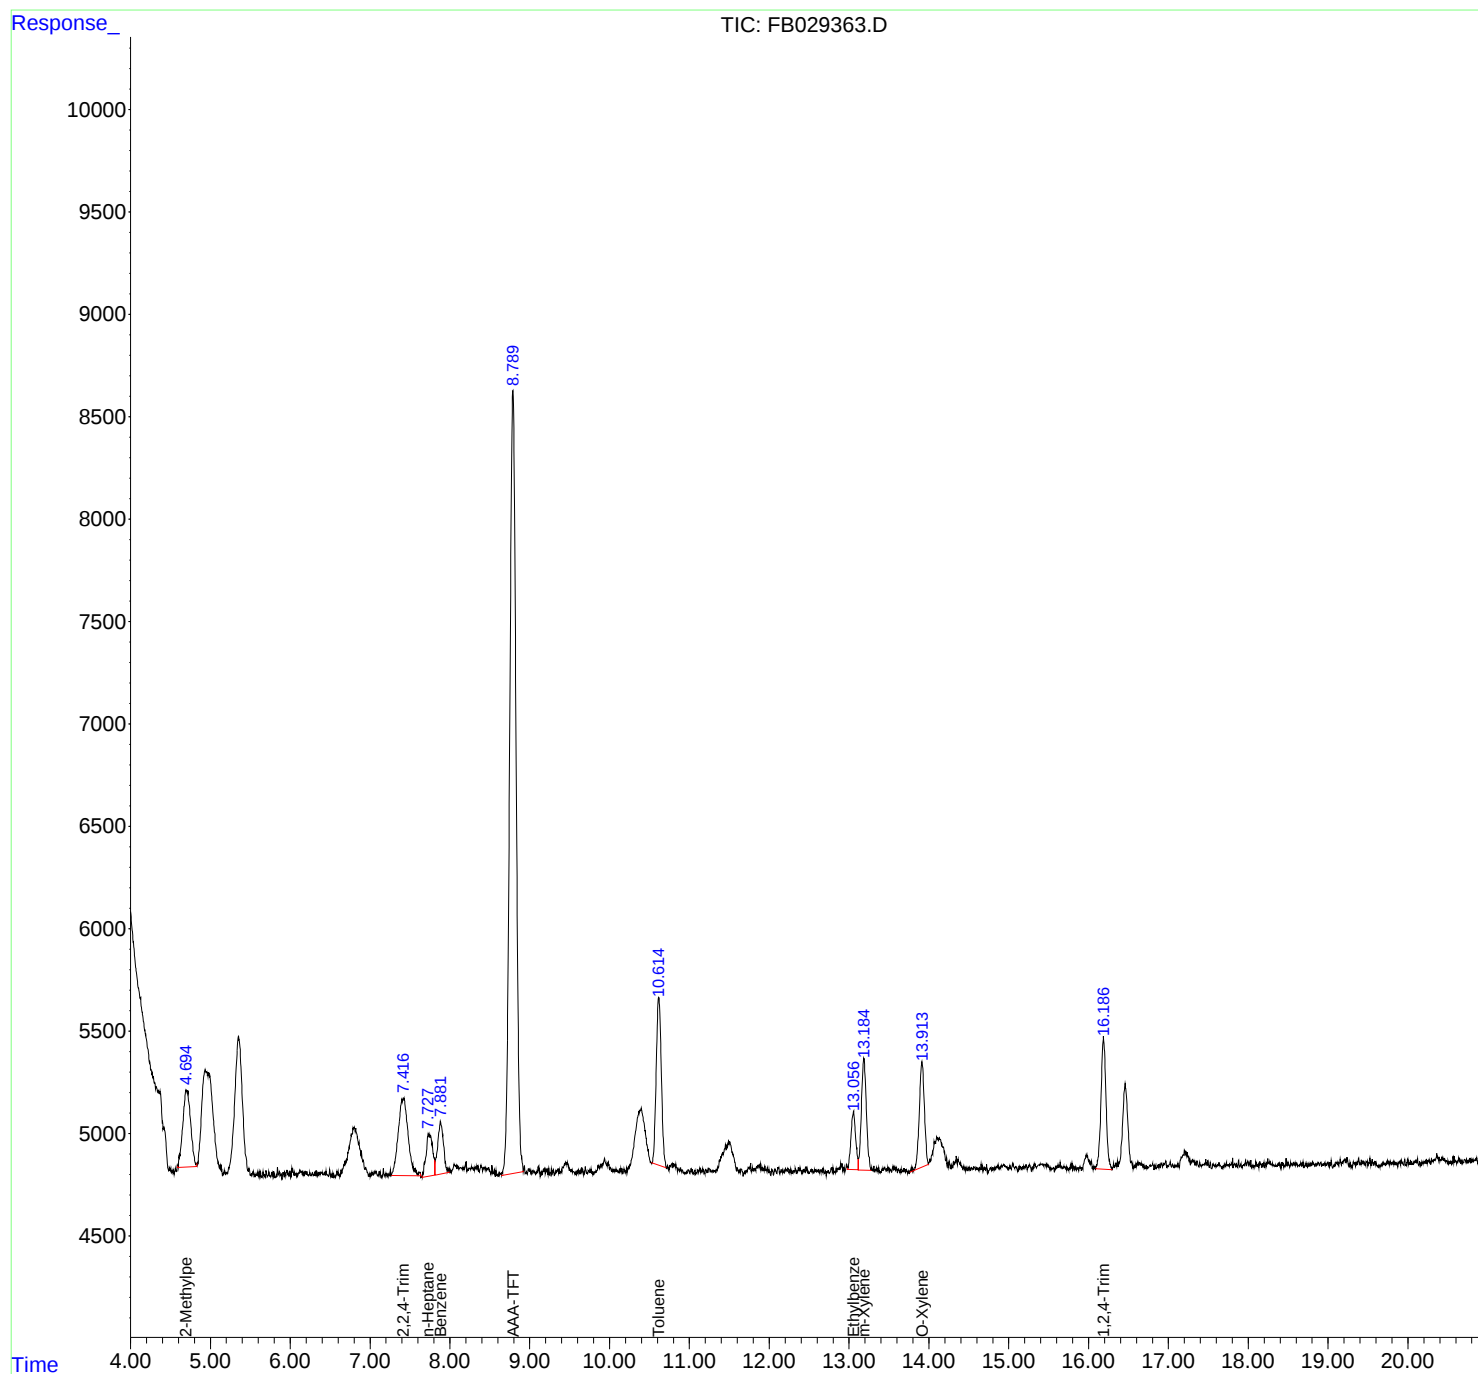

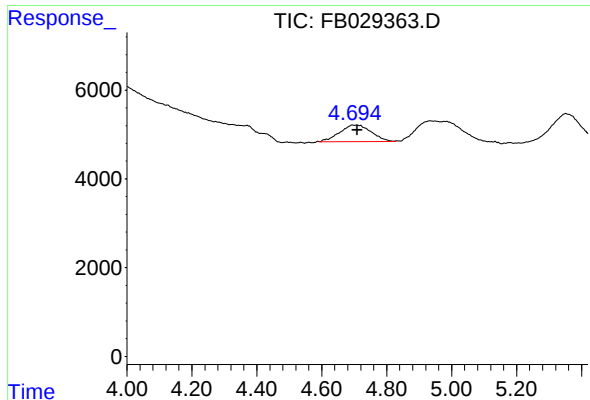


#1 2-Methylpentane

R.T.: 4.694 min
Delta R.T.: -0.015 min
Response: 25617
Conc: 1.61 ng/ml m

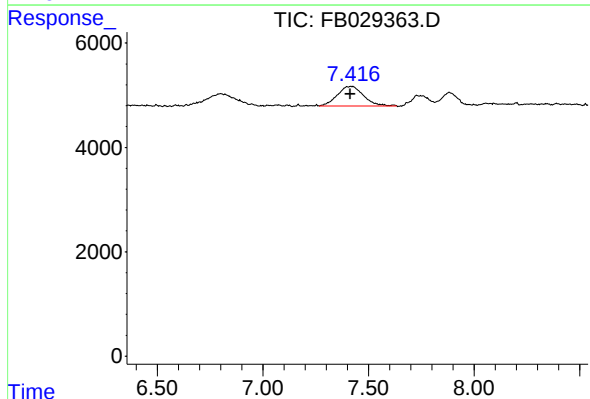


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.002 min
Response: 32386
Conc: 1.88 ng/ml m

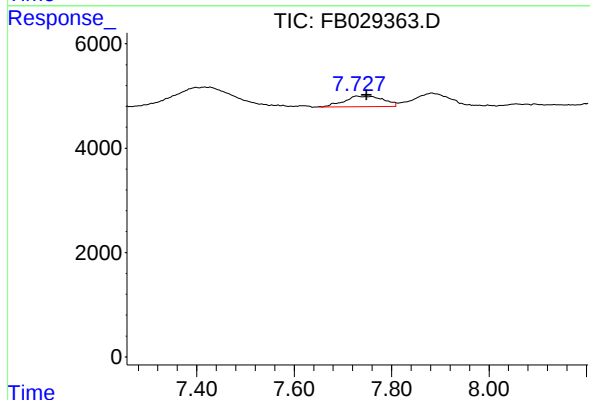


#3 n-Heptane

R.T.: 7.727 min
Delta R.T.: -0.022 min
Response: 11441
Conc: 0.63 ng/ml m

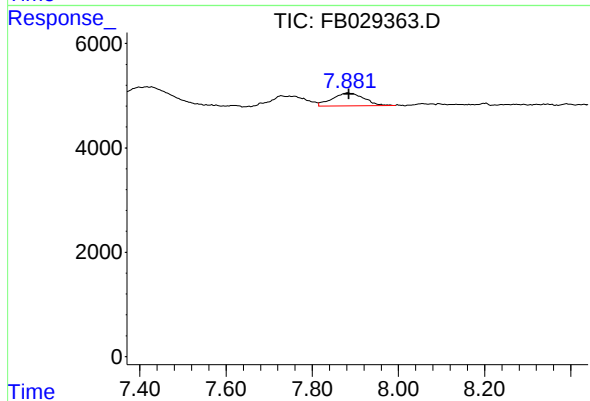


#4 Benzene

R.T.: 7.883 min
Delta R.T.: -0.002 min
Response: 12920
Conc: 0.62 ng/ml

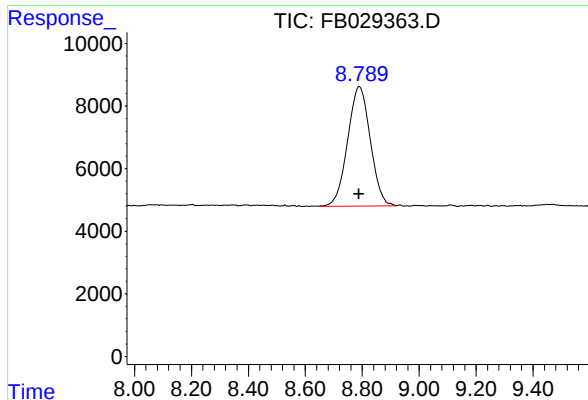


#5 AAA-TFT

R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 211103
Conc: 21.95 ng/ml

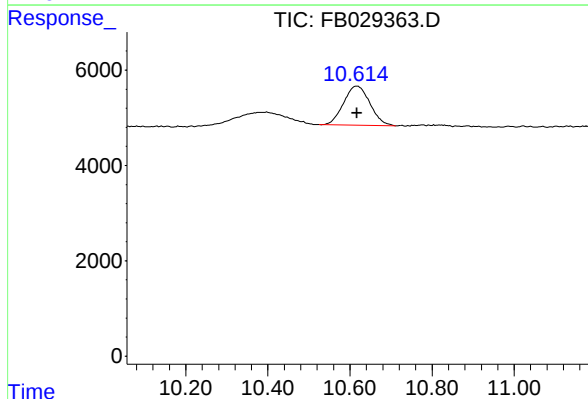


#6 Toluene

R.T.: 10.616 min
Delta R.T.: 0.000 min
Response: 36462
Conc: 1.80 ng/ml

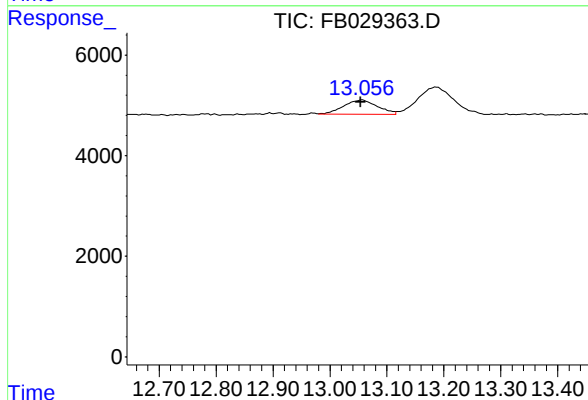


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.003 min
Response: 11576
Conc: 0.61 ng/ml

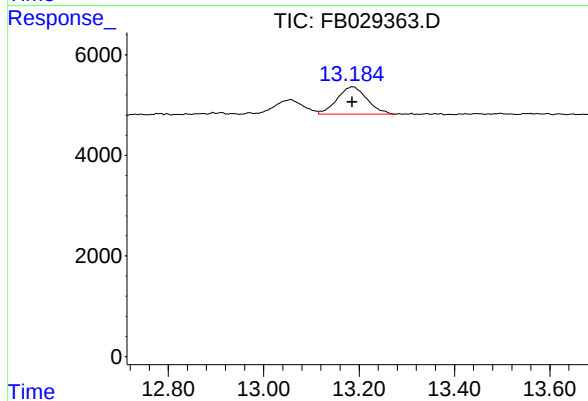


#8 m-Xylene

R.T.: 13.186 min
Delta R.T.: 0.000 min
Response: 23594
Conc: 1.24 ng/ml

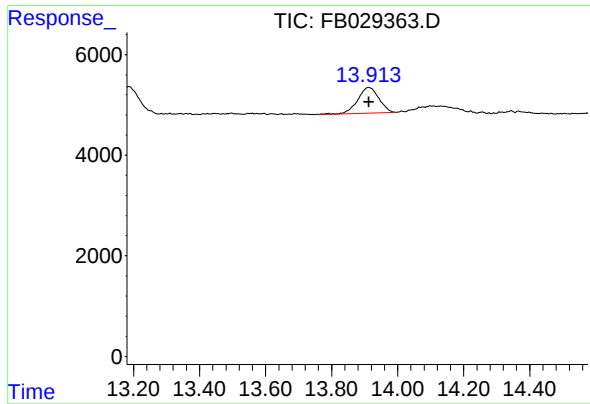

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: 0.001 min
Response: 22710
Conc: 1.24 ng/ml

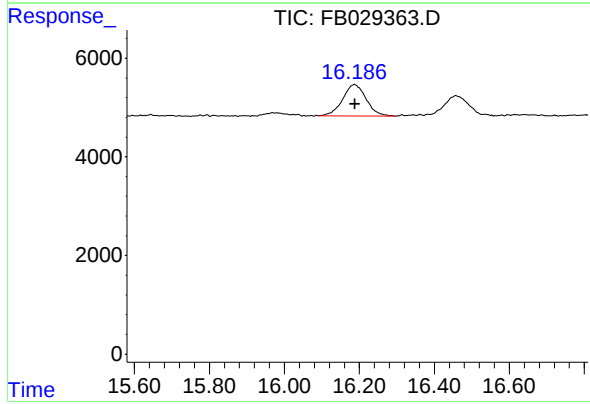

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: 0.000 min
Response: 28000
Conc: 1.49 ng/ml