

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022223\
 Data File : FB029367.D
 Signal(s) : FID2B.CH
 Acq On : 22 Feb 2023 14:09
 Operator : YP/AJ
 Sample : BSF0222W2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 23 00:25:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	204540	21.266 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	428179	26.986 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	521606	30.285 ng/ml
3) t n-Heptane	7.750	159313	8.805 ng/ml
4) t Benzene	7.886	195163	9.370 ng/ml
6) t Toluene	10.618	569699	28.113 ng/ml
7) t Ethylbenzene	13.056	180817	9.474 ng/ml
8) t m-Xylene	13.188	362870	19.141 ng/ml
9) t O-Xylene	13.914	356511	19.539 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	366354	19.467 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022223\
Data File : FB029367.D
Signal(s) : FID2B.CH
Acq On : 22 Feb 2023 14:09
Operator : YP/AJ
Sample : BSF0222W2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 23 00:25:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

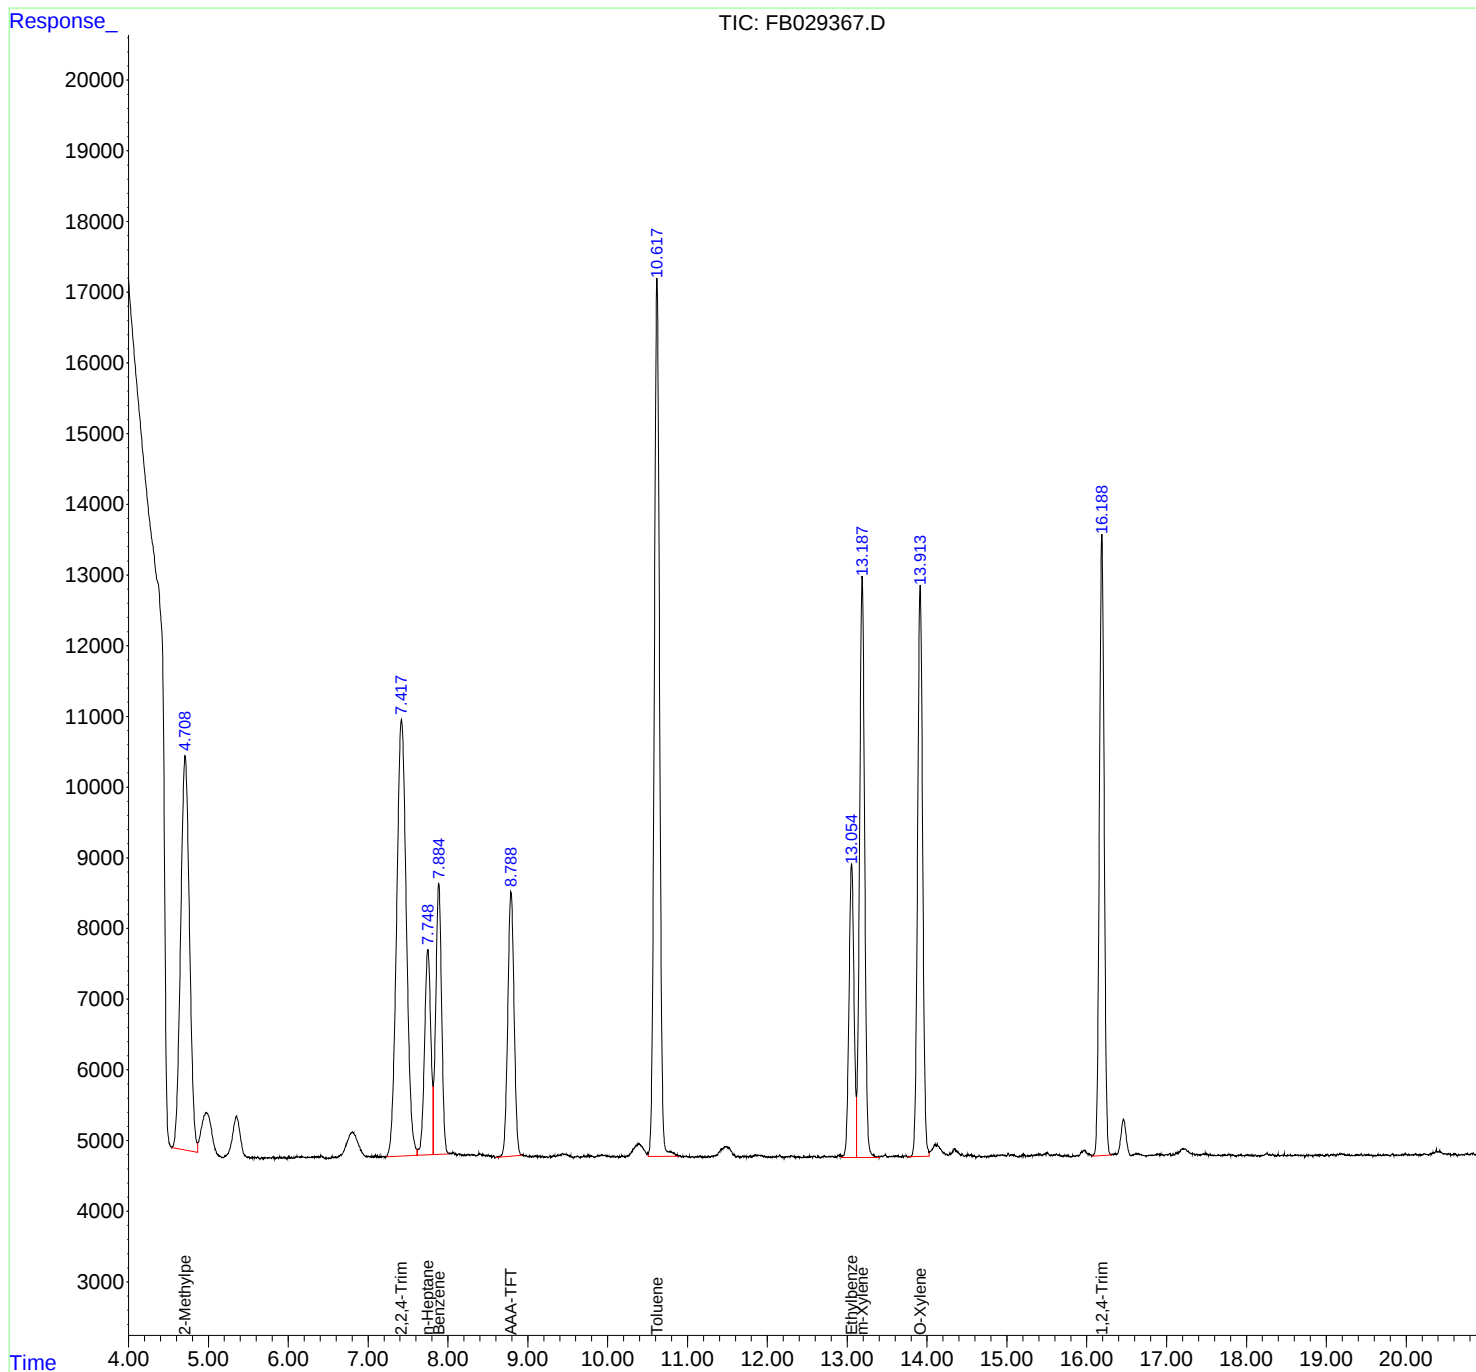

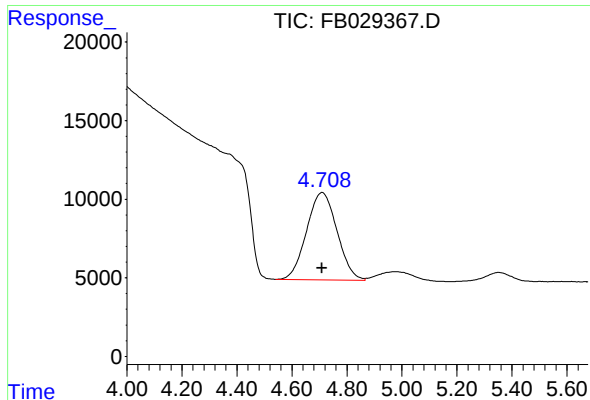


#1 2-Methylpentane

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 428179
Conc: 26.99 ng/ml

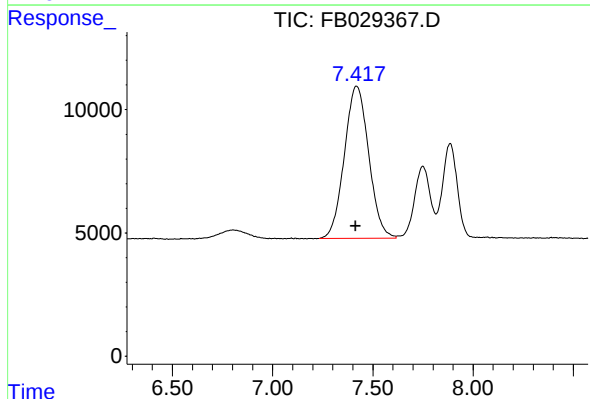


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.004 min
Response: 521606
Conc: 30.28 ng/ml

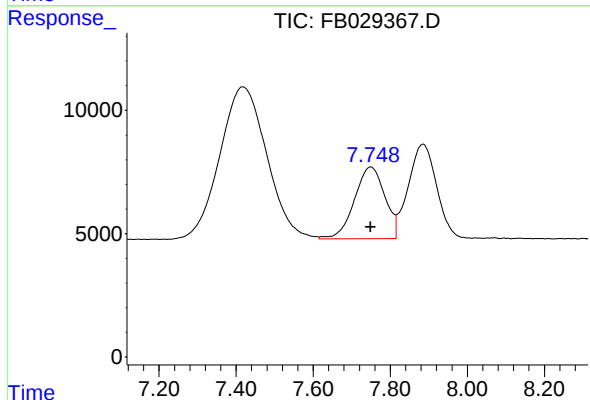


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.000 min
Response: 159313
Conc: 8.80 ng/ml

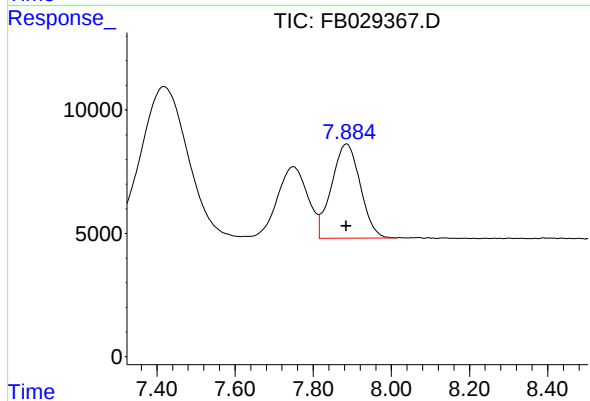


#4 Benzene

R.T.: 7.886 min
Delta R.T.: 0.001 min
Response: 195163
Conc: 9.37 ng/ml

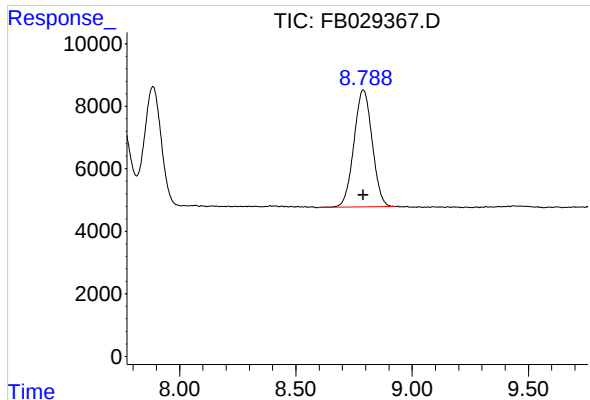


#5 AAA-TFT

R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 204540
Conc: 21.27 ng/ml

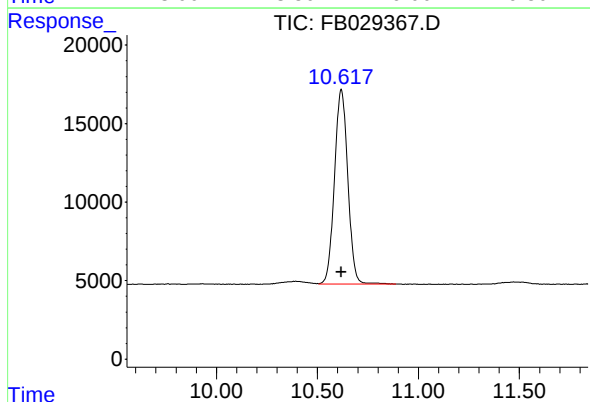


#6 Toluene

R.T.: 10.618 min
Delta R.T.: 0.001 min
Response: 569699
Conc: 28.11 ng/ml

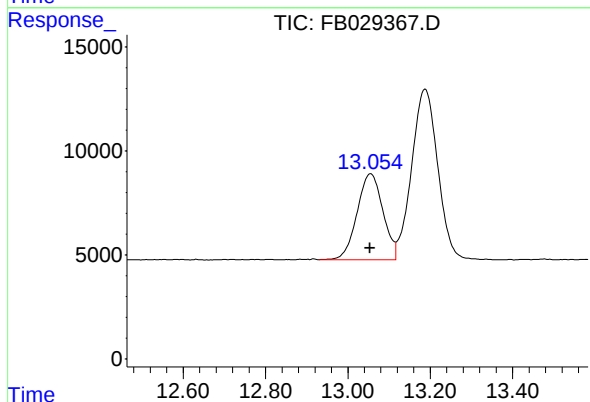


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.002 min
Response: 180817
Conc: 9.47 ng/ml

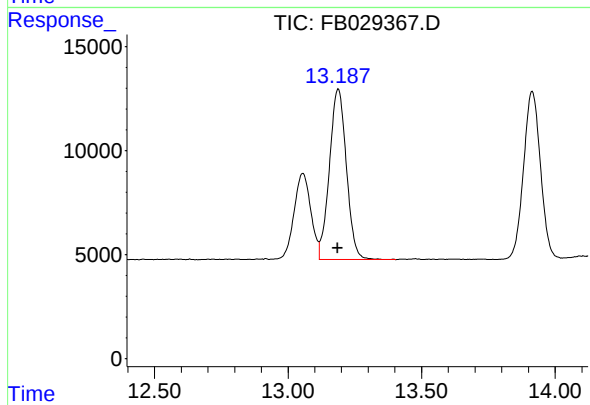


#8 m-Xylene

R.T.: 13.188 min
Delta R.T.: 0.002 min
Response: 362870
Conc: 19.14 ng/ml

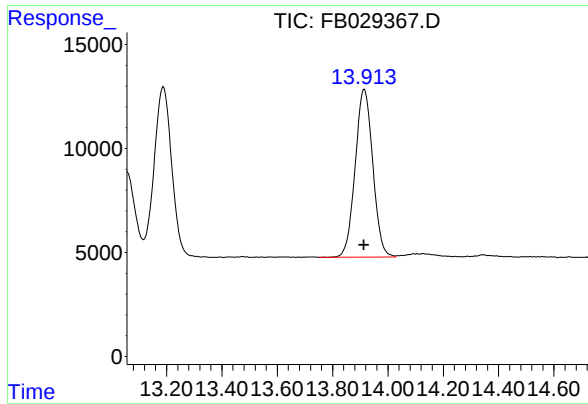

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: 0.002 min
Response: 356511
Conc: 19.54 ng/ml

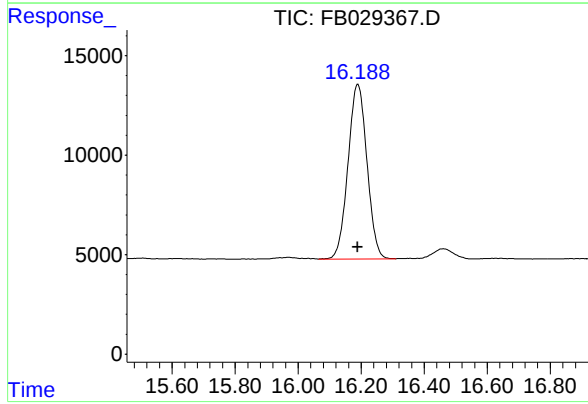

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: 0.002 min
Response: 366354
Conc: 19.47 ng/ml