

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022223\
 Data File : FB029368.D
 Signal(s) : FID2B.CH
 Acq On : 22 Feb 2023 14:46
 Operator : YP/AJ
 Sample : 01627-07
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Feb 23 00:25:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
 Quant Title :
 QLast Update : Mon Feb 06 14:33:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.793	197799	20.565 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.714	26835	1.691 ng/mlm
2) t	2,2,4-Trimethylpentane	7.417	25682	1.491 ng/mlm
3) t	n-Heptane	7.747	9846	0.544 ng/ml
4) t	Benzene	7.885	12336	0.592 ng/ml
6) t	Toluene	10.620	35941	1.774 ng/ml
7) t	Ethylbenzene	13.057	10945	0.573 ng/ml
8) t	m-Xylene	13.191	22732	1.199 ng/ml
9) t	O-Xylene	13.918	20264	1.111 ng/ml
10) t	1,2,4-Trimethylbenzene	16.193	24988	1.328 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB022223\
Data File : FB029368.D
Signal(s) : FID2B.CH
Acq On : 22 Feb 2023 14:46
Operator : YP/AJ
Sample : 01627-07
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Feb 23 00:25:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB020623.M
Quant Title :
QLast Update : Mon Feb 06 14:33:16 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

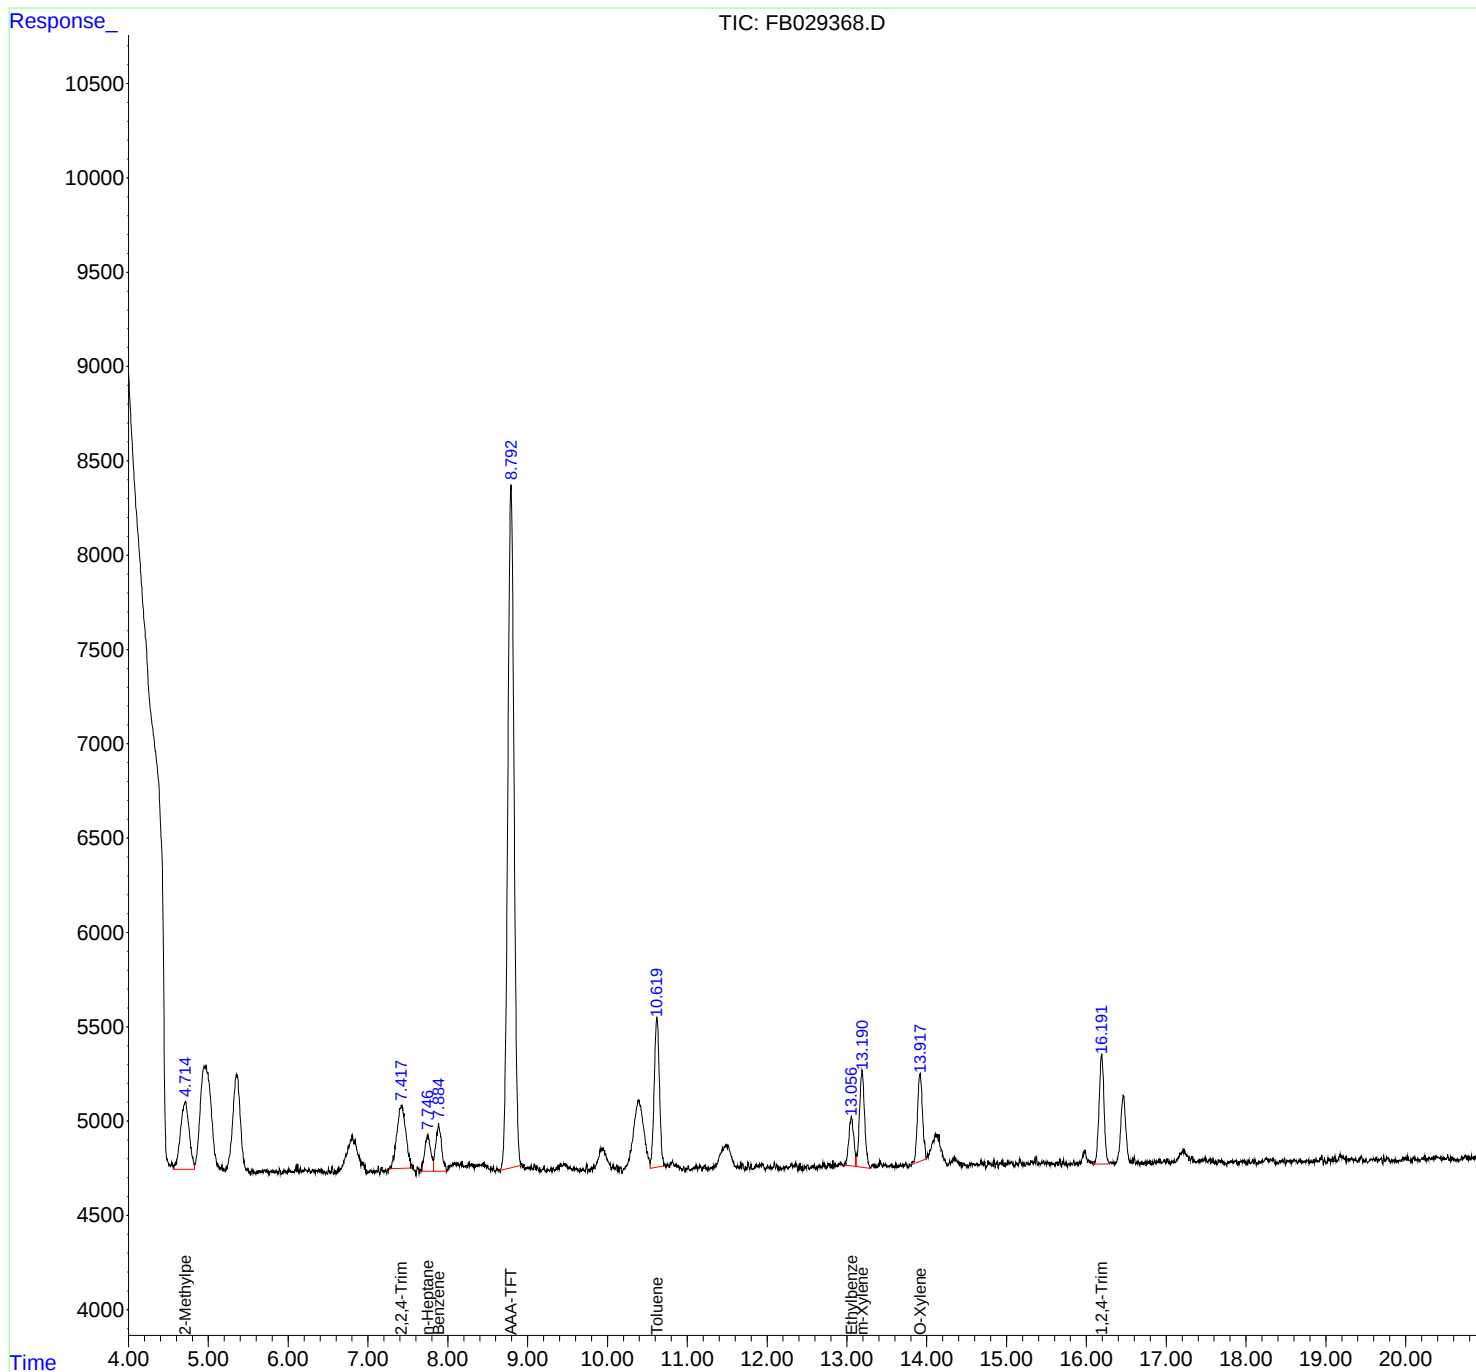

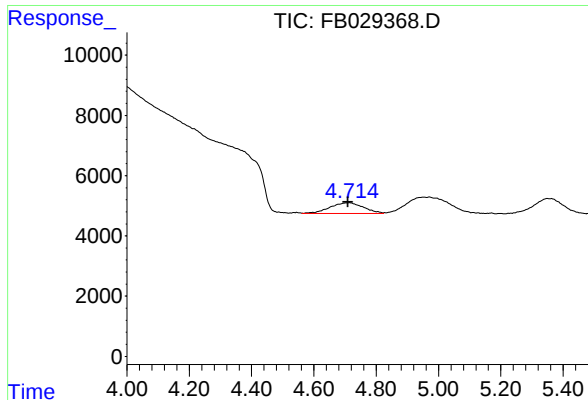


#1 2-Methylpentane

R.T.: 4.714 min
Delta R.T.: 0.005 min
Response: 26835
Conc: 1.69 ng/ml m

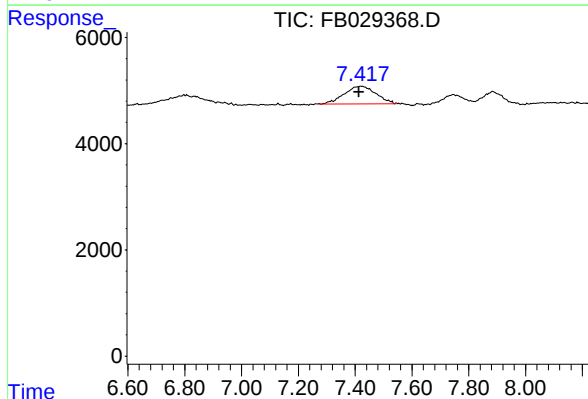


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.003 min
Response: 25682
Conc: 1.49 ng/ml m

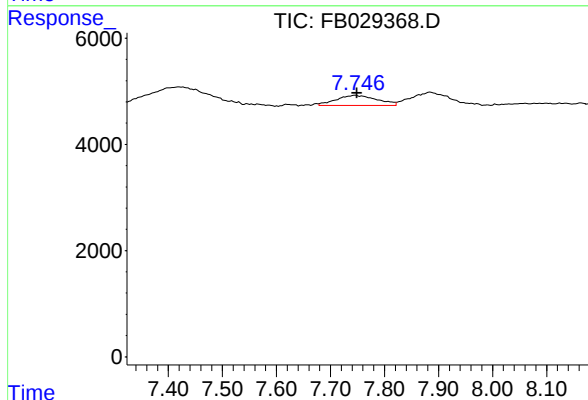


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.002 min
Response: 9846
Conc: 0.54 ng/ml

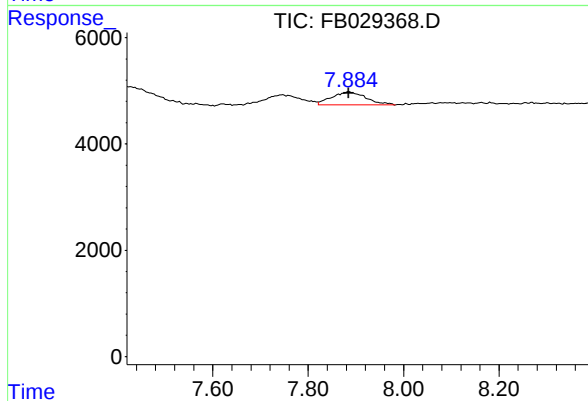


#4 Benzene

R.T.: 7.885 min
Delta R.T.: 0.000 min
Response: 12336
Conc: 0.59 ng/ml

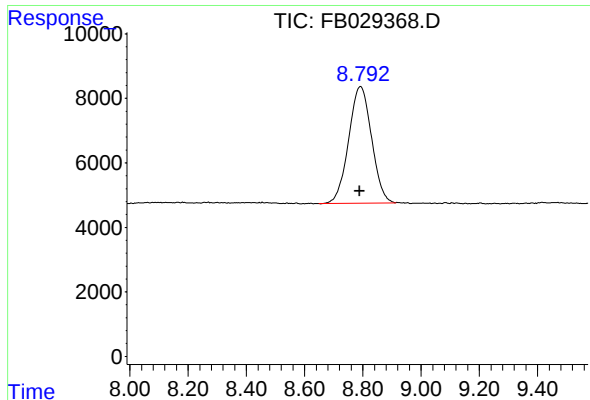


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: 0.004 min
Response: 197799
Conc: 20.56 ng/ml

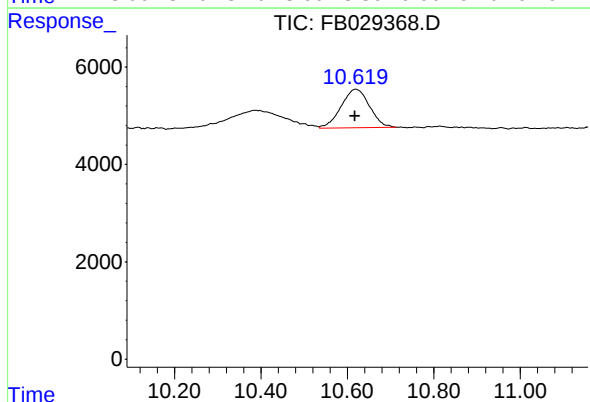


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.003 min
Response: 35941
Conc: 1.77 ng/ml

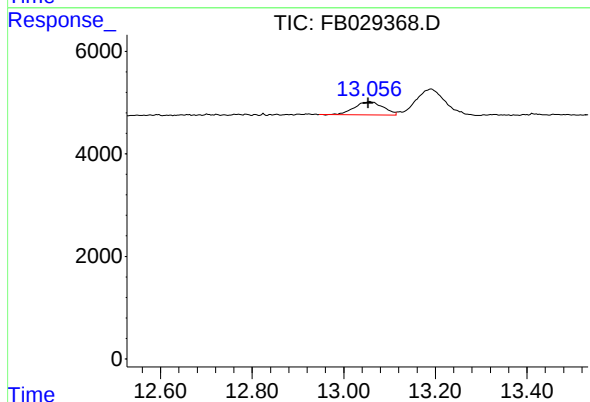


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.003 min
Response: 10945
Conc: 0.57 ng/ml

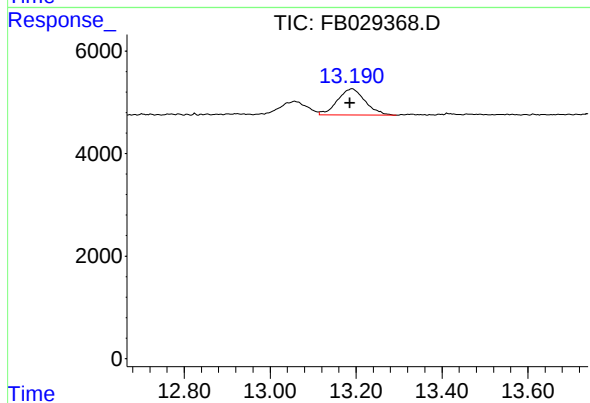


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: 0.005 min
Response: 22732
Conc: 1.20 ng/ml

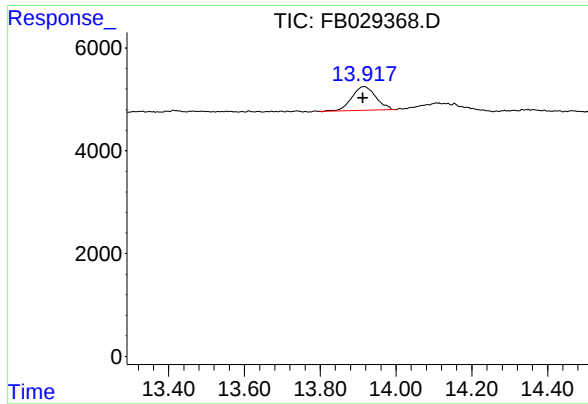

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.006 min
Response: 20264
Conc: 1.11 ng/ml

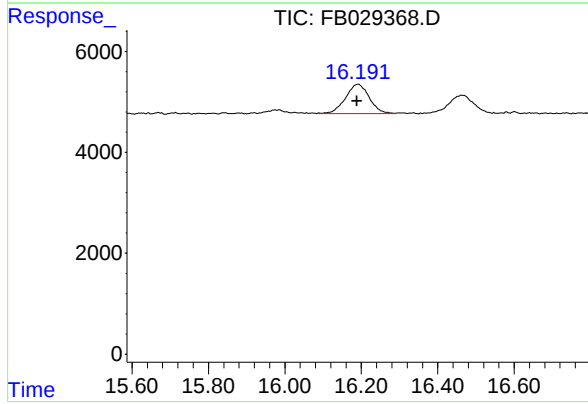

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.005 min
Response: 24988
Conc: 1.33 ng/ml